

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035390.D
 Acq On : 24 Apr 2024 16:21
 Operator : SY/MD
 Sample : P2203-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	232129	245910	14.73%	2.072%
2	1.532	146	153	169	rVB	207808	242467	14.52%	2.043%
3	2.059	307	317	331	rBV	379810	551259	33.02%	4.644%
4	2.449	432	438	450	rVB4	3449	5725	0.34%	0.048%
5	2.551	469	470	471	rBV4	260	91	0.01%	0.001%
6	2.654	499	502	504	rVB2	506	258	0.02%	0.002%
7	2.712	511	520	527	rVB5	1313	2278	0.14%	0.019%
8	2.741	527	529	531	rVB2	413	160	0.01%	0.001%
9	2.760	531	535	538	rBV2	202	203	0.01%	0.002%
10	2.818	551	553	556	rBV2	302	134	0.01%	0.001%
11	2.895	574	577	578	rBV	318	148	0.01%	0.001%
12	2.934	585	589	592	rBV	366	301	0.02%	0.003%
13	3.076	632	633	638	rVB	257	145	0.01%	0.001%
14	3.108	638	643	646	rBV2	461	438	0.03%	0.004%
15	3.220	676	678	680	rVB	182	59	0.00%	0.000%
16	3.249	680	687	690	rBV2	205	247	0.01%	0.002%
17	3.342	714	716	722	rVB3	217	177	0.01%	0.001%
18	3.378	722	727	730	rBV	204	178	0.01%	0.001%
19	3.420	738	740	742	rBV2	193	69	0.00%	0.001%
20	3.432	742	744	748	rVB2	236	130	0.01%	0.001%
21	3.535	773	776	777	rBV2	248	132	0.01%	0.001%
22	3.612	796	800	804	rBV2	177	185	0.01%	0.002%
23	3.648	808	811	814	rVB2	107	77	0.00%	0.001%
24	3.677	814	820	825	rVB3	271	324	0.02%	0.003%
25	3.706	825	829	831	rBV	183	124	0.01%	0.001%
26	3.796	848	857	894	rBV	105794	334664	20.05%	2.819%
27	4.246	983	997	1030	rBV	264111	687946	41.21%	5.795%
28	4.638	1117	1119	1121	rBV	324	131	0.01%	0.001%
29	4.953	1202	1217	1263	rBV2	623827	1669455	100.00%	14.063%
30	5.368	1344	1346	1350	rVB2	398	219	0.01%	0.002%
31	5.394	1350	1354	1359	rBV2	568	577	0.03%	0.005%
32	5.535	1387	1398	1425	rBV	359154	762833	45.69%	6.426%
33	5.989	1526	1539	1571	rBV	362382	763311	45.72%	6.430%
34	6.320	1640	1642	1648	rVB2	337	286	0.02%	0.002%
35	6.358	1651	1654	1655	rBV2	319	197	0.01%	0.002%
36	6.413	1669	1671	1673	rBV	229	85	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035390.D
 Acq On : 24 Apr 2024 16:21
 Operator : SY/MD
 Sample : P2203-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.436	1673	1678	1682	rBV4	518	535	0.03%	0.005%
38	6.471	1688	1689	1690	rBV4	169	49	0.00%	0.000%
39	6.522	1703	1705	1707	rVB	132	55	0.00%	0.000%
40	6.551	1711	1714	1715	rBV2	360	185	0.01%	0.002%
41	6.590	1725	1726	1730	rVB2	337	115	0.01%	0.001%
42	6.612	1730	1733	1734	rBV2	202	121	0.01%	0.001%
43	6.619	1734	1735	1738	rBV2	291	144	0.01%	0.001%
44	6.693	1757	1758	1759	rBV	88	30	0.00%	0.000%
45	6.757	1772	1778	1782	rBV3	525	602	0.04%	0.005%
46	6.812	1792	1795	1797	rBV	138	96	0.01%	0.001%
47	6.844	1803	1805	1807	rVB	158	61	0.00%	0.001%
48	6.911	1816	1826	1855	rBV	171608	338410	20.27%	2.851%
49	7.243	1917	1929	1954	rBV	702023	1242455	74.42%	10.466%
50	7.554	2017	2026	2057	rBV	121428	234032	14.02%	1.971%
51	7.860	2117	2121	2122	rBV2	677	485	0.03%	0.004%
52	7.915	2133	2138	2144	rVB4	884	897	0.05%	0.008%
53	7.969	2151	2155	2159	rBV3	468	415	0.02%	0.003%
54	7.995	2161	2163	2164	rBV3	259	77	0.00%	0.001%
55	8.027	2164	2173	2234	rBV3	300294	761871	45.64%	6.418%
56	8.628	2355	2360	2366	rVB3	434	436	0.03%	0.004%
57	8.783	2397	2408	2440	rBV	587919	984378	58.96%	8.292%
58	9.095	2498	2505	2510	rBV6	1165	1745	0.10%	0.015%
59	9.143	2518	2520	2523	rVB2	419	172	0.01%	0.001%
60	9.188	2530	2534	2536	rBV2	504	350	0.02%	0.003%
61	9.214	2540	2542	2543	rBV	116	31	0.00%	0.000%
62	9.246	2550	2552	2555	rBV2	200	130	0.01%	0.001%
63	9.268	2556	2559	2561	rVV2	318	164	0.01%	0.001%
64	9.310	2570	2572	2574	rBV2	324	134	0.01%	0.001%
65	9.342	2580	2582	2584	rBV	219	92	0.01%	0.001%
66	9.378	2591	2593	2596	rBV	168	128	0.01%	0.001%
67	9.406	2600	2602	2605	rVV	274	147	0.01%	0.001%
68	9.423	2605	2607	2612	rVB2	317	176	0.01%	0.001%
69	9.445	2612	2614	2616	rBV2	174	51	0.00%	0.000%
70	9.461	2617	2619	2622	rVB	321	155	0.01%	0.001%
71	9.490	2623	2628	2636	rVB5	1009	1409	0.08%	0.012%
72	9.596	2659	2661	2663	rBV	219	131	0.01%	0.001%
73	9.670	2682	2684	2687	rVB3	229	137	0.01%	0.001%
74	9.689	2688	2690	2693	rBV	178	105	0.01%	0.001%
75	9.750	2707	2709	2711	rBV	231	86	0.01%	0.001%
76	9.873	2742	2747	2754	rBV3	763	1045	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035390.D
 Acq On : 24 Apr 2024 16:21
 Operator : SY/MD
 Sample : P2203-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.053	2799	2803	2806	rBV2	418	268	0.02%	0.002%
78	10.104	2817	2819	2821	rBV	195	92	0.01%	0.001%
79	10.149	2822	2833	2867	rVV	555791	874767	52.40%	7.369%
80	10.394	2906	2909	2912	rVB3	332	254	0.02%	0.002%
81	10.413	2912	2915	2919	rBV3	289	224	0.01%	0.002%
82	10.586	2966	2969	2972	rBV	331	267	0.02%	0.002%
83	10.622	2977	2980	2982	rBV	279	162	0.01%	0.001%
84	10.931	3075	3076	3077	rBV	153	52	0.00%	0.000%
85	10.963	3083	3086	3090	rBV2	254	148	0.01%	0.001%
86	11.014	3100	3102	3104	rBV2	169	100	0.01%	0.001%
87	11.136	3133	3140	3144	rBV5	1123	1610	0.10%	0.014%
88	11.185	3144	3155	3180	rVV	571176	901977	54.03%	7.598%
89	11.461	3238	3241	3243	rBV	528	327	0.02%	0.003%
90	11.496	3244	3252	3260	rVV2	12912	25209	1.51%	0.212%
91	11.557	3261	3271	3293	rVB	776606	1213040	72.66%	10.219%
92	11.882	3370	3372	3376	rBV2	756	489	0.03%	0.004%
93	12.146	3452	3454	3458	rVB	375	200	0.01%	0.002%
94	12.381	3525	3527	3529	rBV	377	225	0.01%	0.002%
95	12.438	3542	3545	3548	rBV2	599	404	0.02%	0.003%
96	12.667	3611	3616	3618	rBV2	835	734	0.04%	0.006%
97	12.789	3651	3654	3656	rBV2	563	241	0.01%	0.002%
98	12.985	3711	3715	3724	rVB5	2037	2570	0.15%	0.022%
99	13.213	3779	3786	3792	rVB3	2870	4116	0.25%	0.035%
100	13.297	3809	3812	3815	rBV2	854	616	0.04%	0.005%




Sum of corrected areas: 11870852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035390.D
Acq On : 24 Apr 2024 16:21
Operator : SY/MD
Sample : P2203-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

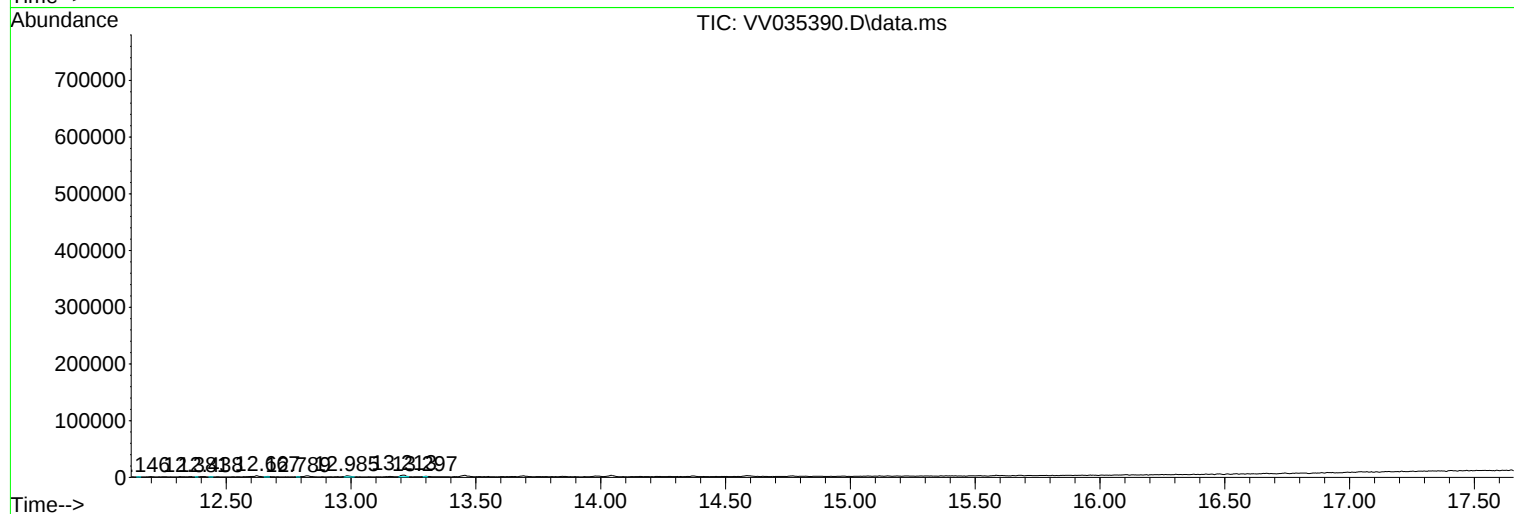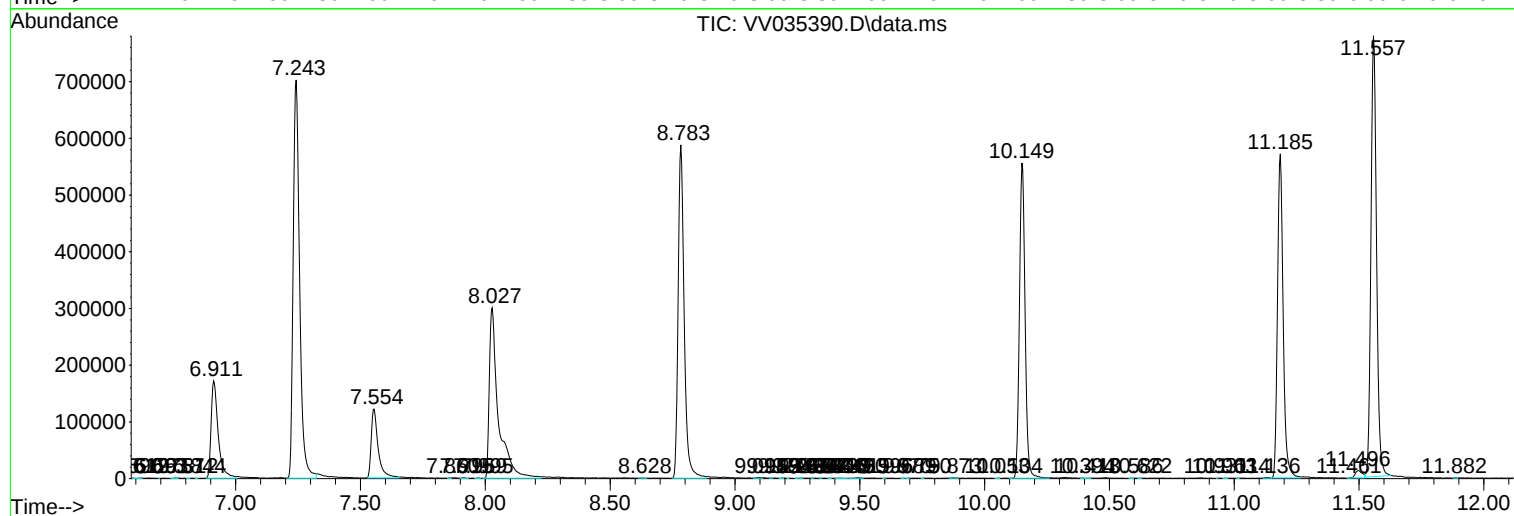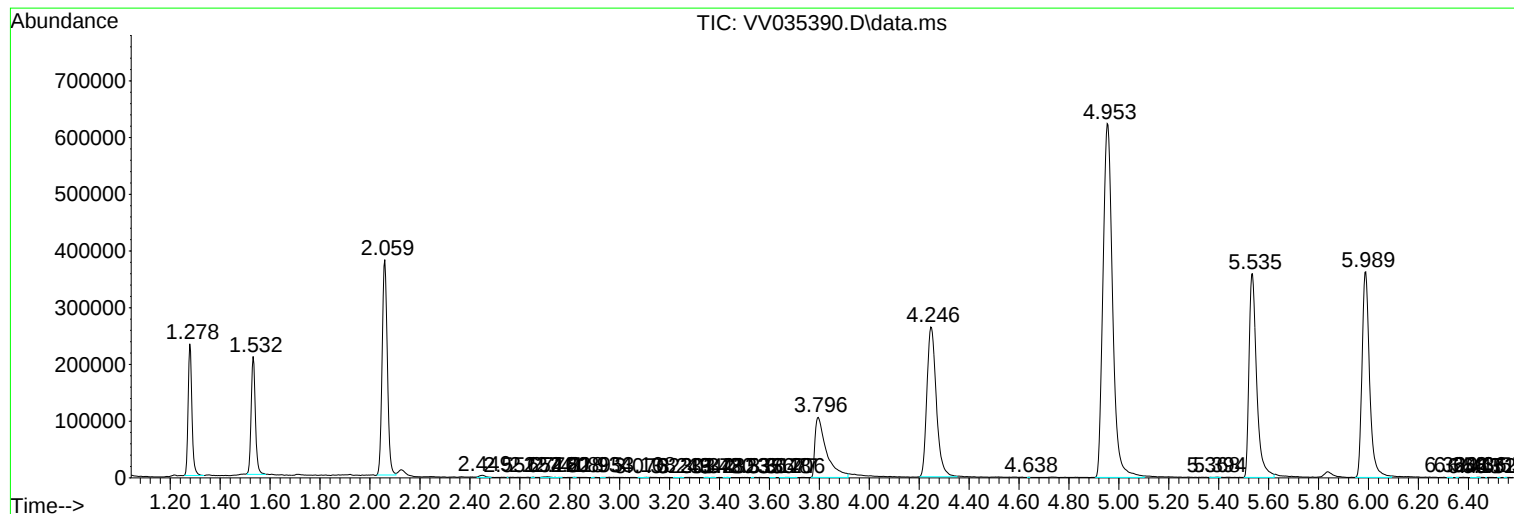

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035390.D
Acq On : 24 Apr 2024 16:21
Operator : SY/MD
Sample : P2203-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035390.D
Acq On : 24 Apr 2024 16:21
Operator : SY/MD
Sample : P2203-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc