

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035391.D
 Acq On : 24 Apr 2024 16:43
 Operator : SY/MD
 Sample : P2203-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	193789	205740	14.57%	2.007%
2	1.532	146	153	177	rVB	178367	211194	14.96%	2.061%
3	2.060	308	317	330	rBV	317700	454048	32.16%	4.430%
4	2.523	458	461	463	rBV	288	179	0.01%	0.002%
5	2.590	480	482	483	rBV	295	138	0.01%	0.001%
6	2.799	543	547	551	rBV2	348	246	0.02%	0.002%
7	2.847	558	562	564	rBV	280	184	0.01%	0.002%
8	2.966	597	599	601	rVV	254	102	0.01%	0.001%
9	2.986	603	605	609	rVV	185	103	0.01%	0.001%
10	3.037	618	621	625	rBV2	344	277	0.02%	0.003%
11	3.105	639	642	645	rBV2	291	194	0.01%	0.002%
12	3.153	655	657	662	rVB2	177	101	0.01%	0.001%
13	3.233	676	682	685	rBV2	308	275	0.02%	0.003%
14	3.320	706	709	712	rVV3	252	201	0.01%	0.002%
15	3.333	712	713	715	rVV3	341	108	0.01%	0.001%
16	3.359	717	721	724	rVB2	250	210	0.01%	0.002%
17	3.375	724	726	728	rBV	204	119	0.01%	0.001%
18	3.410	733	737	738	rBV2	204	137	0.01%	0.001%
19	3.455	748	751	754	rBV2	292	205	0.01%	0.002%
20	3.558	778	783	786	rBV2	198	173	0.01%	0.002%
21	3.642	807	809	811	rVB	235	103	0.01%	0.001%
22	3.664	811	816	819	rBV2	147	124	0.01%	0.001%
23	3.687	821	823	826	rVB	200	101	0.01%	0.001%
24	3.796	849	857	889	rBV	90191	276541	19.59%	2.698%
25	4.249	983	998	1035	rBV	224867	588674	41.70%	5.744%
26	4.796	1165	1168	1169	rBV	270	183	0.01%	0.002%
27	4.957	1202	1218	1262	rBV2	524907	1411635	100.00%	13.774%
28	5.349	1338	1340	1344	rBV3	386	247	0.02%	0.002%
29	5.535	1387	1398	1434	rBV	332017	712958	50.51%	6.957%
30	5.838	1480	1492	1512	rBV4	7445	18777	1.33%	0.183%
31	5.989	1523	1539	1573	rBV	307125	653882	46.32%	6.380%
32	6.243	1615	1618	1620	rBV	544	368	0.03%	0.004%
33	6.304	1633	1637	1642	rVB3	475	486	0.03%	0.005%
34	6.330	1642	1645	1646	rBV	365	149	0.01%	0.001%
35	6.368	1655	1657	1663	rBV3	464	382	0.03%	0.004%
36	6.397	1663	1666	1669	rBV2	324	209	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035391.D
 Acq On : 24 Apr 2024 16:43
 Operator : SY/MD
 Sample : P2203-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.420	1669	1673	1677	rBV2	247	195	0.01%	0.002%
38	6.558	1713	1716	1718	rBV	230	129	0.01%	0.001%
39	6.590	1723	1726	1731	rVV3	324	283	0.02%	0.003%
40	6.642	1740	1742	1744	rBV	315	159	0.01%	0.002%
41	6.690	1753	1757	1759	rBV2	242	163	0.01%	0.002%
42	6.741	1769	1773	1775	rBV	267	126	0.01%	0.001%
43	6.770	1780	1782	1786	rVB	312	148	0.01%	0.001%
44	6.838	1799	1803	1805	rBV2	199	123	0.01%	0.001%
45	6.915	1815	1827	1857	rBV	145215	286569	20.30%	2.796%
46	7.191	1909	1913	1916	rBV3	461	343	0.02%	0.003%
47	7.243	1918	1929	1958	rBV	579937	1037752	73.51%	10.126%
48	7.555	2017	2026	2051	rBV	102413	191970	13.60%	1.873%
49	7.760	2088	2090	2091	rBV2	418	152	0.01%	0.001%
50	7.992	2160	2162	2164	rBV	192	117	0.01%	0.001%
51	8.027	2164	2173	2211	rBV2	252671	617330	43.73%	6.024%
52	8.616	2354	2356	2359	rVB	400	159	0.01%	0.002%
53	8.632	2359	2361	2363	rBV2	197	96	0.01%	0.001%
54	8.696	2378	2381	2384	rBV2	288	264	0.02%	0.003%
55	8.738	2392	2394	2397	rBV	266	122	0.01%	0.001%
56	8.783	2397	2408	2437	rBV	533793	907021	64.25%	8.850%
57	9.011	2477	2479	2483	rBV3	511	334	0.02%	0.003%
58	9.104	2505	2508	2514	rVB3	823	747	0.05%	0.007%
59	9.249	2547	2553	2558	rVB3	561	645	0.05%	0.006%
60	9.285	2562	2564	2566	rBV	203	115	0.01%	0.001%
61	9.346	2581	2583	2586	rVB	294	160	0.01%	0.002%
62	9.378	2590	2593	2596	rBV2	363	226	0.02%	0.002%
63	9.426	2605	2608	2609	rBV2	195	100	0.01%	0.001%
64	9.439	2609	2612	2614	rBV	202	124	0.01%	0.001%
65	9.625	2665	2670	2673	rBV2	318	301	0.02%	0.003%
66	9.664	2680	2682	2685	rBV	261	115	0.01%	0.001%
67	9.728	2700	2702	2704	rVB	312	107	0.01%	0.001%
68	9.741	2704	2706	2709	rBV2	219	108	0.01%	0.001%
69	9.789	2717	2721	2726	rBV2	203	273	0.02%	0.003%
70	9.886	2748	2751	2753	rBV	371	263	0.02%	0.003%
71	9.992	2781	2784	2786	rBV	262	152	0.01%	0.001%
72	10.149	2821	2833	2856	rBV	467476	748041	52.99%	7.299%
73	10.429	2917	2920	2924	rVB	310	192	0.01%	0.002%
74	10.455	2925	2928	2930	rBV	384	250	0.02%	0.002%
75	10.603	2971	2974	2976	rBV	197	114	0.01%	0.001%
76	10.744	3012	3018	3020	rBV3	495	444	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035391.D
 Acq On : 24 Apr 2024 16:43
 Operator : SY/MD
 Sample : P2203-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.786	3027	3031	3032	rBV	294	180	0.01%	0.002%
78	10.837	3044	3047	3050	rBV2	457	283	0.02%	0.003%
79	10.895	3062	3065	3068	rBV2	252	174	0.01%	0.002%
80	10.924	3071	3074	3079	rBV2	231	240	0.02%	0.002%
81	11.069	3117	3119	3124	rVB2	236	131	0.01%	0.001%
82	11.130	3135	3138	3144	rBV4	834	937	0.07%	0.009%
83	11.185	3144	3155	3185	rBV	520623	838250	59.38%	8.179%
84	11.493	3244	3251	3260	rBV4	11482	23807	1.69%	0.232%
85	11.558	3261	3271	3299	rVB	658592	1039822	73.66%	10.146%
86	11.866	3365	3367	3372	rBV4	344	268	0.02%	0.003%
87	11.892	3372	3375	3379	rVB2	512	316	0.02%	0.003%
88	11.924	3383	3385	3387	rVB	365	127	0.01%	0.001%
89	11.940	3387	3390	3392	rBV4	712	538	0.04%	0.005%
90	12.098	3438	3439	3441	rBV2	275	108	0.01%	0.001%
91	12.198	3467	3470	3474	rVB4	804	545	0.04%	0.005%
92	12.291	3497	3499	3502	rBV2	289	135	0.01%	0.001%
93	12.381	3524	3527	3528	rBV	388	185	0.01%	0.002%
94	12.484	3557	3559	3564	rVB2	293	170	0.01%	0.002%
95	12.587	3587	3591	3592	rBV3	410	272	0.02%	0.003%
96	12.763	3643	3646	3647	rBV	351	194	0.01%	0.002%
97	12.825	3659	3665	3675	rVB5	1925	2140	0.15%	0.021%
98	13.037	3728	3731	3734	rBV	344	301	0.02%	0.003%
99	13.117	3753	3756	3761	rBV	554	463	0.03%	0.005%
100	13.210	3777	3785	3796	rVB6	2964	4303	0.30%	0.042%




Sum of corrected areas: 10248674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035391.D
Acq On : 24 Apr 2024 16:43
Operator : SY/MD
Sample : P2203-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

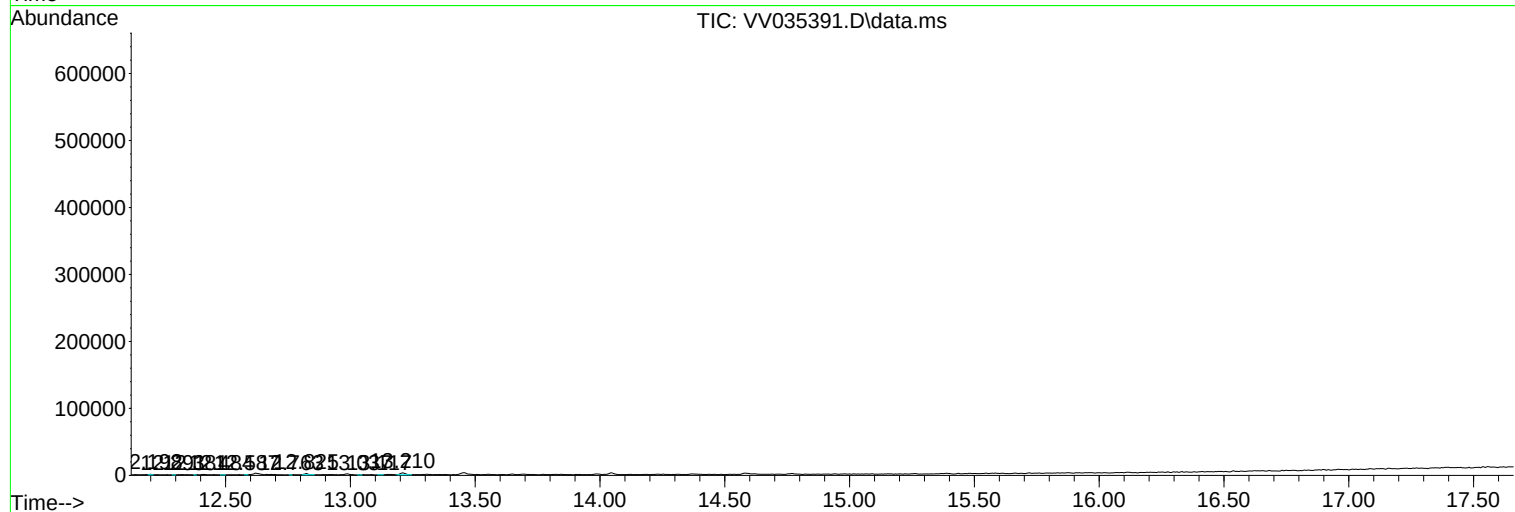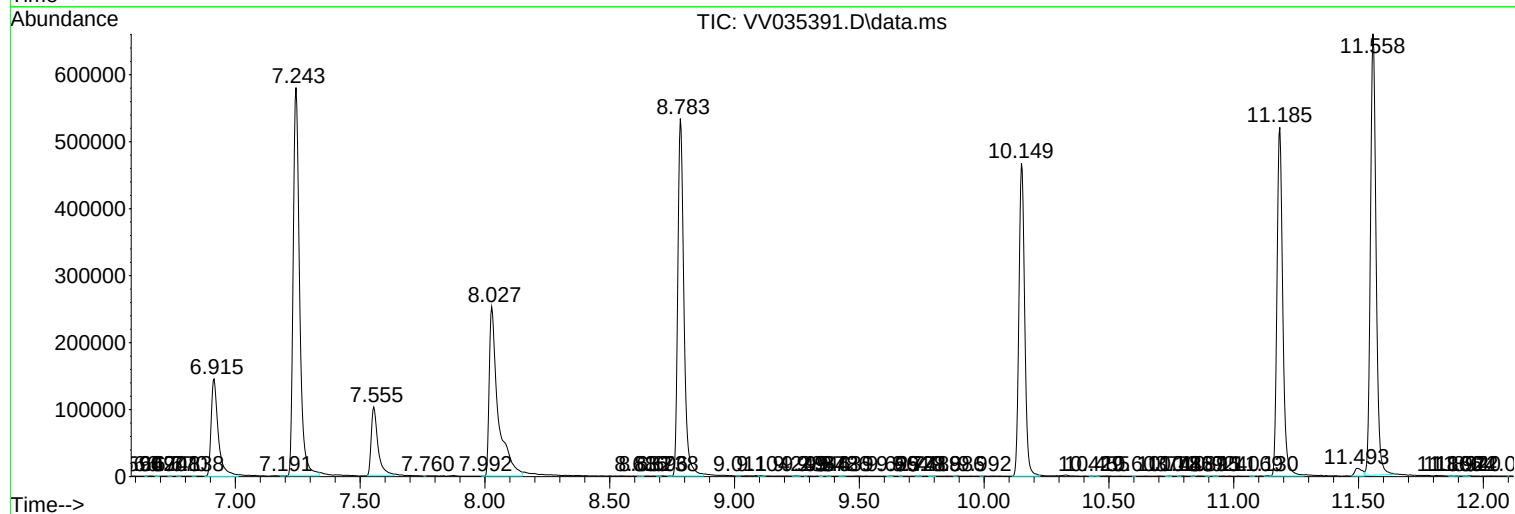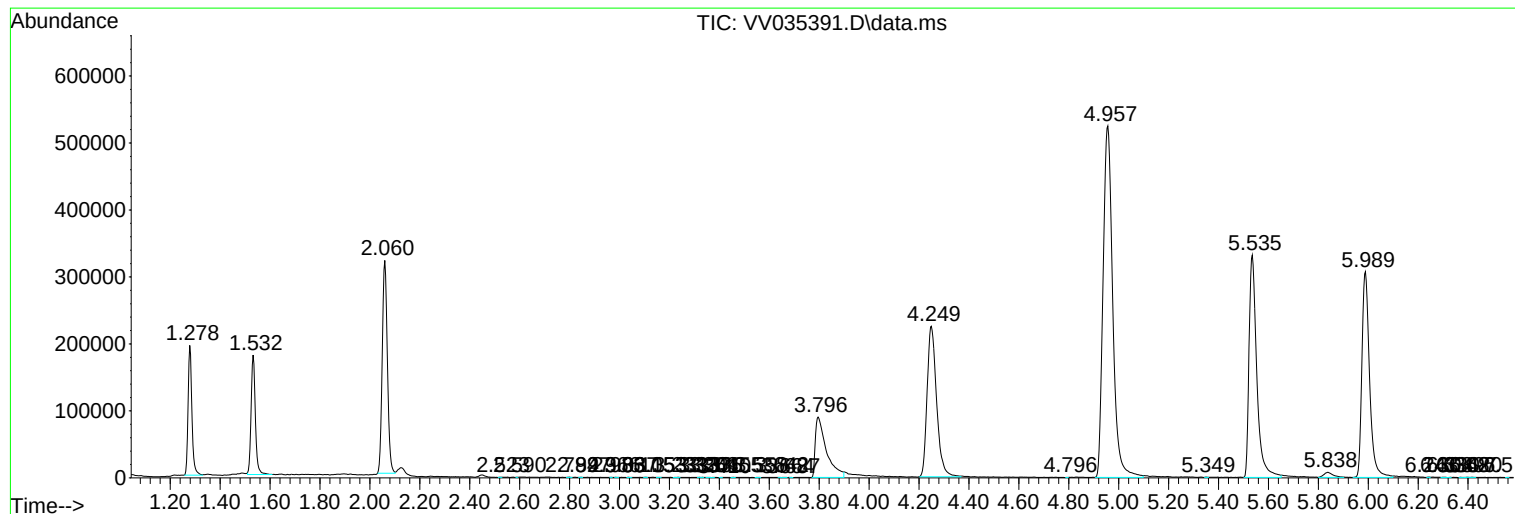

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035391.D
Acq On : 24 Apr 2024 16:43
Operator : SY/MD
Sample : P2203-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035391.D
Acq On : 24 Apr 2024 16:43
Operator : SY/MD
Sample : P2203-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------