

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035392.D
 Acq On : 24 Apr 2024 17:06
 Operator : SY/MD
 Sample : P2203-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	194095	204906	14.80%	2.079%
2	1.532	146	153	166	rVB	172726	199819	14.43%	2.028%
3	2.060	307	317	330	rBV	314331	455865	32.92%	4.626%
4	2.446	431	437	446	rVB4	3213	4918	0.36%	0.050%
5	2.529	458	463	466	rBV3	675	586	0.04%	0.006%
6	2.603	483	486	489	rBV3	389	292	0.02%	0.003%
7	2.690	510	513	515	rBV	261	157	0.01%	0.002%
8	2.854	562	564	566	rBV2	135	83	0.01%	0.001%
9	3.056	624	627	628	rBV2	155	84	0.01%	0.001%
10	3.092	633	638	643	rBV3	311	352	0.03%	0.004%
11	3.182	661	666	670	rBV2	190	194	0.01%	0.002%
12	3.256	686	689	694	rBV	238	175	0.01%	0.002%
13	3.291	698	700	704	rBV2	208	122	0.01%	0.001%
14	3.323	708	710	714	rVB	337	228	0.02%	0.002%
15	3.349	714	718	721	rBV2	306	228	0.02%	0.002%
16	3.368	721	724	727	rBV2	225	131	0.01%	0.001%
17	3.413	735	738	741	rBV2	134	87	0.01%	0.001%
18	3.487	757	761	766	rVB	287	242	0.02%	0.002%
19	3.571	784	787	788	rBV	116	69	0.00%	0.001%
20	3.690	822	824	827	rBV	127	88	0.01%	0.001%
21	3.741	837	840	842	rBV	128	71	0.01%	0.001%
22	3.793	848	856	891	rBV	86459	266063	19.22%	2.700%
23	4.249	983	998	1033	rBV	219812	571842	41.30%	5.803%
24	4.626	1111	1115	1118	rBV2	286	241	0.02%	0.002%
25	4.699	1133	1138	1142	rVB3	339	306	0.02%	0.003%
26	4.722	1142	1145	1150	rBV2	314	323	0.02%	0.003%
27	4.847	1180	1184	1186	rBV	310	285	0.02%	0.003%
28	4.902	1198	1201	1202	rBV2	463	257	0.02%	0.003%
29	4.954	1202	1217	1265	rVV2	515454	1384624	100.00%	14.050%
30	5.397	1353	1355	1358	rBV	219	103	0.01%	0.001%
31	5.423	1360	1363	1366	rVB4	345	205	0.01%	0.002%
32	5.532	1387	1397	1435	rBV	304372	657152	47.46%	6.668%
33	5.834	1482	1491	1507	rBV4	6928	16158	1.17%	0.164%
34	5.986	1526	1538	1569	rBV	300375	633347	45.74%	6.427%
35	6.365	1654	1656	1658	rVB	345	140	0.01%	0.001%
36	6.384	1661	1662	1663	rBV	223	62	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035392.D
 Acq On : 24 Apr 2024 17:06
 Operator : SY/MD
 Sample : P2203-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.413	1669	1671	1672	rBV	257	104	0.01%	0.001%
38	6.490	1693	1695	1698	rVV2	191	104	0.01%	0.001%
39	6.648	1740	1744	1748	rVB	391	250	0.02%	0.003%
40	6.706	1760	1762	1765	rVB2	236	97	0.01%	0.001%
41	6.728	1765	1769	1770	rBV	322	213	0.02%	0.002%
42	6.789	1783	1788	1790	rBV2	375	330	0.02%	0.003%
43	6.834	1799	1802	1805	rBV	199	125	0.01%	0.001%
44	6.915	1816	1827	1862	rBV	138104	279908	20.22%	2.840%
45	7.156	1899	1902	1903	rBV2	453	245	0.02%	0.002%
46	7.198	1912	1915	1918	rBV3	435	347	0.03%	0.004%
47	7.243	1918	1929	1955	rBV	559059	1007786	72.78%	10.226%
48	7.555	2016	2026	2055	rBV	97621	191571	13.84%	1.944%
49	7.834	2109	2113	2116	rBV3	293	274	0.02%	0.003%
50	7.850	2116	2118	2119	rBV3	370	164	0.01%	0.002%
51	7.918	2137	2139	2145	rVB3	481	303	0.02%	0.003%
52	7.953	2149	2150	2153	rVB	254	139	0.01%	0.001%
53	7.969	2153	2155	2158	rVB2	250	90	0.01%	0.001%
54	7.989	2158	2161	2162	rBV2	143	90	0.01%	0.001%
55	8.027	2164	2173	2212	rBV2	239002	598906	43.25%	6.077%
56	8.529	2327	2329	2334	rBV3	356	215	0.02%	0.002%
57	8.555	2334	2337	2339	rBV3	544	360	0.03%	0.004%
58	8.651	2364	2367	2371	rBV2	376	340	0.02%	0.003%
59	8.748	2393	2397	2398	rBV	306	191	0.01%	0.002%
60	8.783	2398	2408	2453	rVV	494900	850729	61.44%	8.633%
61	9.085	2499	2502	2504	rBV2	476	299	0.02%	0.003%
62	9.130	2514	2516	2522	rVB4	593	447	0.03%	0.005%
63	9.175	2527	2530	2535	rVB3	454	367	0.03%	0.004%
64	9.201	2535	2538	2543	rBV2	359	385	0.03%	0.004%
65	9.268	2557	2559	2563	rVB	237	96	0.01%	0.001%
66	9.291	2564	2566	2571	rBV3	315	251	0.02%	0.003%
67	9.445	2612	2614	2616	rBV	301	167	0.01%	0.002%
68	9.481	2624	2625	2626	rBV	242	72	0.01%	0.001%
69	9.539	2641	2643	2646	rVB	142	62	0.00%	0.001%
70	9.558	2646	2649	2651	rBV2	195	137	0.01%	0.001%
71	9.834	2733	2735	2739	rVB2	312	167	0.01%	0.002%
72	9.879	2745	2749	2751	rBV2	227	196	0.01%	0.002%
73	9.940	2760	2768	2770	rBV2	293	262	0.02%	0.003%
74	9.992	2782	2784	2786	rVB	329	145	0.01%	0.001%
75	10.014	2789	2791	2797	rVB2	275	175	0.01%	0.002%
76	10.056	2801	2804	2807	rBV2	291	116	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035392.D
 Acq On : 24 Apr 2024 17:06
 Operator : SY/MD
 Sample : P2203-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2821	2833	2864	rBV	453646	723115	52.22%	7.338%
78	10.365	2898	2900	2905	rBV2	355	290	0.02%	0.003%
79	10.429	2917	2920	2925	rVB2	476	432	0.03%	0.004%
80	10.465	2925	2931	2932	rBV2	603	526	0.04%	0.005%
81	10.590	2966	2970	2972	rBV3	244	191	0.01%	0.002%
82	10.706	3004	3006	3012	rVB	236	153	0.01%	0.002%
83	10.841	3046	3048	3052	rVB2	198	98	0.01%	0.001%
84	10.863	3053	3055	3058	rVV2	340	158	0.01%	0.002%
85	10.969	3085	3088	3092	rVB3	299	242	0.02%	0.002%
86	11.005	3096	3099	3102	rBV2	274	216	0.02%	0.002%
87	11.185	3144	3155	3179	rBV	489956	775306	55.99%	7.867%
88	11.445	3232	3236	3238	rBV2	349	305	0.02%	0.003%
89	11.500	3244	3253	3260	rBV4	9562	19038	1.37%	0.193%
90	11.558	3261	3271	3298	rVB	626454	994091	71.80%	10.087%
91	12.069	3428	3430	3431	rBV	254	112	0.01%	0.001%
92	12.104	3437	3441	3443	rBV	376	292	0.02%	0.003%
93	12.227	3477	3479	3482	rBV3	331	217	0.02%	0.002%
94	12.307	3501	3504	3506	rBV3	732	479	0.03%	0.005%
95	12.387	3527	3529	3533	rVB2	491	259	0.02%	0.003%
96	12.407	3533	3535	3536	rBV	252	84	0.01%	0.001%
97	12.439	3542	3545	3546	rBV2	469	305	0.02%	0.003%
98	12.587	3588	3591	3594	rBV2	537	406	0.03%	0.004%
99	12.985	3712	3715	3719	rBV4	419	432	0.03%	0.004%
100	13.207	3780	3784	3790	rBV3	2052	1927	0.14%	0.020%




Sum of corrected areas: 9854704

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035392.D
Acq On : 24 Apr 2024 17:06
Operator : SY/MD
Sample : P2203-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

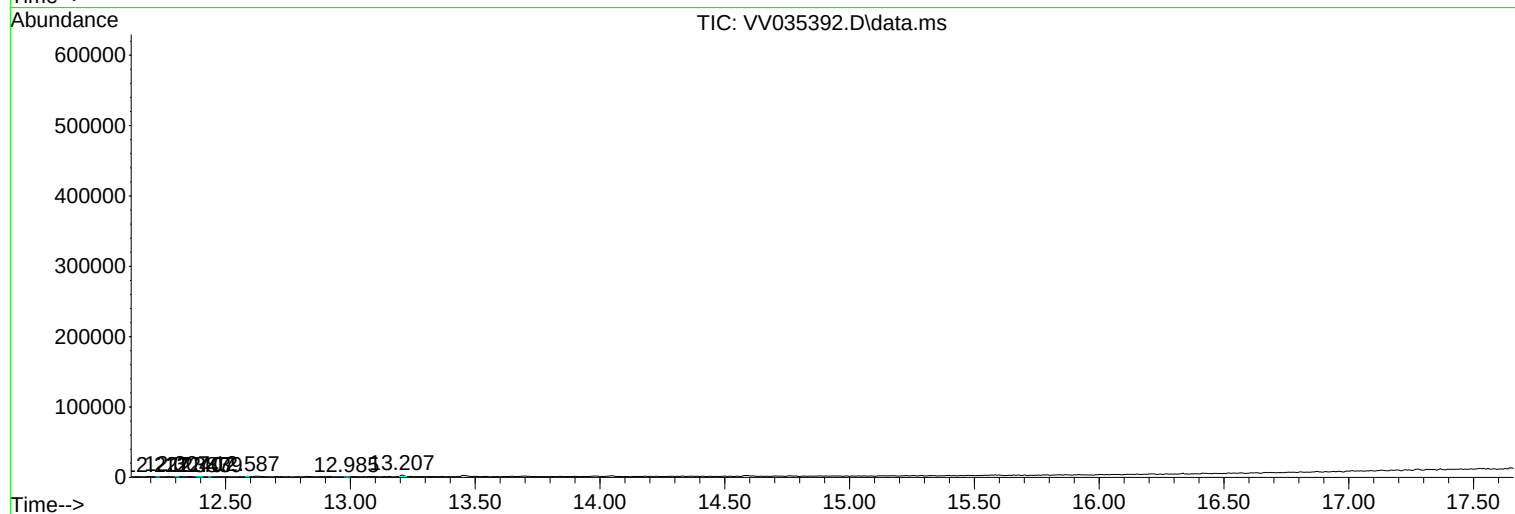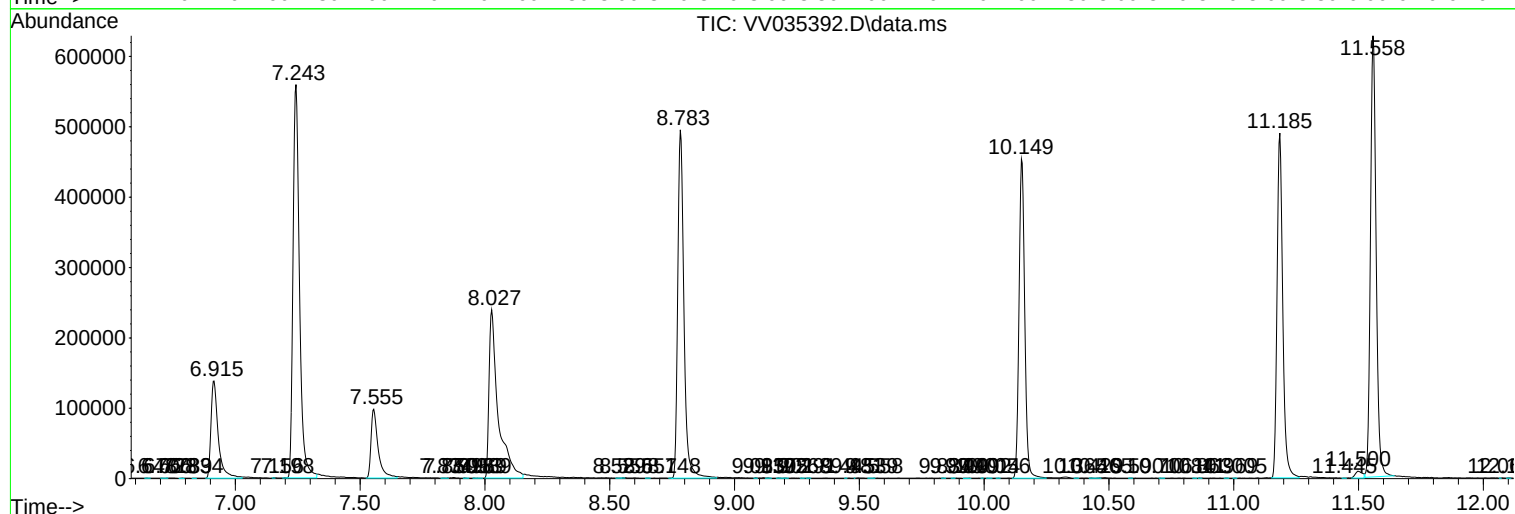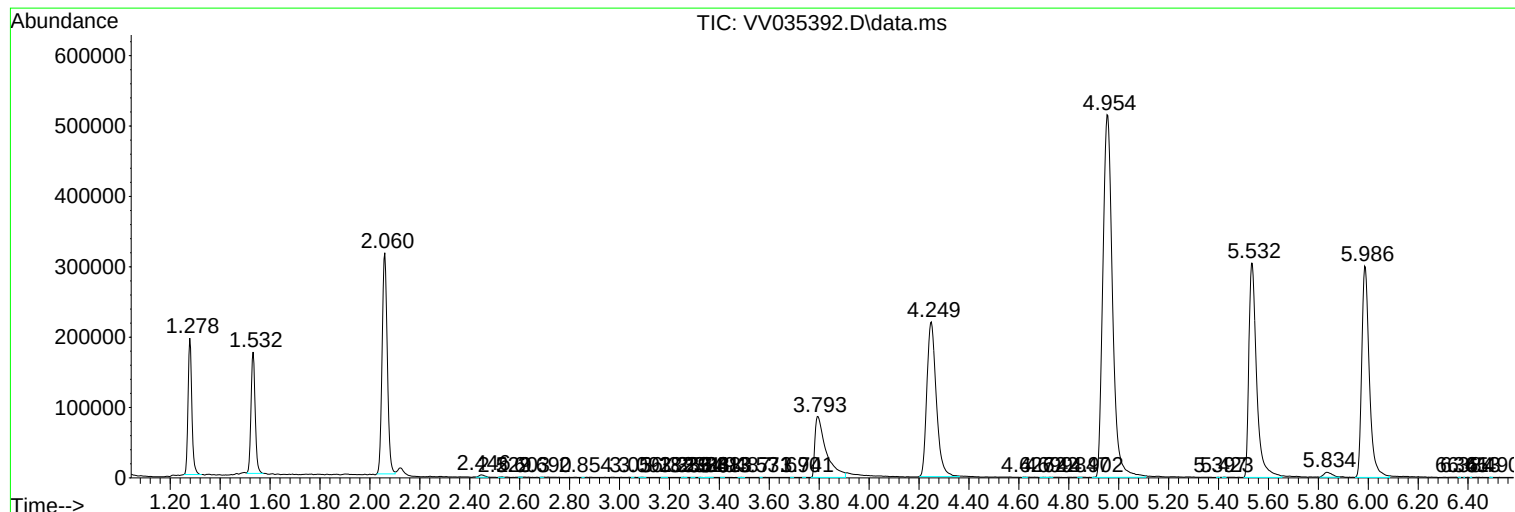

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035392.D
Acq On : 24 Apr 2024 17:06
Operator : SY/MD
Sample : P2203-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035392.D
Acq On : 24 Apr 2024 17:06
Operator : SY/MD
Sample : P2203-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc