

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035393.D
 Acq On : 24 Apr 2024 17:29
 Operator : SY/MD
 Sample : P2203-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	230533	246198	14.74%	1.991%
2	1.532	146	153	167	rVB	209592	246473	14.75%	1.994%
3	2.060	307	317	332	rBV	380384	553721	33.14%	4.479%
4	2.384	411	418	431	rBV	11084	20157	1.21%	0.163%
5	2.564	472	474	478	rVB3	410	203	0.01%	0.002%
6	2.658	501	503	506	rBV	406	258	0.02%	0.002%
7	2.699	514	516	519	rBV3	407	282	0.02%	0.002%
8	2.751	529	532	535	rBV2	280	196	0.01%	0.002%
9	2.770	535	538	540	rBV	199	141	0.01%	0.001%
10	2.841	558	560	563	rBV2	319	243	0.01%	0.002%
11	2.986	603	605	606	rBV2	374	120	0.01%	0.001%
12	3.018	613	615	618	rVB	297	113	0.01%	0.001%
13	3.056	625	627	630	rVB	192	73	0.00%	0.001%
14	3.156	655	658	660	rBV2	156	103	0.01%	0.001%
15	3.214	673	676	678	rBV2	198	152	0.01%	0.001%
16	3.288	696	699	700	rBV	96	51	0.00%	0.000%
17	3.301	700	703	707	rVV	225	238	0.01%	0.002%
18	3.336	711	714	716	rBV	116	83	0.00%	0.001%
19	3.349	716	718	720	rVV2	133	60	0.00%	0.000%
20	3.365	720	723	725	rVV2	124	74	0.00%	0.001%
21	3.407	732	736	741	rVB2	234	237	0.01%	0.002%
22	3.429	741	743	744	rBV	171	85	0.01%	0.001%
23	3.471	754	756	760	rBV	172	105	0.01%	0.001%
24	3.532	772	775	780	rBV2	176	178	0.01%	0.001%
25	3.584	789	791	797	rVB2	223	221	0.01%	0.002%
26	3.616	798	801	803	rBV2	106	74	0.00%	0.001%
27	3.642	807	809	812	rBV2	165	95	0.01%	0.001%
28	3.661	812	815	816	rBV	172	104	0.01%	0.001%
29	3.716	830	832	837	rBV2	216	109	0.01%	0.001%
30	3.793	847	856	899	rBV	109951	343805	20.58%	2.781%
31	4.246	983	997	1037	rBV2	267222	697676	41.76%	5.643%
32	4.748	1149	1153	1155	rBV	432	315	0.02%	0.003%
33	4.831	1176	1179	1182	rVB2	417	250	0.01%	0.002%
34	4.957	1201	1218	1249	rBV2	626451	1670731	100.00%	13.514%
35	5.532	1386	1397	1447	rBV	417682	894676	53.55%	7.237%
36	5.838	1482	1492	1511	rVB5	8629	20898	1.25%	0.169%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035393.D
 Acq On : 24 Apr 2024 17:29
 Operator : SY/MD
 Sample : P2203-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1526	1538	1576	rBV	369852	774055	46.33%	6.261%
38	6.278	1627	1629	1632	rVB2	512	269	0.02%	0.002%
39	6.358	1650	1654	1655	rBV2	357	193	0.01%	0.002%
40	6.371	1656	1658	1661	rVV	334	183	0.01%	0.001%
41	6.391	1661	1664	1669	rVB	470	383	0.02%	0.003%
42	6.416	1669	1672	1675	rVB2	302	175	0.01%	0.001%
43	6.436	1675	1678	1681	rBV2	275	186	0.01%	0.002%
44	6.449	1681	1682	1684	rBV	141	74	0.00%	0.001%
45	6.513	1700	1702	1703	rBV	206	73	0.00%	0.001%
46	6.635	1736	1740	1742	rBV2	482	310	0.02%	0.003%
47	6.735	1766	1771	1775	rBV2	322	365	0.02%	0.003%
48	6.767	1779	1781	1782	rBV	148	36	0.00%	0.000%
49	6.776	1782	1784	1789	rVB2	245	150	0.01%	0.001%
50	6.841	1802	1804	1810	rVB3	260	172	0.01%	0.001%
51	6.912	1816	1826	1851	rBV	171392	336990	20.17%	2.726%
52	7.243	1917	1929	1954	rBV	705544	1249898	74.81%	10.110%
53	7.555	2016	2026	2055	rBV	122602	231505	13.86%	1.873%
54	7.911	2133	2137	2141	rBV3	503	533	0.03%	0.004%
55	7.976	2155	2157	2160	rVB2	384	156	0.01%	0.001%
56	8.027	2160	2173	2237	rBV2	312521	781012	46.75%	6.317%
57	8.426	2295	2297	2304	rVB3	644	518	0.03%	0.004%
58	8.664	2369	2371	2374	rVB	220	86	0.01%	0.001%
59	8.677	2374	2375	2377	rBV	109	51	0.00%	0.000%
60	8.783	2397	2408	2447	rBV	680691	1128756	67.56%	9.130%
61	9.194	2532	2536	2539	rBV3	455	489	0.03%	0.004%
62	9.236	2545	2549	2551	rBV2	339	203	0.01%	0.002%
63	9.246	2551	2552	2555	rVB	271	127	0.01%	0.001%
64	9.288	2563	2565	2569	rBV2	264	171	0.01%	0.001%
65	9.339	2578	2581	2582	rBV	241	124	0.01%	0.001%
66	9.413	2602	2604	2605	rBV	201	75	0.00%	0.001%
67	9.445	2612	2614	2618	rVB	300	144	0.01%	0.001%
68	9.535	2639	2642	2644	rBV2	334	142	0.01%	0.001%
69	9.548	2644	2646	2648	rVB	342	118	0.01%	0.001%
70	9.561	2648	2650	2652	rBV	183	77	0.00%	0.001%
71	9.603	2658	2663	2667	rBV3	480	416	0.02%	0.003%
72	9.664	2680	2682	2684	rBV2	260	152	0.01%	0.001%
73	9.699	2690	2693	2695	rBV2	149	98	0.01%	0.001%
74	9.809	2723	2727	2729	rBV2	179	138	0.01%	0.001%
75	9.821	2729	2731	2738	rVB	194	186	0.01%	0.002%
76	9.850	2738	2740	2743	rBV2	167	77	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035393.D
 Acq On : 24 Apr 2024 17:29
 Operator : SY/MD
 Sample : P2203-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.870	2743	2746	2748	rBV2	271	192	0.01%	0.002%
78	9.934	2761	2766	2768	rBV	266	260	0.02%	0.002%
79	10.149	2821	2833	2868	rBV	555530	891772	53.38%	7.213%
80	10.365	2898	2900	2902	rBV3	273	118	0.01%	0.001%
81	10.484	2933	2937	2939	rBV4	620	448	0.03%	0.004%
82	10.551	2956	2958	2959	rBV4	202	77	0.00%	0.001%
83	10.690	2999	3001	3003	rBV	250	91	0.01%	0.001%
84	10.738	3015	3016	3019	rVB2	265	98	0.01%	0.001%
85	10.805	3035	3037	3041	rBV2	180	92	0.01%	0.001%
86	11.001	3094	3098	3100	rBV2	419	302	0.02%	0.002%
87	11.024	3104	3105	3109	rVV	205	137	0.01%	0.001%
88	11.185	3144	3155	3179	rBV	657267	1034145	61.90%	8.365%
89	11.458	3237	3240	3242	rBV2	239	152	0.01%	0.001%
90	11.509	3248	3256	3259	rBV6	4152	6138	0.37%	0.050%
91	11.558	3261	3271	3300	rVB	768390	1217126	72.85%	9.845%
92	11.927	3382	3386	3389	rBV3	664	582	0.03%	0.005%
93	12.410	3532	3536	3543	rVB4	508	507	0.03%	0.004%
94	12.587	3589	3591	3595	rBV3	539	291	0.02%	0.002%
95	12.622	3598	3602	3611	rVB4	1343	2055	0.12%	0.017%
96	12.976	3710	3712	3716	rBV3	359	248	0.01%	0.002%
97	13.538	3885	3887	3888	rBV	499	205	0.01%	0.002%
98	13.686	3928	3933	3934	rBV3	748	701	0.04%	0.006%




Sum of corrected areas: 12363101

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035393.D
Acq On : 24 Apr 2024 17:29
Operator : SY/MD
Sample : P2203-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

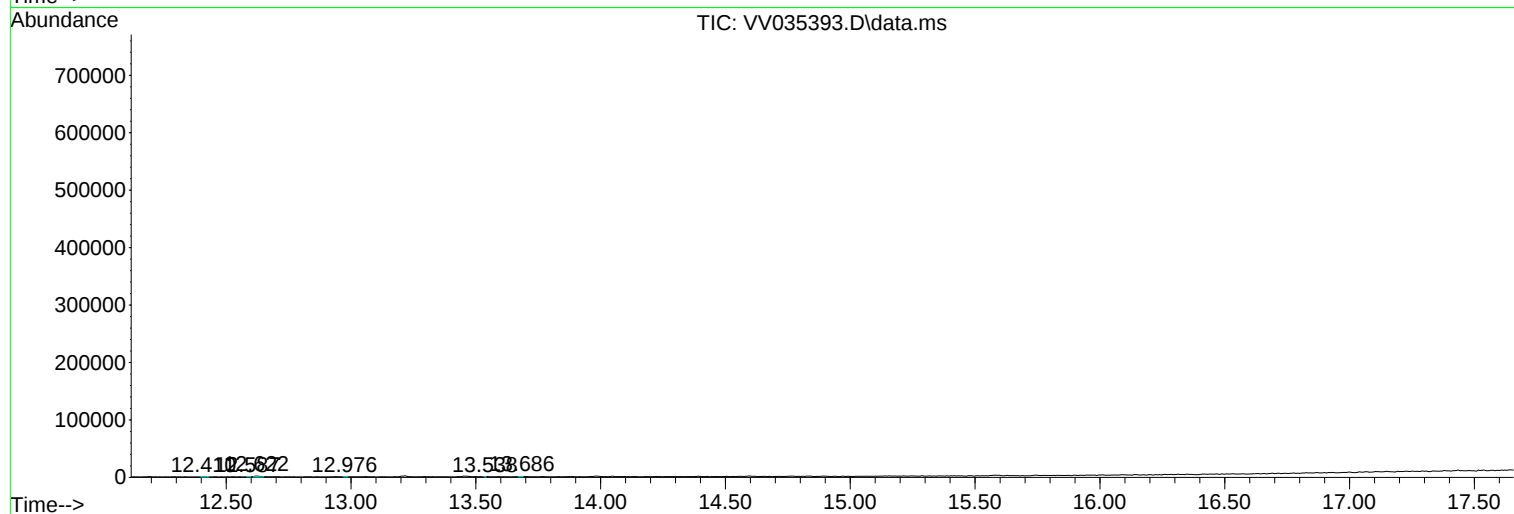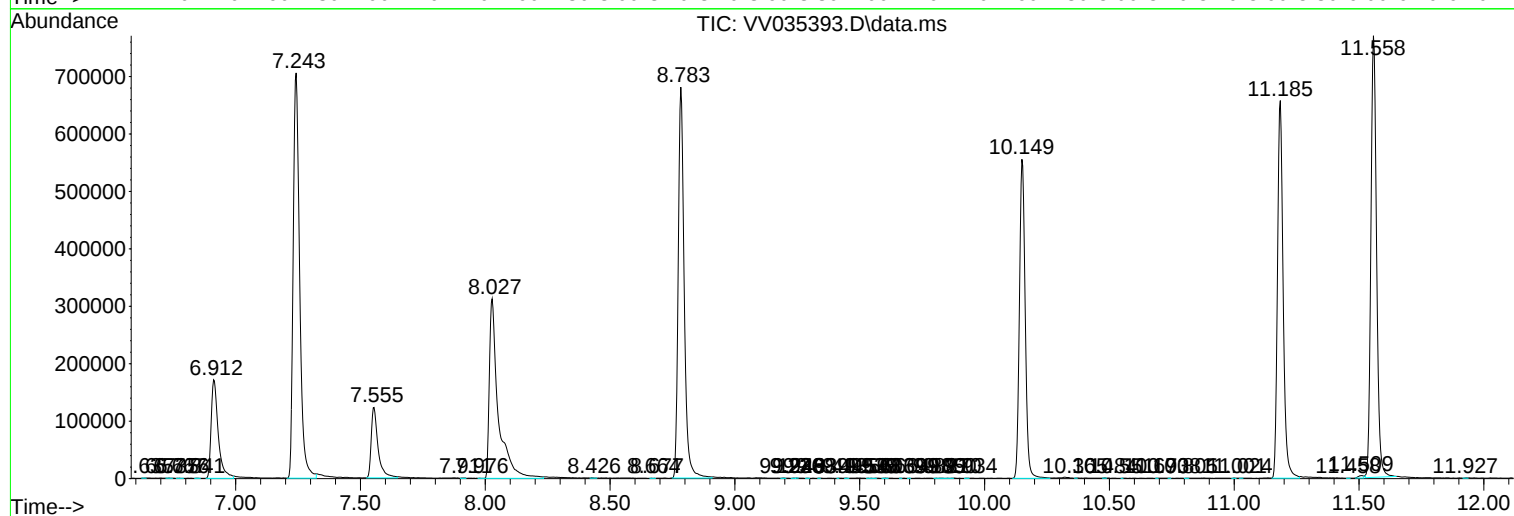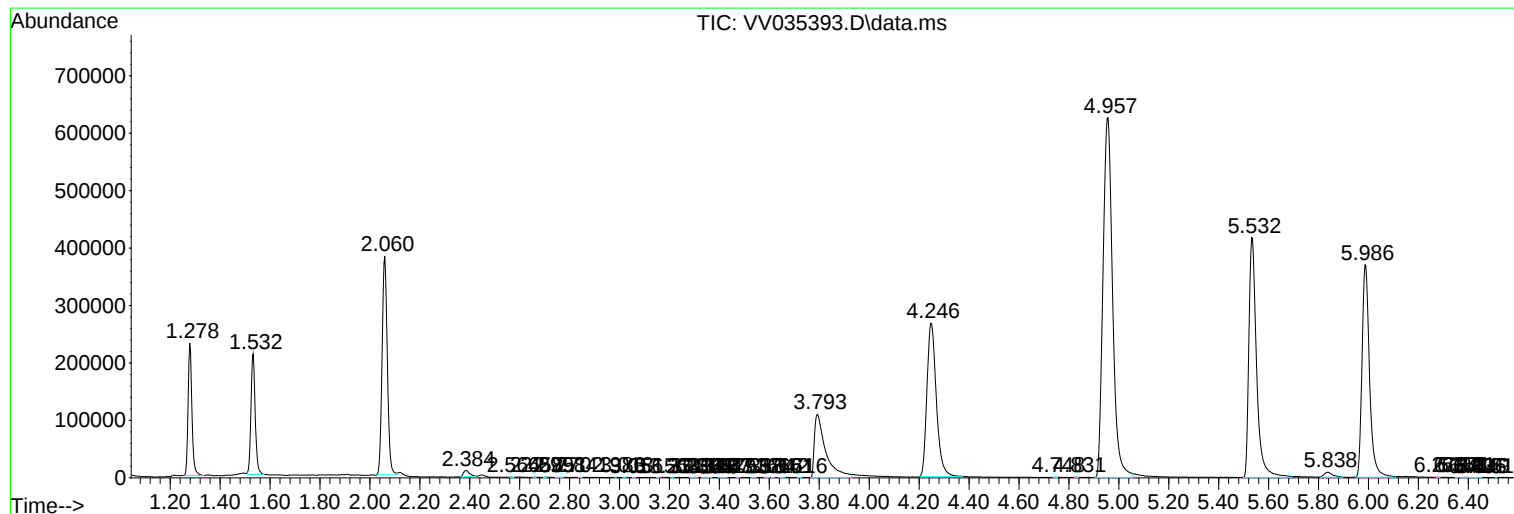

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035393.D
Acq On : 24 Apr 2024 17:29
Operator : SY/MD
Sample : P2203-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035393.D
Acq On : 24 Apr 2024 17:29
Operator : SY/MD
Sample : P2203-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------