

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035394.D
 Acq On : 24 Apr 2024 17:53
 Operator : SY/MD
 Sample : P2203-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	226002	238648	14.49%	1.962%
2	1.532	146	153	173	rVB	204480	241505	14.67%	1.985%
3	2.060	307	317	330	rBV	371758	539018	32.74%	4.431%
4	2.381	410	417	431	rBV	10433	19632	1.19%	0.161%
5	2.751	530	532	535	rBV2	227	167	0.01%	0.001%
6	2.767	535	537	541	rVB	536	317	0.02%	0.003%
7	2.947	589	593	596	rBV2	163	157	0.01%	0.001%
8	2.963	596	598	599	rVV	363	137	0.01%	0.001%
9	2.973	599	601	606	rVB3	327	193	0.01%	0.002%
10	3.092	636	638	641	rBV	167	142	0.01%	0.001%
11	3.137	649	652	656	rVB	300	195	0.01%	0.002%
12	3.368	721	724	727	rBV2	195	161	0.01%	0.001%
13	3.455	749	751	754	rBV	193	109	0.01%	0.001%
14	3.500	760	765	772	rBV2	255	383	0.02%	0.003%
15	3.532	772	775	778	rBV2	164	142	0.01%	0.001%
16	3.600	793	796	802	rBV2	207	220	0.01%	0.002%
17	3.645	806	810	812	rBV2	172	157	0.01%	0.001%
18	3.690	821	824	828	rBV2	351	335	0.02%	0.003%
19	3.793	847	856	893	rBV	108205	335293	20.36%	2.756%
20	4.249	983	998	1033	rBV	262933	681061	41.36%	5.598%
21	4.596	1104	1106	1108	rBV2	354	197	0.01%	0.002%
22	4.895	1196	1199	1202	rBV2	301	231	0.01%	0.002%
23	4.953	1202	1217	1257	rBV2	620206	1646604	100.00%	13.535%
24	5.413	1358	1360	1365	rVB3	478	253	0.02%	0.002%
25	5.532	1387	1397	1441	rBV	416860	890640	54.09%	7.321%
26	5.838	1482	1492	1504	rBV3	8372	18073	1.10%	0.149%
27	5.924	1518	1519	1521	rBV	397	140	0.01%	0.001%
28	5.985	1525	1538	1573	rBV	360853	764785	46.45%	6.286%
29	6.333	1642	1646	1652	rBV2	712	667	0.04%	0.005%
30	6.358	1652	1654	1655	rBV	154	39	0.00%	0.000%
31	6.445	1678	1681	1685	rVB3	586	379	0.02%	0.003%
32	6.465	1685	1687	1691	rBV	289	118	0.01%	0.001%
33	6.481	1691	1692	1694	rBV	226	91	0.01%	0.001%
34	6.497	1694	1697	1699	rBV	220	126	0.01%	0.001%
35	6.532	1707	1708	1710	rVB	210	65	0.00%	0.001%
36	6.545	1710	1712	1713	rBV	263	89	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042424\
 Data File : VW035394.D
 Acq On : 24 Apr 2024 17:53
 Operator : SY/MD
 Sample : P2203-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.583	1722	1724	1727	rVB	324	158	0.01%	0.001%
38	6.619	1733	1735	1737	rVB	427	173	0.01%	0.001%
39	6.648	1737	1744	1746	rVV4	442	530	0.03%	0.004%
40	6.674	1750	1752	1755	rVV2	352	166	0.01%	0.001%
41	6.702	1758	1761	1764	rBV	264	152	0.01%	0.001%
42	6.728	1766	1769	1772	rVV	578	420	0.03%	0.003%
43	6.747	1772	1775	1778	rVV	341	239	0.01%	0.002%
44	6.776	1782	1784	1787	rVV	329	129	0.01%	0.001%
45	6.792	1787	1789	1794	rVB2	234	162	0.01%	0.001%
46	6.818	1794	1797	1799	rBV2	162	87	0.01%	0.001%
47	6.911	1816	1826	1859	rBV	171035	334610	20.32%	2.750%
48	7.243	1917	1929	1970	rBV	684000	1232543	74.85%	10.131%
49	7.555	2016	2026	2052	rBV	118404	225202	13.68%	1.851%
50	7.918	2137	2139	2142	rVB2	388	186	0.01%	0.002%
51	7.950	2146	2149	2150	rBV	217	110	0.01%	0.001%
52	7.960	2150	2152	2154	rBV2	220	88	0.01%	0.001%
53	8.027	2164	2173	2225	rBV2	303423	749927	45.54%	6.164%
54	8.548	2332	2335	2337	rBV2	663	485	0.03%	0.004%
55	8.783	2396	2408	2445	rBV	677814	1128573	68.54%	9.277%
56	9.246	2549	2552	2554	rBV	301	142	0.01%	0.001%
57	9.275	2560	2561	2562	rBV	253	82	0.00%	0.001%
58	9.525	2637	2639	2641	rVB	213	105	0.01%	0.001%
59	9.548	2644	2646	2648	rVB2	163	60	0.00%	0.000%
60	9.599	2658	2662	2667	rBV2	353	357	0.02%	0.003%
61	9.683	2684	2688	2694	rVB4	310	274	0.02%	0.002%
62	9.751	2707	2709	2711	rBV	194	102	0.01%	0.001%
63	9.924	2760	2763	2764	rBV	324	160	0.01%	0.001%
64	10.149	2820	2833	2861	rBV	549492	867173	52.66%	7.128%
65	10.500	2941	2942	2945	rBV	253	126	0.01%	0.001%
66	10.542	2953	2955	2959	rBV	243	148	0.01%	0.001%
67	10.619	2977	2979	2986	rBV3	315	275	0.02%	0.002%
68	10.699	3002	3004	3007	rBV2	295	152	0.01%	0.001%
69	10.715	3007	3009	3013	rVB	374	155	0.01%	0.001%
70	10.818	3038	3041	3043	rBV2	311	190	0.01%	0.002%
71	10.869	3053	3057	3059	rBV2	345	273	0.02%	0.002%
72	11.056	3111	3115	3116	rBV	304	194	0.01%	0.002%
73	11.091	3124	3126	3130	rVB2	361	171	0.01%	0.001%
74	11.185	3144	3155	3177	rBV	648057	1034189	62.81%	8.501%
75	11.558	3250	3271	3295	rBV	757390	1204293	73.14%	9.899%
76	12.326	3508	3510	3511	rBV	402	190	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035394.D
Acq On : 24 Apr 2024 17:53
Operator : SY/MD
Sample : P2203-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D03

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

77	12.506	3564	3566	3568	rBV2	402	223	0.01%	0.002%
78	12.522	3569	3571	3572	rVV	381	102	0.01%	0.001%
79	12.696	3623	3625	3628	rBV2	482	227	0.01%	0.002%
80	12.908	3689	3691	3695	rBV2	444	353	0.02%	0.003%
81	13.213	3780	3786	3791	rVB5	1467	1600	0.10%	0.013%




Sum of corrected areas: 12165725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035394.D
Acq On : 24 Apr 2024 17:53
Operator : SY/MD
Sample : P2203-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

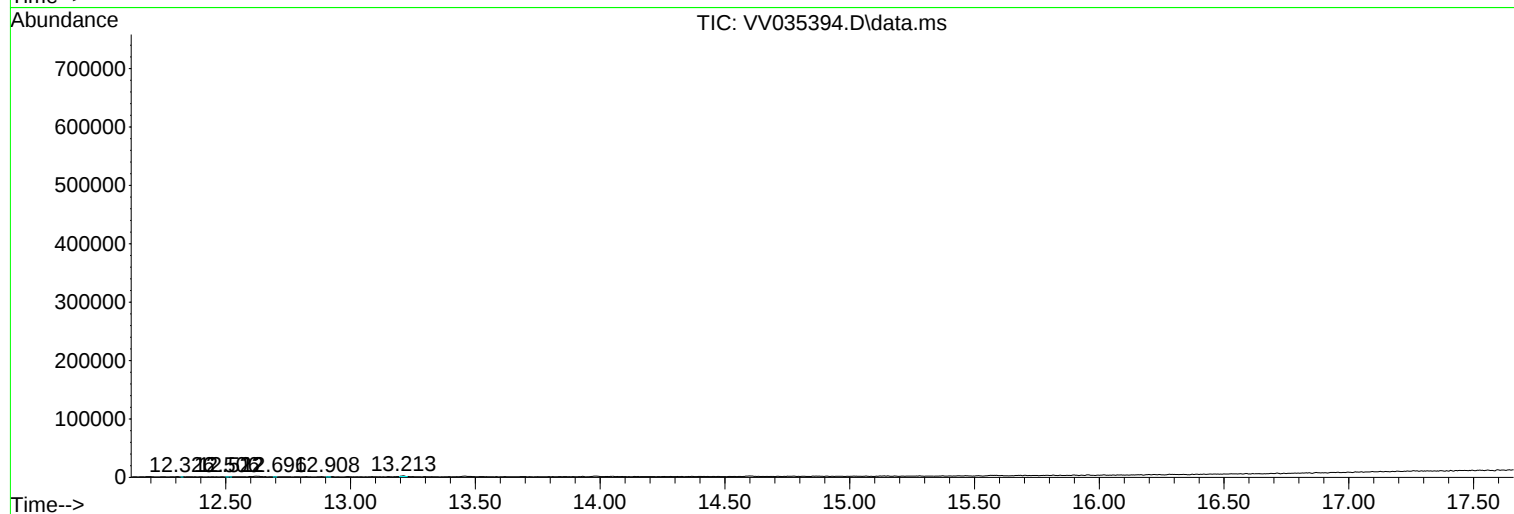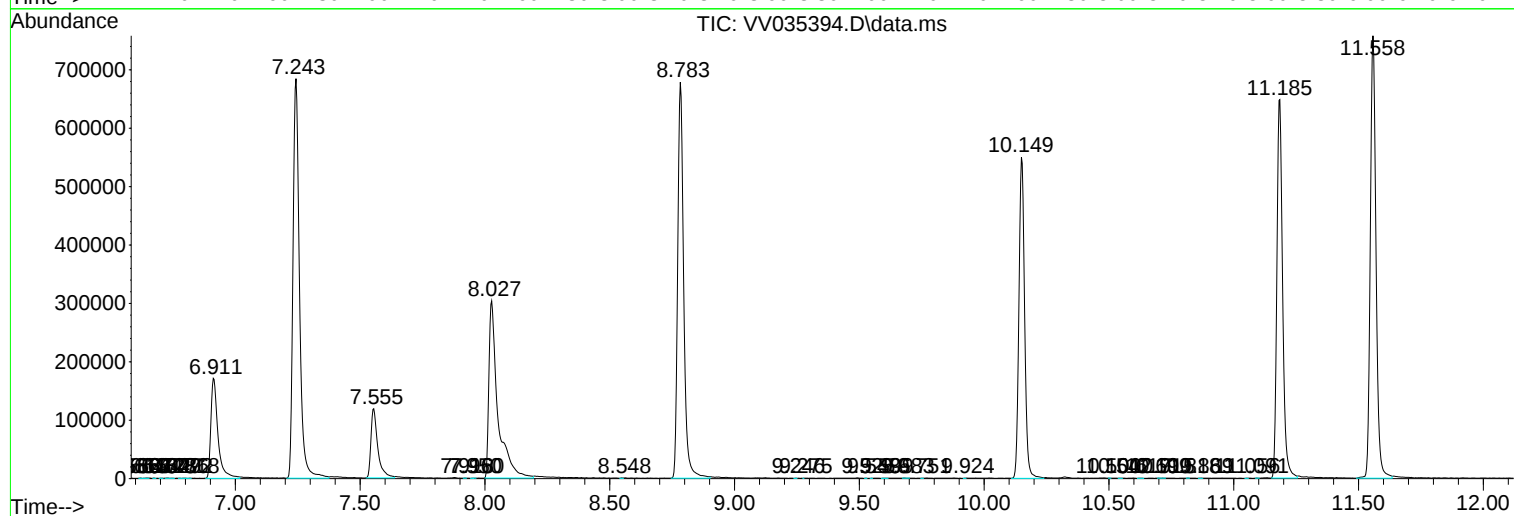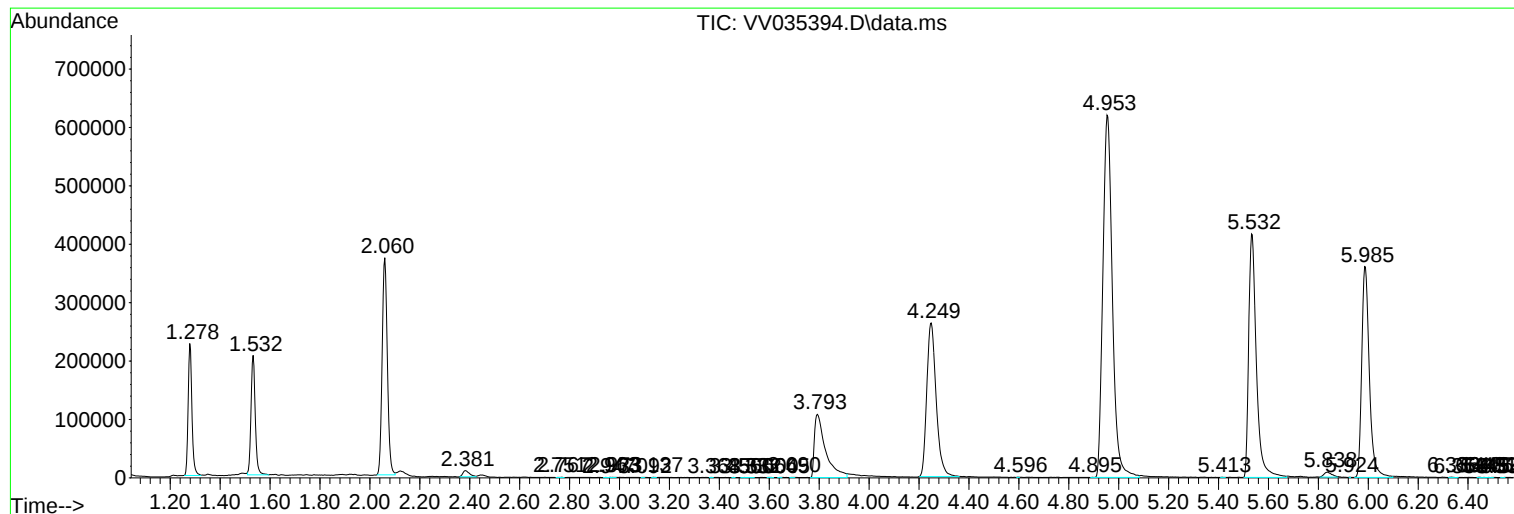

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035394.D
Acq On : 24 Apr 2024 17:53
Operator : SY/MD
Sample : P2203-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035394.D
Acq On : 24 Apr 2024 17:53
Operator : SY/MD
Sample : P2203-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc