

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035395.D
 Acq On : 24 Apr 2024 18:16
 Operator : SY/MD
 Sample : P2203-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	219179	232755	14.38%	1.963%
2	1.532	146	153	166	rVB	197829	230480	14.24%	1.944%
3	2.060	308	317	331	rBV	359726	513796	31.74%	4.334%
4	2.381	411	417	430	rBV	9997	18151	1.12%	0.153%
5	2.783	540	542	543	rBV	329	159	0.01%	0.001%
6	2.844	558	561	565	rVB3	267	190	0.01%	0.002%
7	2.912	580	582	586	rBV2	204	136	0.01%	0.001%
8	2.931	586	588	595	rVB	241	185	0.01%	0.002%
9	2.973	599	601	602	rBV	361	112	0.01%	0.001%
10	2.982	602	604	607	rVB2	315	145	0.01%	0.001%
11	2.998	607	609	611	rBV2	200	136	0.01%	0.001%
12	3.043	620	623	625	rVB	370	181	0.01%	0.002%
13	3.089	633	637	640	rBV	180	148	0.01%	0.001%
14	3.117	644	646	647	rBV	218	99	0.01%	0.001%
15	3.150	653	656	658	rBV	185	112	0.01%	0.001%
16	3.166	658	661	664	rVV3	272	196	0.01%	0.002%
17	3.281	694	697	699	rBV2	162	114	0.01%	0.001%
18	3.314	703	707	710	rVB2	342	217	0.01%	0.002%
19	3.365	720	723	726	rBV	127	91	0.01%	0.001%
20	3.423	738	741	744	rBV	147	115	0.01%	0.001%
21	3.445	744	748	752	rBV2	324	257	0.02%	0.002%
22	3.542	775	778	781	rBV2	180	99	0.01%	0.001%
23	3.590	791	793	795	rVB	326	126	0.01%	0.001%
24	3.667	813	817	820	rBV2	238	151	0.01%	0.001%
25	3.709	827	830	833	rBV2	245	209	0.01%	0.002%
26	3.793	847	856	892	rBV	107434	328156	20.27%	2.768%
27	4.249	982	998	1035	rBV	257795	676101	41.77%	5.703%
28	4.506	1076	1078	1081	rBV3	597	282	0.02%	0.002%
29	4.658	1121	1125	1126	rBV	351	269	0.02%	0.002%
30	4.725	1143	1146	1148	rBV3	269	172	0.01%	0.001%
31	4.805	1169	1171	1178	rBV3	409	317	0.02%	0.003%
32	4.892	1196	1198	1199	rBV3	348	143	0.01%	0.001%
33	4.953	1202	1217	1259	rVV2	611061	1618642	100.00%	13.653%
34	5.532	1387	1397	1428	rBV	404847	851177	52.59%	7.179%
35	5.989	1525	1539	1574	rBV	354858	755420	46.67%	6.372%
36	6.317	1638	1641	1643	rBV2	340	176	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035395.D
 Acq On : 24 Apr 2024 18:16
 Operator : SY/MD
 Sample : P2203-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.330	1643	1645	1646	rBV2	305	114	0.01%	0.001%
38	6.362	1653	1655	1658	rVB2	285	143	0.01%	0.001%
39	6.522	1703	1705	1708	rVB2	226	95	0.01%	0.001%
40	6.558	1713	1716	1719	rBV2	108	98	0.01%	0.001%
41	6.600	1726	1729	1732	rVB3	245	166	0.01%	0.001%
42	6.632	1736	1739	1741	rBV	376	274	0.02%	0.002%
43	6.680	1750	1754	1755	rBV3	286	192	0.01%	0.002%
44	6.793	1787	1789	1792	rVB	294	111	0.01%	0.001%
45	6.809	1792	1794	1796	rBV	152	87	0.01%	0.001%
46	6.847	1801	1806	1808	rBV2	215	222	0.01%	0.002%
47	6.912	1816	1826	1852	rBV	166868	325276	20.10%	2.744%
48	7.188	1909	1912	1913	rBV	311	174	0.01%	0.001%
49	7.243	1918	1929	1953	rBV	677175	1197226	73.96%	10.098%
50	7.555	2016	2026	2059	rBV	117869	225602	13.94%	1.903%
51	7.918	2135	2139	2143	rVB3	619	585	0.04%	0.005%
52	7.944	2143	2147	2151	rBV	303	312	0.02%	0.003%
53	7.985	2156	2160	2163	rVB2	355	228	0.01%	0.002%
54	8.027	2164	2173	2223	rBV3	299021	740159	45.73%	6.243%
55	8.465	2306	2309	2311	rBV2	374	247	0.02%	0.002%
56	8.506	2320	2322	2328	rBV3	440	384	0.02%	0.003%
57	8.596	2348	2350	2354	rVB2	310	188	0.01%	0.002%
58	8.657	2363	2369	2379	rBV5	634	879	0.05%	0.007%
59	8.699	2380	2382	2385	rVB2	471	219	0.01%	0.002%
60	8.715	2385	2387	2389	rBV	225	118	0.01%	0.001%
61	8.741	2389	2395	2396	rBV	307	290	0.02%	0.002%
62	8.783	2397	2408	2446	rBV	651436	1097803	67.82%	9.260%
63	9.149	2520	2522	2523	rBV	281	102	0.01%	0.001%
64	9.239	2547	2550	2552	rBV2	312	228	0.01%	0.002%
65	9.320	2570	2575	2579	rVB3	358	354	0.02%	0.003%
66	9.368	2586	2590	2592	rBV2	271	223	0.01%	0.002%
67	9.455	2612	2617	2620	rBV2	228	236	0.01%	0.002%
68	9.490	2624	2628	2633	rVB3	313	290	0.02%	0.002%
69	9.526	2637	2639	2640	rBV3	234	94	0.01%	0.001%
70	9.609	2663	2665	2674	rVB2	282	209	0.01%	0.002%
71	9.664	2680	2682	2685	rBV2	338	197	0.01%	0.002%
72	9.718	2697	2699	2704	rVB	277	205	0.01%	0.002%
73	9.747	2706	2708	2713	rVV2	279	194	0.01%	0.002%
74	9.799	2722	2724	2728	rVB2	261	184	0.01%	0.002%
75	9.818	2728	2730	2731	rBV2	258	116	0.01%	0.001%
76	9.879	2746	2749	2753	rBV3	537	422	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035395.D
 Acq On : 24 Apr 2024 18:16
 Operator : SY/MD
 Sample : P2203-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.966	2770	2776	2778	rBV2	279	256	0.02%	0.002%
78	10.017	2790	2792	2794	rBV2	163	87	0.01%	0.001%
79	10.149	2821	2833	2859	rBV	544469	864143	53.39%	7.289%
80	10.400	2908	2911	2917	rVB2	550	335	0.02%	0.003%
81	10.435	2919	2922	2927	rBV	371	251	0.02%	0.002%
82	10.471	2927	2933	2936	rBV5	610	723	0.04%	0.006%
83	10.558	2957	2960	2962	rBV	389	240	0.01%	0.002%
84	10.786	3029	3031	3035	rBV	333	176	0.01%	0.001%
85	10.918	3067	3072	3074	rBV	344	310	0.02%	0.003%
86	11.127	3130	3137	3140	rBV3	634	805	0.05%	0.007%
87	11.185	3144	3155	3184	rBV	620826	999779	61.77%	8.433%
88	11.558	3261	3271	3303	rVB	739010	1162483	71.82%	9.805%
89	11.757	3331	3333	3338	rBV4	566	405	0.03%	0.003%
90	12.033	3417	3419	3420	rBV	412	164	0.01%	0.001%
91	12.133	3448	3450	3452	rVB	340	153	0.01%	0.001%
92	12.165	3458	3460	3462	rBV	397	175	0.01%	0.001%
93	12.313	3502	3506	3509	rBV2	424	309	0.02%	0.003%
94	12.336	3509	3513	3516	rVB2	568	406	0.03%	0.003%
95	12.400	3531	3533	3535	rBV2	387	135	0.01%	0.001%
96	12.535	3573	3575	3577	rBV	275	153	0.01%	0.001%
97	12.718	3629	3632	3635	rBV3	318	266	0.02%	0.002%
98	13.062	3735	3739	3741	rBV	430	315	0.02%	0.003%
99	13.078	3741	3744	3746	rBV2	374	216	0.01%	0.002%
100	13.287	3807	3809	3810	rBV2	317	140	0.01%	0.001%




Sum of corrected areas: 11855886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035395.D
Acq On : 24 Apr 2024 18:16
Operator : SY/MD
Sample : P2203-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

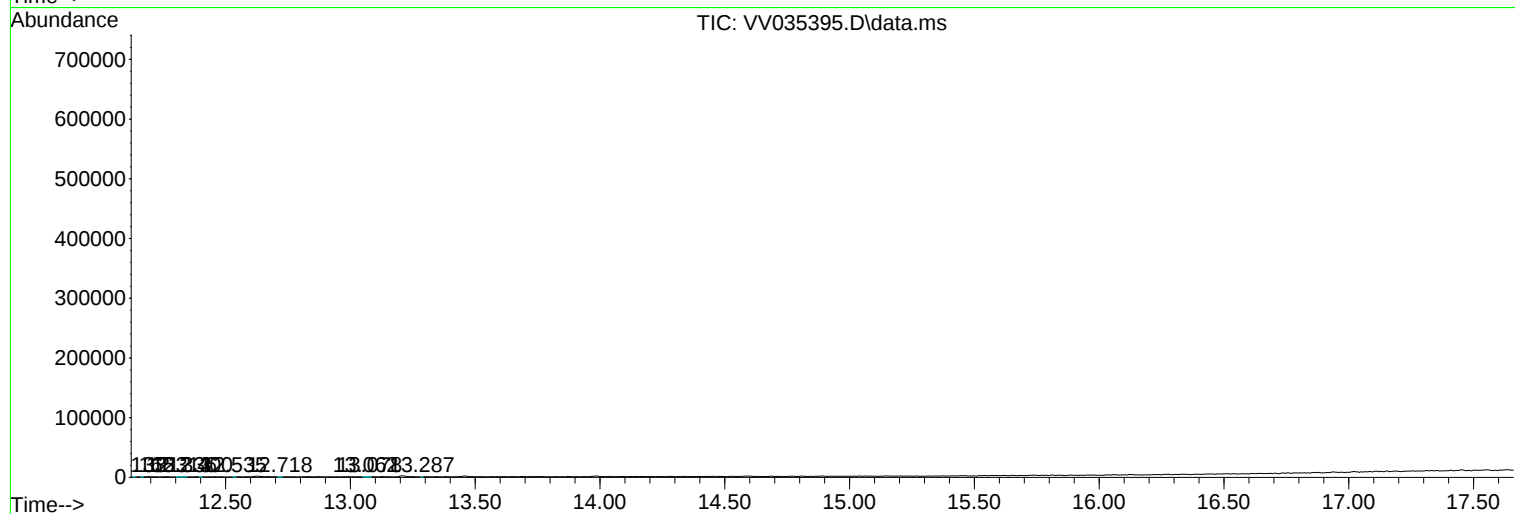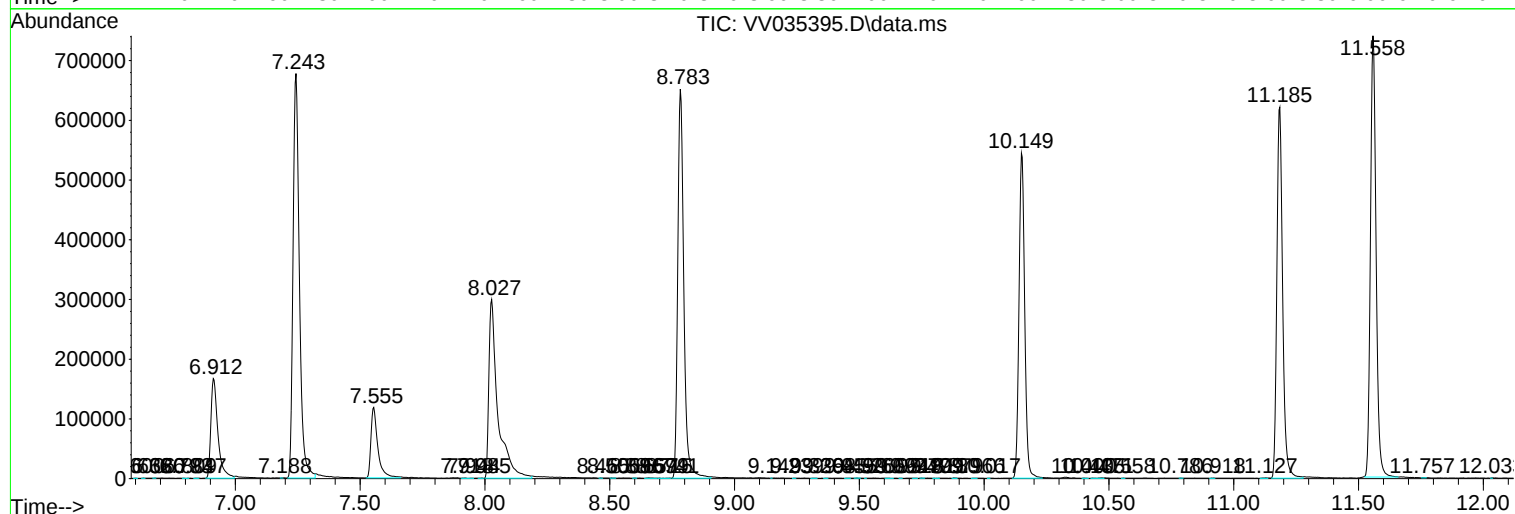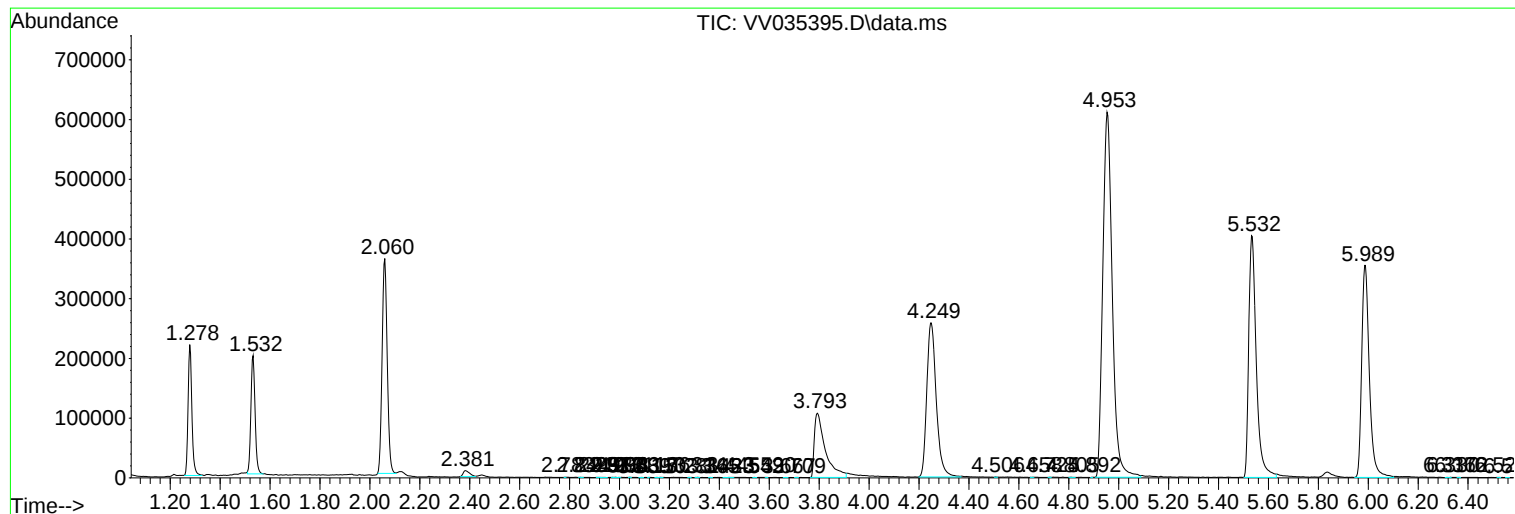

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035395.D
Acq On : 24 Apr 2024 18:16
Operator : SY/MD
Sample : P2203-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035395.D
Acq On : 24 Apr 2024 18:16
Operator : SY/MD
Sample : P2203-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc