
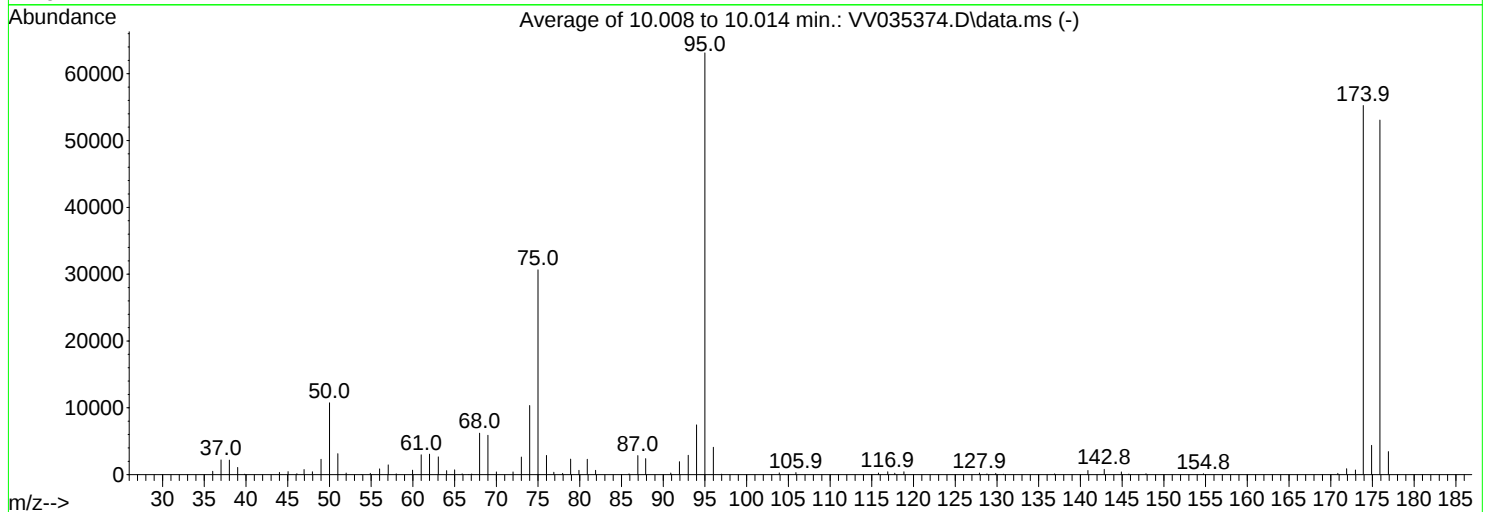


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035374.D
Acq On : 24 Apr 2024 09:02
Operator : SY/MD
Sample : BFB290
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB290

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Thu Apr 25 01:57:41 2024

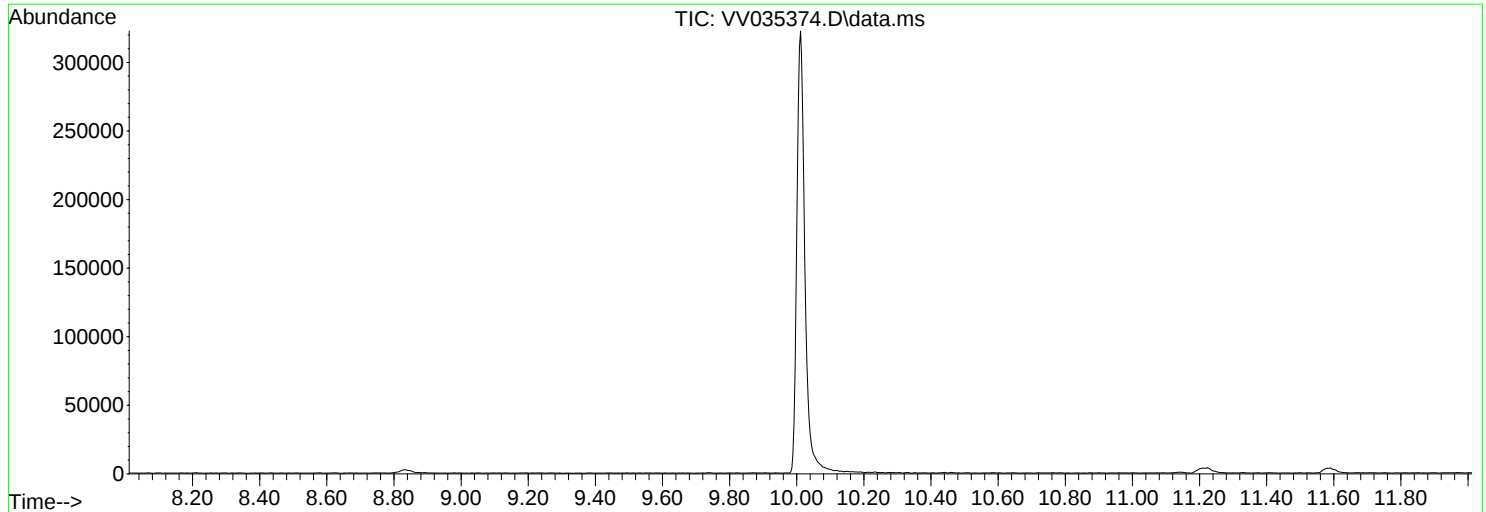

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	10746	PASS
75	95	30	80	48.5	30645	PASS
95	95	100	100	100.0	63125	PASS
96	95	5	9	6.5	4105	PASS
173	174	0.00	2	1.3	703	PASS
174	95	50	120	87.5	55245	PASS
175	174	5	9	7.9	4391	PASS
176	174	95	105	96.1	53072	PASS
177	176	5	10	6.5	3460	PASS

m/z	Abundance
39.80	267.0
44.10	409.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	538.0
37.00	2219.0
38.00	2285.0
39.00	1080.0
39.90	338.0
44.00	790.0
45.00	439.0
46.10	165.0
47.00	749.0
48.00	432.0
49.00	2413.0
50.00	11074.0
51.00	3262.0
52.00	251.0
54.90	182.0
56.00	954.0
57.00	1502.0
58.00	131.0
60.00	668.0
61.00	3135.0
62.00	3256.0
63.10	2717.0
64.10	617.0
65.00	628.0
66.00	111.0
66.70	105.0
68.00	6121.0
69.00	5860.0
70.00	430.0
72.00	420.0
73.00	2692.0
74.00	10506.0
75.00	30272.0
76.00	2882.0
76.90	351.0
78.00	230.0
78.90	2284.0
79.90	603.0
80.90	2377.0
81.90	589.0
85.90	137.0
87.00	3053.0
87.90	2387.0
90.90	205.0
91.90	1982.0
93.00	2884.0
94.00	7445.0
95.00	63552.0
96.00	4123.0
97.00	135.0
103.90	256.0
105.90	324.0
115.80	223.0
116.90	404.0
117.70	252.0
118.80	379.0
127.90	258.0
128.80	123.0
129.90	189.0
130.80	126.0
136.90	151.0
140.90	613.0
142.80	781.0
144.90	387.0
145.80	106.0
147.90	162.0
154.70	164.0
170.90	200.0
171.90	860.0
172.90	732.0
173.90	53704.0
174.90	4445.0
175.90	51064.0
176.90	3370.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	515.0
37.00	2227.0
38.00	2229.0
39.00	1109.0
39.90	353.0
44.00	747.0
45.10	483.0
46.10	154.0
47.00	818.0
47.90	442.0
49.00	2365.0
50.00	11083.0
51.00	3246.0
52.00	250.0
54.90	206.0
56.00	896.0
57.10	1514.0
58.00	143.0
59.90	712.0
61.00	3015.0
62.00	3177.0
63.10	2764.0
64.00	646.0
65.00	693.0
65.90	128.0
67.10	125.0
68.00	6318.0
69.00	6095.0
70.00	436.0
72.00	418.0
73.00	2694.0
74.00	10682.0
75.00	31592.0
76.00	2959.0
76.90	381.0
78.00	206.0
78.90	2383.0
79.90	667.0
80.90	2323.0
81.90	665.0
85.90	135.0
87.00	2967.0
87.90	2431.0
90.90	257.0
91.90	2002.0
93.00	3000.0
94.00	7772.0
95.00	65176.0
96.00	4270.0
97.00	105.0
103.90	265.0
105.90	330.0
115.80	259.0
116.90	440.0
117.80	228.0
118.90	434.0
127.90	267.0
128.80	128.0
129.80	188.0
130.80	126.0
136.90	142.0
140.90	677.0
142.90	800.0
144.90	426.0
145.80	104.0
147.80	154.0
154.80	140.0
170.80	191.0
171.90	927.0
173.00	740.0
173.90	56968.0
174.90	4562.0
175.90	54840.0
176.90	3613.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	446.0
37.00	2140.0
38.00	2021.0
39.00	1015.0
39.90	345.0
44.00	697.0
45.00	452.0
46.10	121.0
46.90	733.0
47.90	395.0
49.00	2152.0
50.00	10082.0
51.00	2898.0
52.00	217.0
53.80	105.0
54.90	201.0
56.00	749.0
57.00	1392.0
58.00	122.0
59.90	622.0
61.00	2761.0
62.00	2792.0
63.00	2522.0
64.00	564.0
65.00	803.0
65.80	134.0
67.00	169.0
68.00	6149.0
69.00	5746.0
70.00	383.0
72.00	382.0
73.00	2541.0
74.00	9832.0
75.00	30072.0
76.00	2756.0
76.90	323.0
77.90	166.0
78.90	2325.0
79.90	664.0
80.90	2174.0
81.90	691.0
85.90	133.0
86.90	2534.0
87.90	2380.0
90.90	275.0
92.00	1861.0
93.00	2790.0
94.00	7161.0
95.00	60648.0
96.00	3923.0
103.90	256.0
105.90	275.0
115.80	263.0
116.90	446.0
117.80	214.0
118.90	465.0
127.90	233.0
128.80	131.0
129.80	199.0
136.90	108.0
140.90	578.0
142.90	808.0
144.90	401.0
145.80	105.0
147.80	135.0
154.80	117.0
170.80	196.0
171.90	895.0
173.00	636.0
173.90	55064.0
174.90	4167.0
175.90	53312.0
176.90	3396.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290