
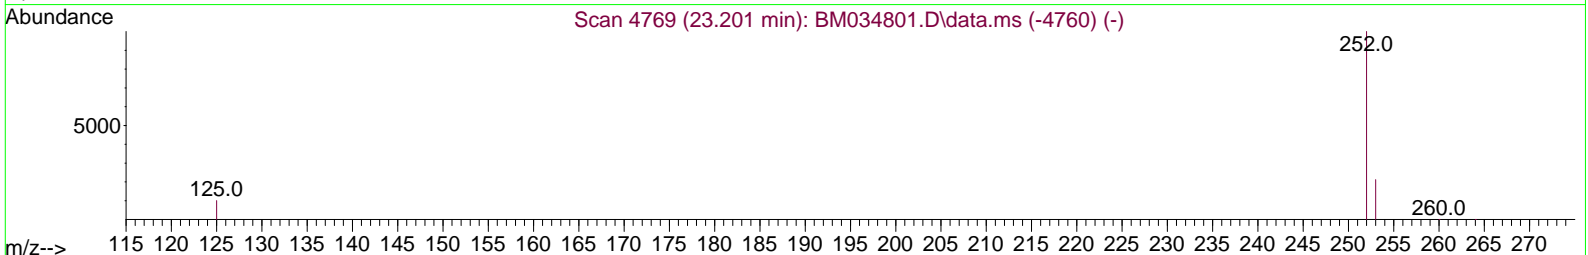
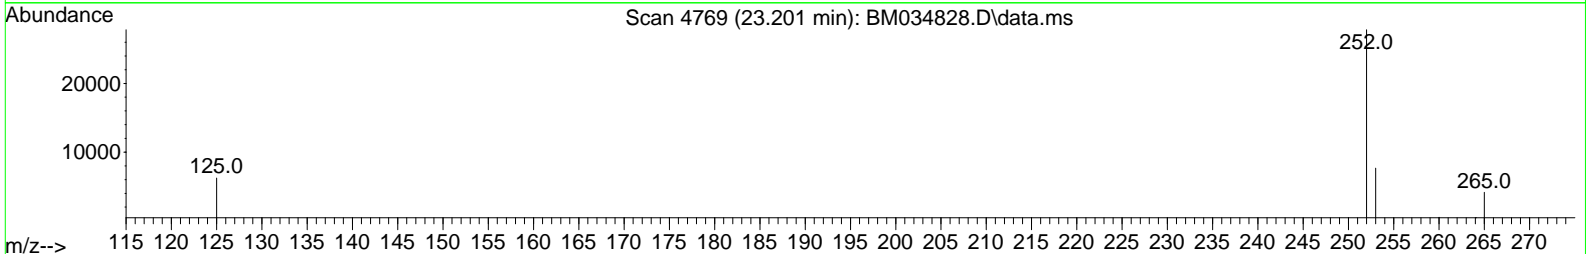


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042522\  
 Data File : BM034828.D  
 Acq On : 26 Apr 2022 09:08  
 Operator : CG/JU  
 Sample : N2374-09  
 Misc :  
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Apr 26 15:59:44 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM042222.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Apr 22 16:54:34 2022  
 Response via : Initial Calibration

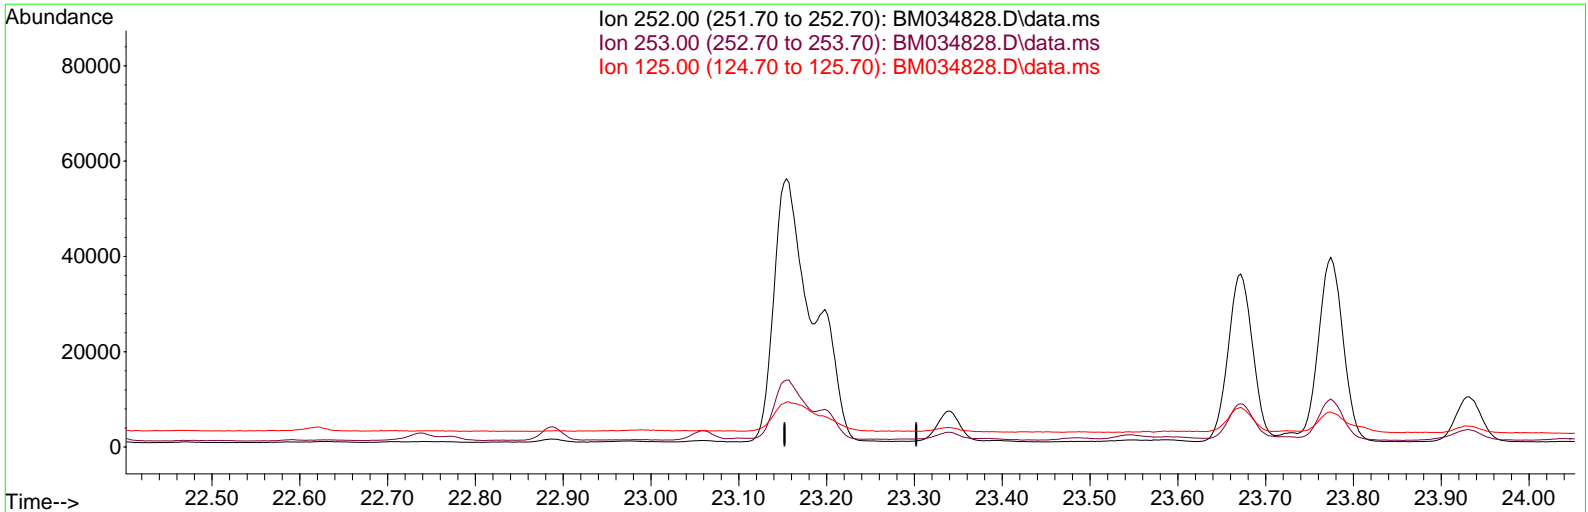

TIC: BM034828.D\data.ms

(25) Benzo(k)fluoranthene

23.202min (-23.202) 0.00 ng/ul

response	0	
Ion	Exp%	Act%
252.00	100.00	0.00
253.00	33.50	0.00#
125.00	15.00	0.00#
0.00	0.00	0.00