

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042522\
 Data File : VW025707.D
 Acq On : 25 Apr 2022 11:29
 Operator : SY/MD
 Sample : N2530-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X1

Quant Time: Apr 26 06:33:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 26 06:32:17 2022
 Response via : Initial Calibration


Compound	R.T. QIon		Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	155975	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	160893	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72406	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	93871	6.473	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	129.400%	
7) Chloroethane-d5	1.571	69	91781	5.949	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	119.000%	
11) 1,1-Dichloroethene-d2	2.111	63	142278	4.898	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	98.000%	
20) 2-Butanone-d5	3.886	46	119419	67.701	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	135.400%#	
24) Chloroform-d	4.349	84	145782	6.653	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	133.000%#	
26) 1,2-Dichloroethane-d4	5.031	65	68119	7.215	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	144.200%#	
32) Benzene-d6	5.050	84	302793	6.504	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	130.000%#	
36) 1,2-Dichloropropane-d6	6.069	67	86644	6.674	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	133.400%	
41) Toluene-d8	7.313	98	259049	5.996	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	120.000%	
43) trans-1,3-Dichloroprop...	7.622	79	26371	6.043	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	120.800%	
46) 2-Hexanone-d5	8.085	63	90505	59.094	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	118.180%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	49305	6.011	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	120.200%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	81822	6.740	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	134.800%#	
Target Compounds						Qvalue
14) Carbon disulfide	2.298	76	3136	0.097	ug/L #	92
42) Toluene	7.394	91	10830	0.209	ug/L	95
47) Tetrachloroethene	7.979	164	2350	0.238	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025707.D
Acq On : 25 Apr 2022 11:29
Operator : SY/MD
Sample : N2530-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X1


Quant Time: Apr 26 06:33:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 26 06:32:17 2022
Response via : Initial Calibration

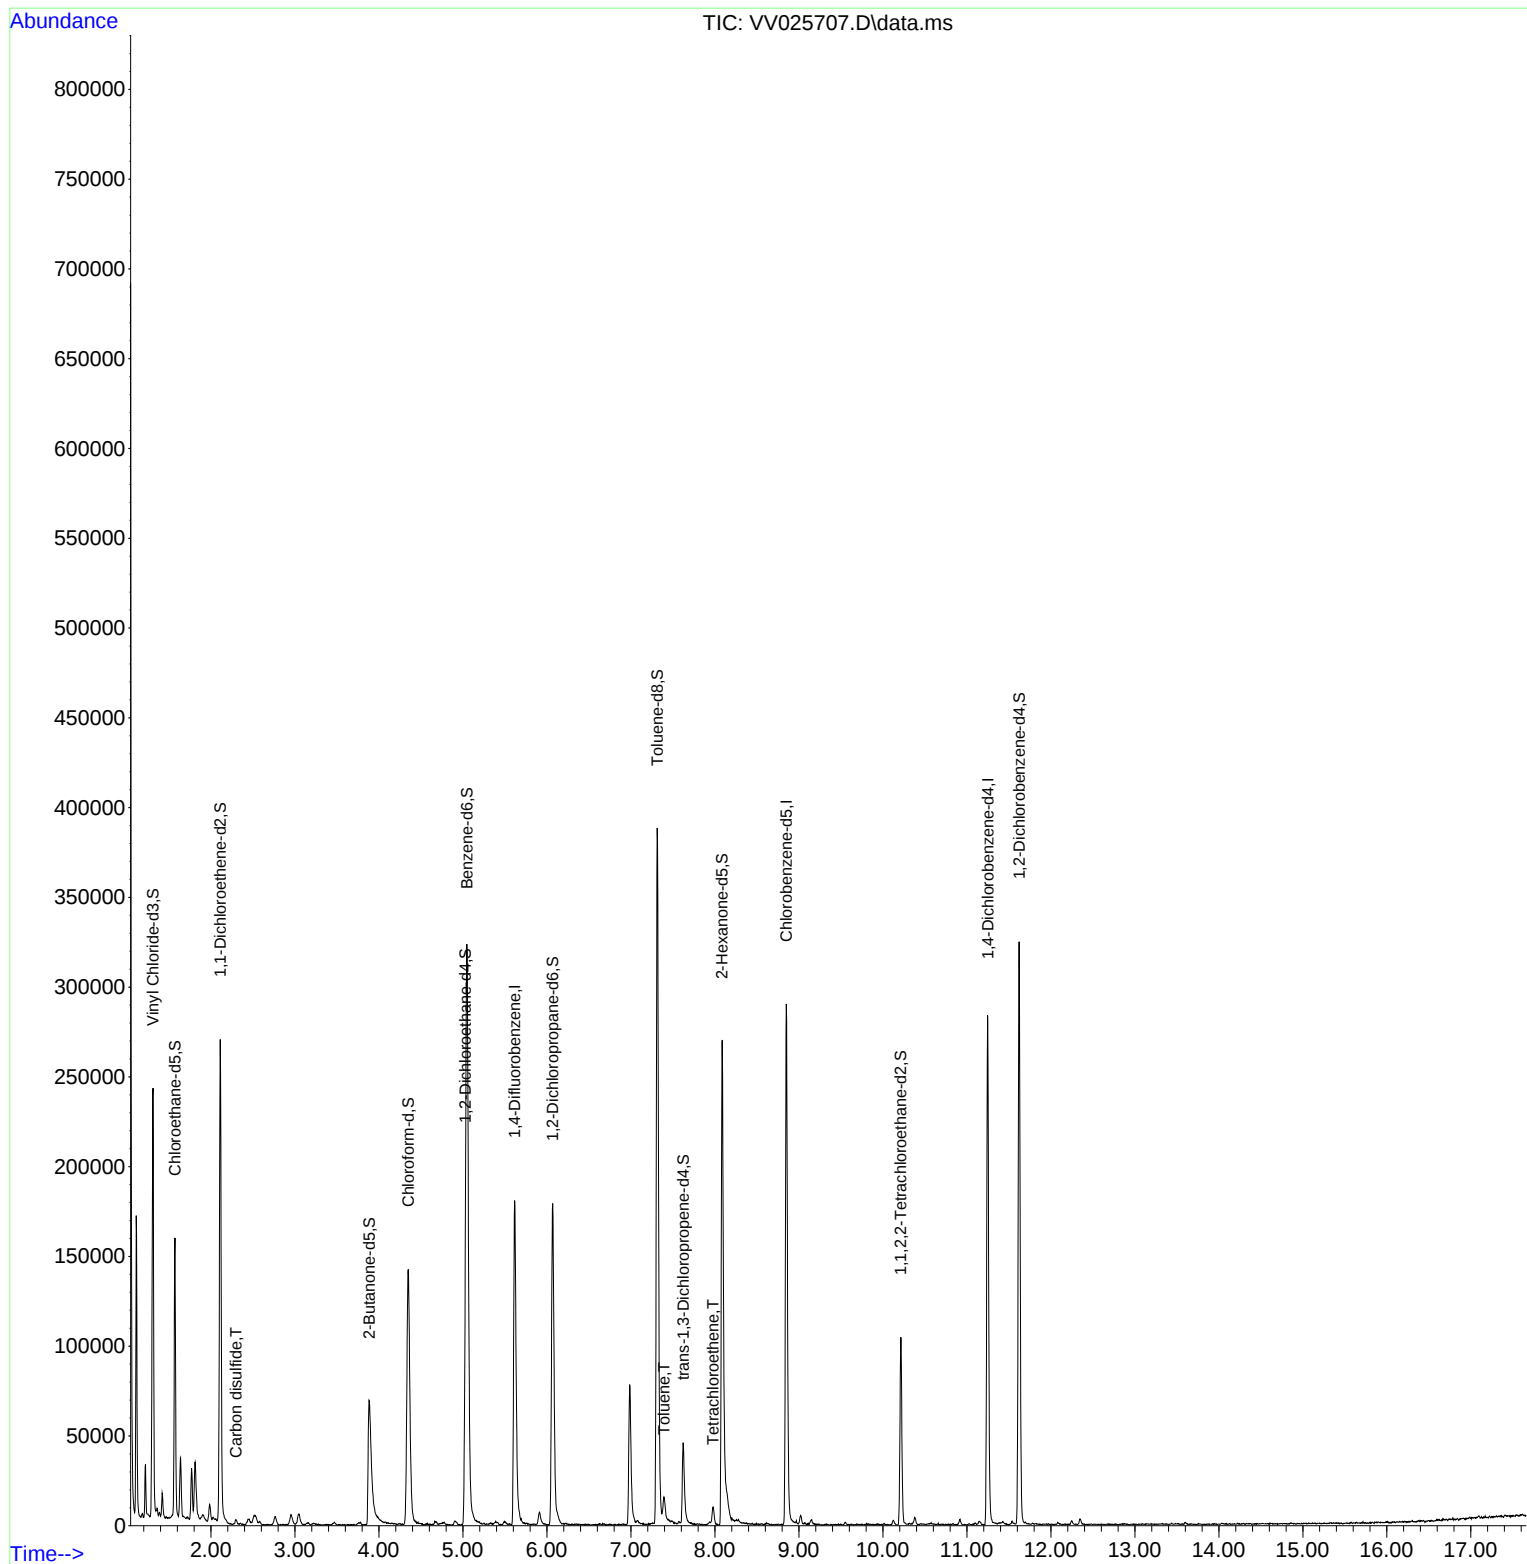



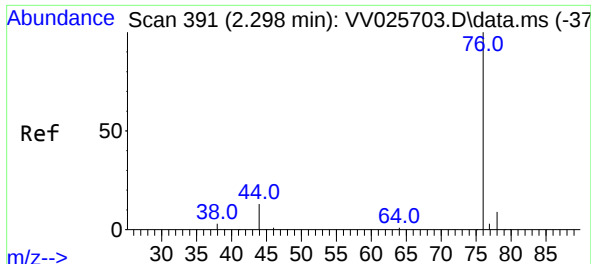


#14
Carbon disulfide
Concen: 0.097 ug/L
RT: 2.298 min Scan# 391
Delta R.T. -0.000 min
Lab File: VV025707.D
Acq: 25 Apr 2022 11:29

Instrument :
MSVOA_V
ClientSampleId :
EW6X1



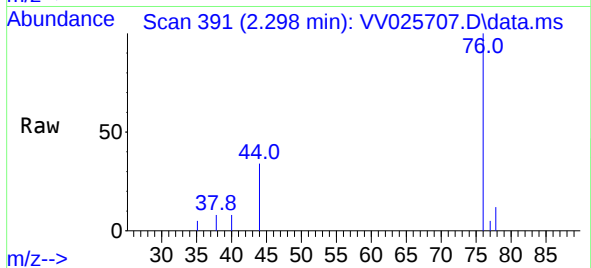



Tgt Ion: 76 Resp: 3136
Ion Ratio Lower Upper
76 100
78 12.0 7.3 10.9#

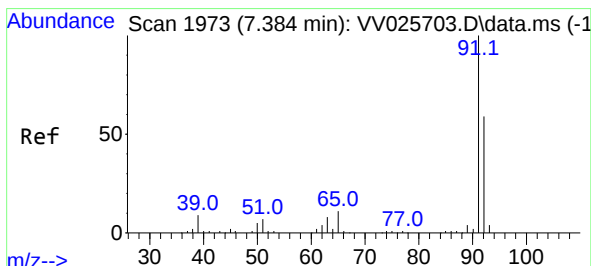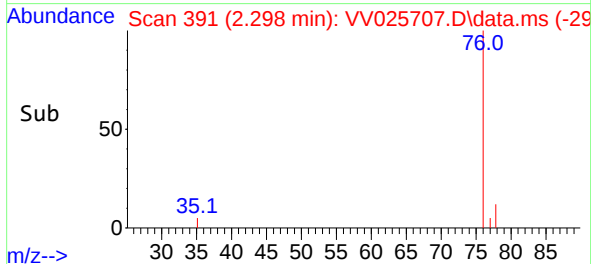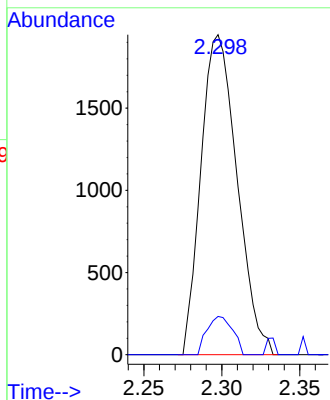

#42
Toluene
Concen: 0.209 ug/L
RT: 7.394 min Scan# 1976
Delta R.T. 0.010 min
Lab File: VV025707.D
Acq: 25 Apr 2022 11:29


Tgt Ion: 91 Resp: 10830
Ion Ratio Lower Upper
91 100
92 62.4 40.8 75.8

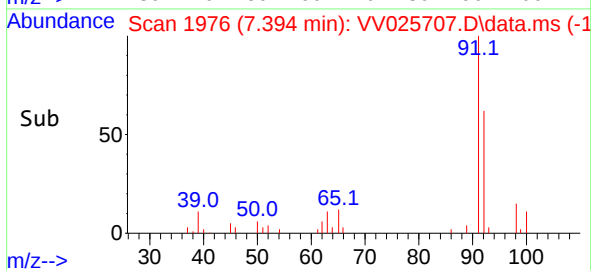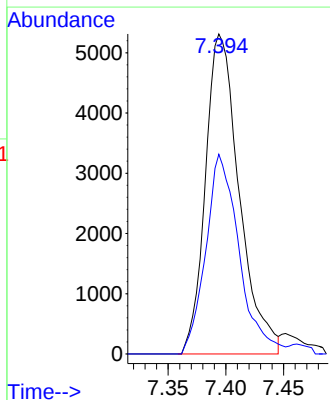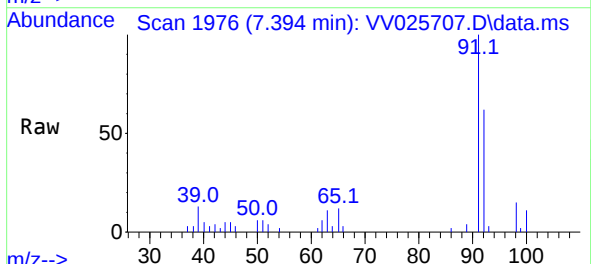

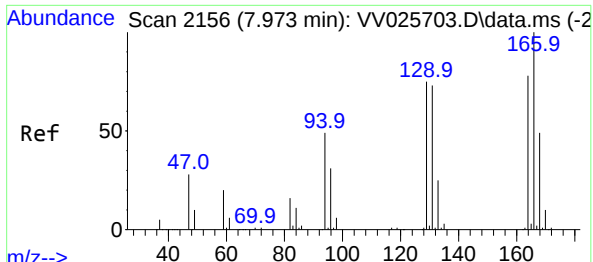

#47
 Tetrachloroethene
 Concen: 0.238 ug/L
 RT: 7.979 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VV025707.D
 Acq: 25 Apr 2022 11:29

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X1

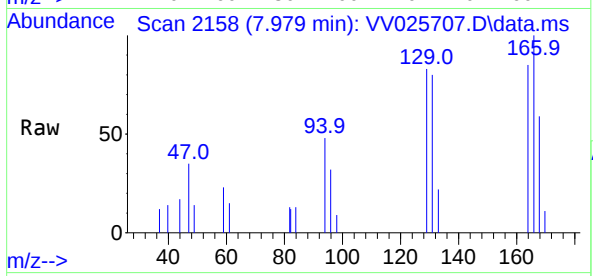

Tgt Ion:164 Resp: 2350

Ion	Ratio	Lower	Upper
164	100		
129	97.9	66.8	124.2
131	93.6	66.4	123.4
166	117.5	91.7	170.3

