

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042522\
 Data File : VW025709.D
 Acq On : 25 Apr 2022 12:16
 Operator : SY/MD
 Sample : N2530-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X4

Quant Time: Apr 26 06:34:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 26 06:32:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	159926	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	163478	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73243	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	76780	5.164	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.200%
7) Chloroethane-d5	1.571	69	75259	4.758	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.200%
11) 1,1-Dichloroethene-d2	2.111	63	115036	3.862	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.200%
20) 2-Butanone-d5	3.889	46	100345	55.482	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.960%
24) Chloroform-d	4.352	84	120989	5.385	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.600%
26) 1,2-Dichloroethane-d4	5.034	65	55506	5.734	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.600%
32) Benzene-d6	5.050	84	241845	5.113	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.200%
36) 1,2-Dichloropropane-d6	6.069	67	71872	5.448	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.000%
41) Toluene-d8	7.317	98	201974	4.601	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	7.625	79	20893	4.712	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.200%
46) 2-Hexanone-d5	8.088	63	75354	48.424	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.840%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	42604	5.112	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	65986	5.373	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.400%
Target Compounds						Qvalue
14) Carbon disulfide	2.298	76	3586	0.108	ug/L	97
47) Tetrachloroethene	7.979	164	2088	0.208	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025709.D
Acq On : 25 Apr 2022 12:16
Operator : SY/MD
Sample : N2530-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X4

Quant Time: Apr 26 06:34:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 26 06:32:17 2022
Response via : Initial Calibration




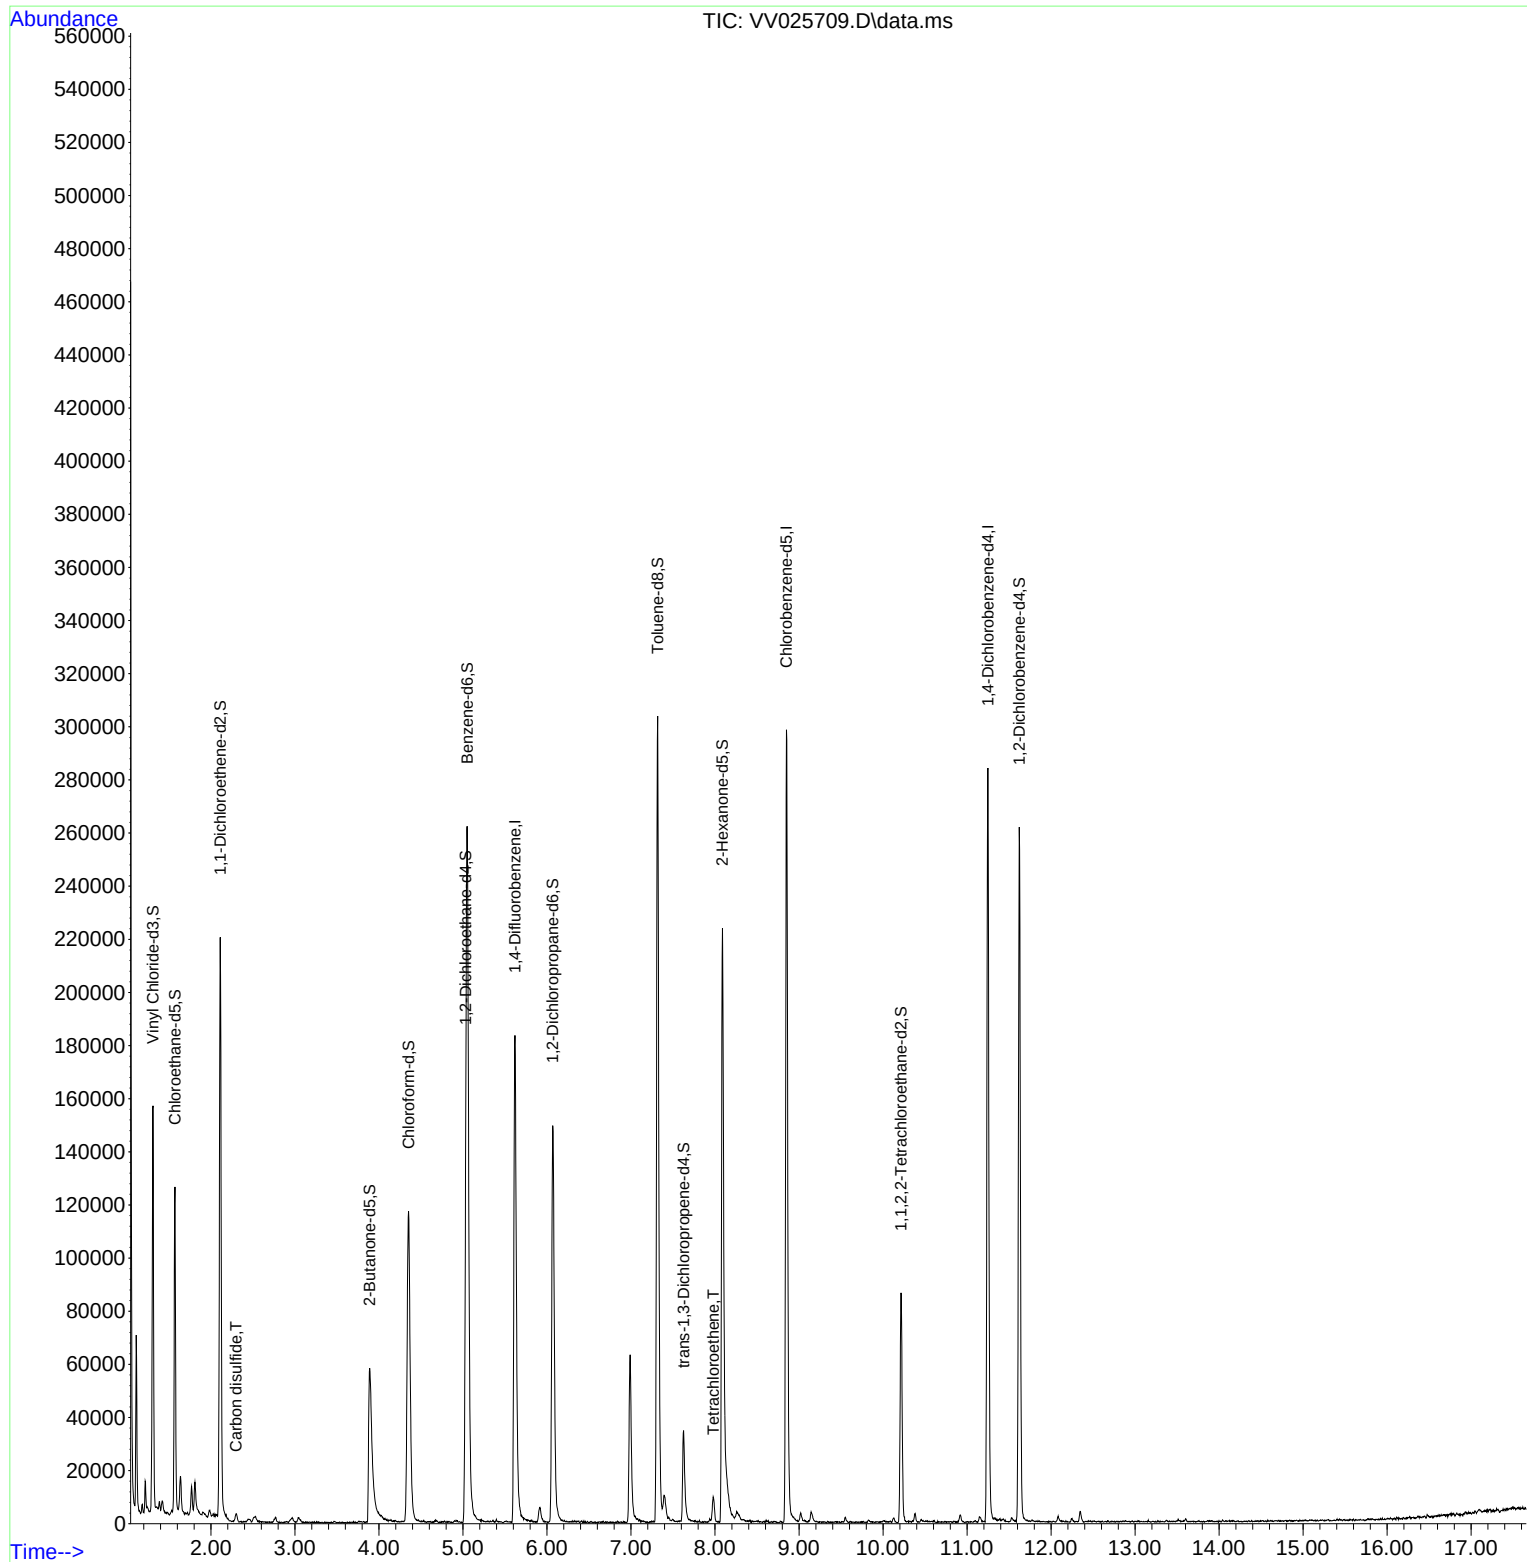


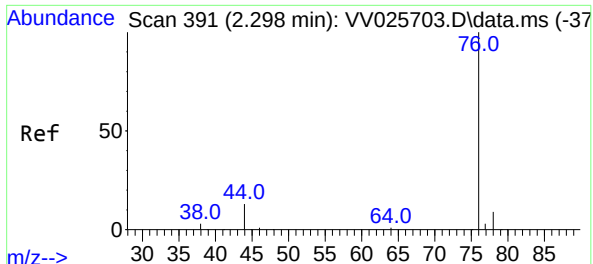

#14
Carbon disulfide
Concen: 0.108 ug/L
RT: 2.298 min Scan# 391
Delta R.T. -0.000 min
Lab File: VV025709.D
Acq: 25 Apr 2022 12:16

Instrument :
MSVOA_V
ClientSampleId :
EW6X4

Tgt Ion: 76 Resp: 3586
Ion Ratio Lower Upper
76 100
78 10.3 7.3 10.9

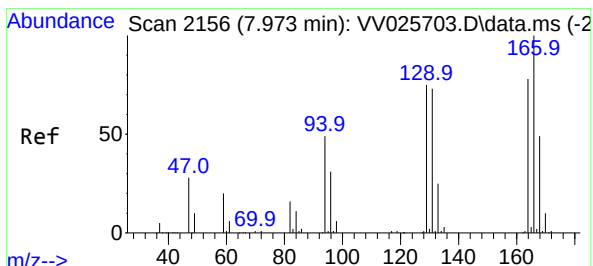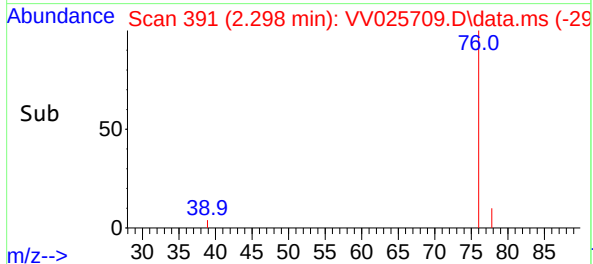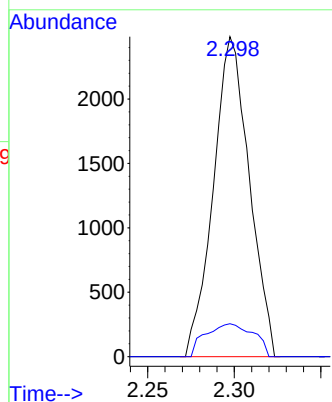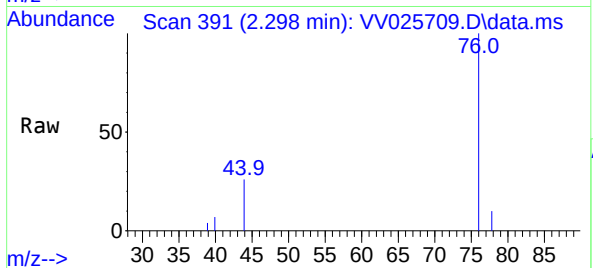

#47
Tetrachloroethene
Concen: 0.208 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. 0.006 min
Lab File: VV025709.D
Acq: 25 Apr 2022 12:16

Tgt Ion:164 Resp: 2088
Ion Ratio Lower Upper
164 100
129 86.4 66.8 124.2
131 97.2 66.4 123.4
166 142.8 91.7 170.3

