

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042522\
 Data File : VW025712.D
 Acq On : 25 Apr 2022 13:27
 Operator : SY/MD
 Sample : N2492-04DL 500X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T6DL

Quant Time: Apr 26 06:34:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 26 06:32:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	150248	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	152620	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69057	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	63567	4.551	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.000%	
7) Chloroethane-d5	1.571	69	57494	3.869	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	77.400%	
11) 1,1-Dichloroethene-d2	2.111	63	93766	3.351	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.000%	
20) 2-Butanone-d5	3.905	46	76891	45.253	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	90.500%	
24) Chloroform-d	4.352	84	95166	4.508	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.200%	
26) 1,2-Dichloroethane-d4	5.037	65	42398	4.662	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.200%	
32) Benzene-d6	5.053	84	185444	4.199	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.000%	
36) 1,2-Dichloropropane-d6	6.072	67	55171	4.480	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.600%	
41) Toluene-d8	7.317	98	155745	3.801	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.000%	
43) trans-1,3-Dichloroprop...	7.625	79	15726	3.799	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	76.000%	
46) 2-Hexanone-d5	8.088	63	54942	37.818	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	75.640%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32406	4.165	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	83.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	51345	4.435	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	88.600%	
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.976	164	15550	1.659	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025712.D
Acq On : 25 Apr 2022 13:27
Operator : SY/MD
Sample : N2492-04DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Quant Time: Apr 26 06:34:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 26 06:32:17 2022
Response via : Initial Calibration

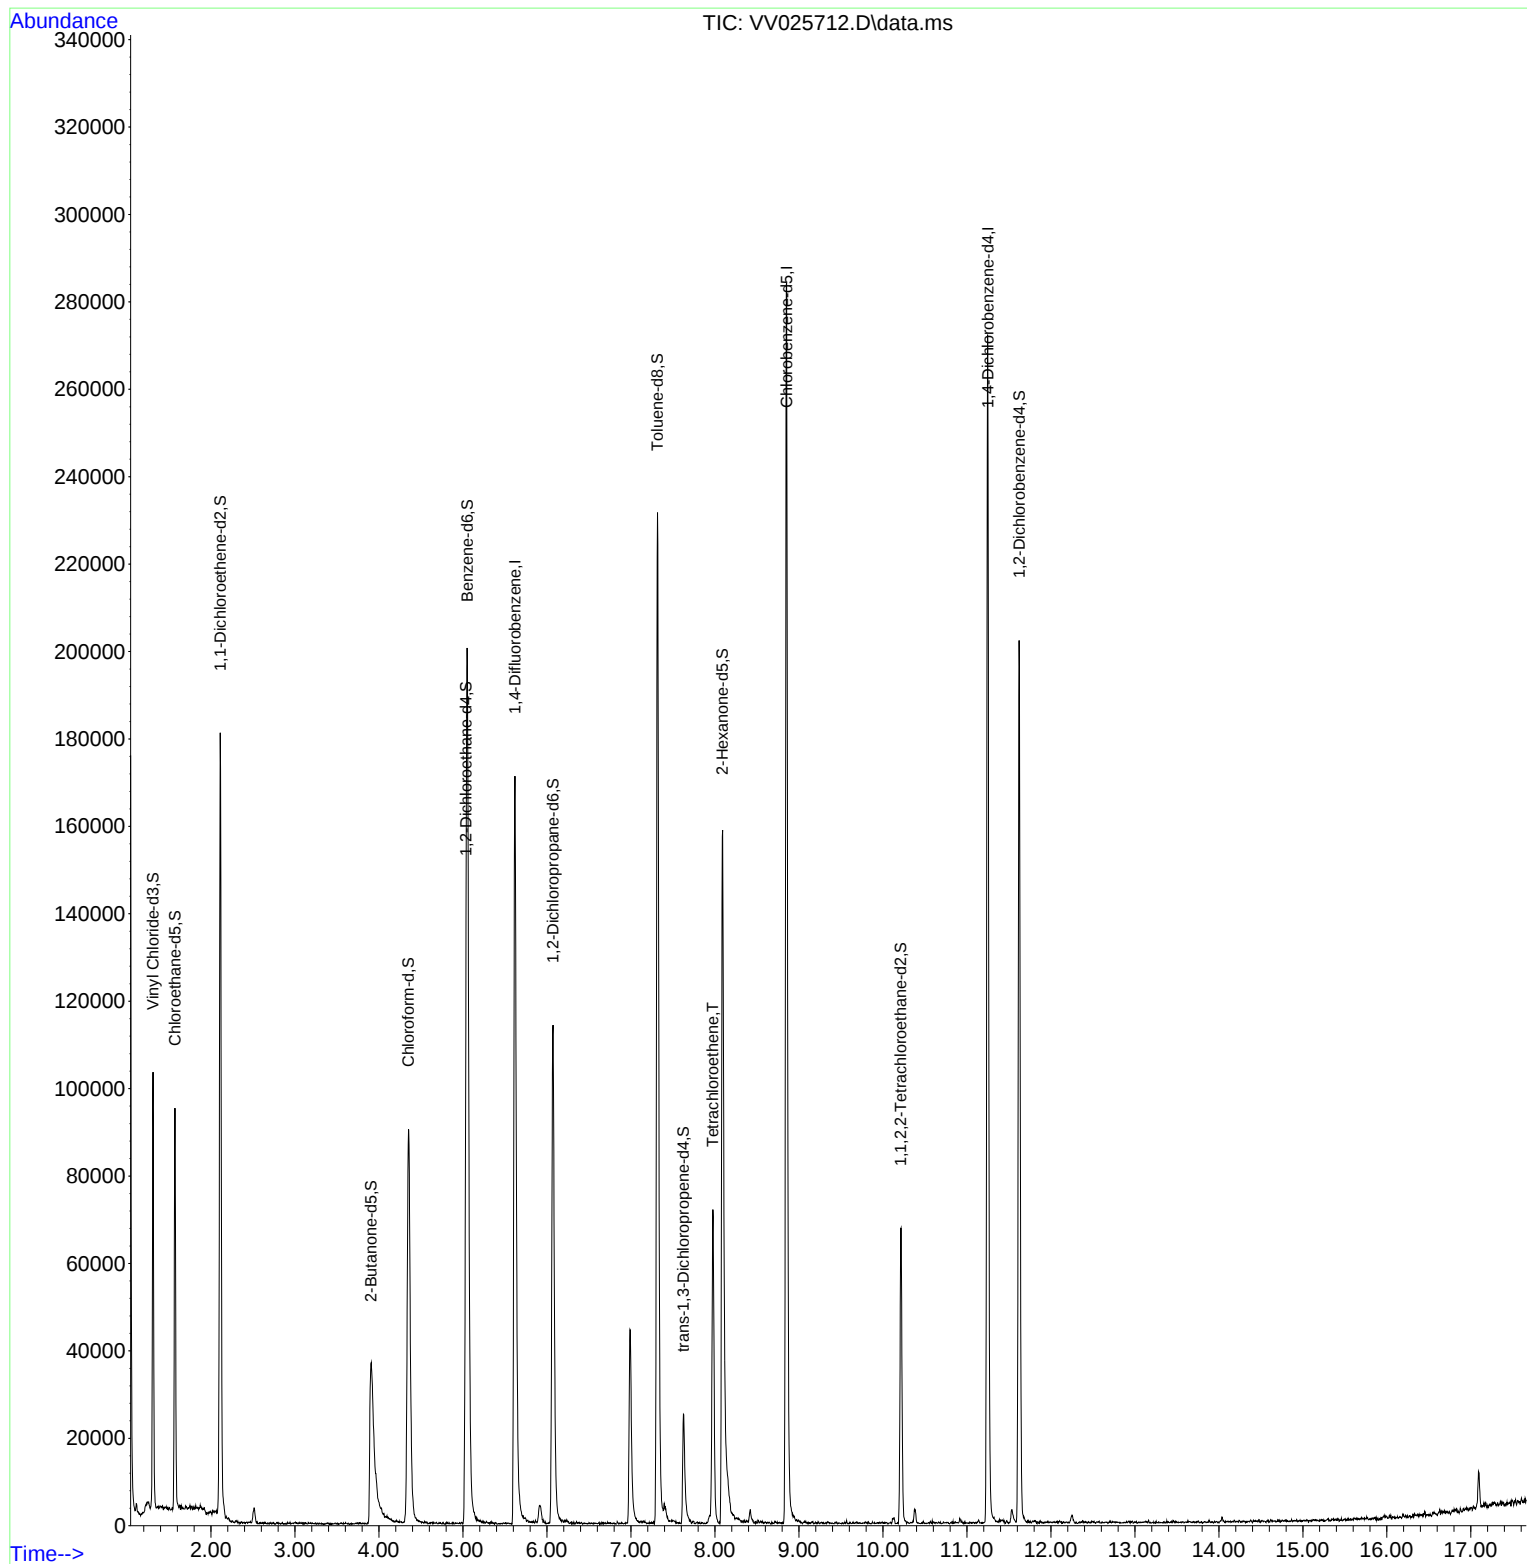

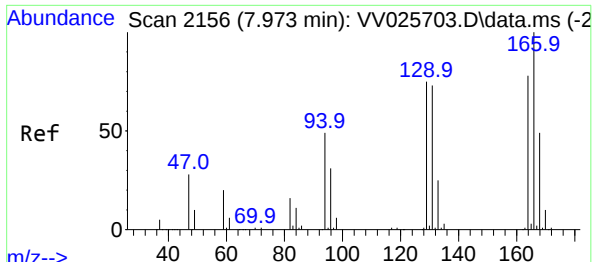

#47
Tetrachloroethene
Concen: 1.659 ug/L
RT: 7.976 min Scan# 2156
Delta R.T. 0.003 min
Lab File: VV025712.D
Acq: 25 Apr 2022 13:27

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Tgt Ion:164 Resp: 15550

Ion	Ratio	Lower	Upper
164	100		
129	94.0	66.8	124.2
131	97.3	66.4	123.4
166	125.6	91.7	170.3

