

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042522\
 Data File : VW025714.D
 Acq On : 25 Apr 2022 14:20
 Operator : SY/MD
 Sample : N2492-16DL 50X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W4DL

Quant Time: Apr 26 06:35:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 26 06:32:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	167099	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	170730	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	78003	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	85014	5.472	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.400%
7) Chloroethane-d5	1.571	69	81939	4.958	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.200%
11) 1,1-Dichloroethene-d2	2.111	63	128395	4.126	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%
20) 2-Butanone-d5	3.889	46	109734	58.069	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.140%
24) Chloroform-d	4.352	84	131254	5.591	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.800%
26) 1,2-Dichloroethane-d4	5.034	65	61085	6.039	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.800%
32) Benzene-d6	5.050	84	261524	5.294	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.800%
36) 1,2-Dichloropropane-d6	6.069	67	76994	5.589	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.800%
41) Toluene-d8	7.317	98	221427	4.830	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
43) trans-1,3-Dichloroprop...	7.625	79	22364	4.830	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.600%
46) 2-Hexanone-d5	8.088	63	81486	50.140	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.280%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43837	5.037	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	72932	5.577	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.600%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.976	164	34385	3.280	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025714.D
Acq On : 25 Apr 2022 14:20
Operator : SY/MD
Sample : N2492-16DL 50X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W4DL

Quant Time: Apr 26 06:35:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 26 06:32:17 2022
Response via : Initial Calibration

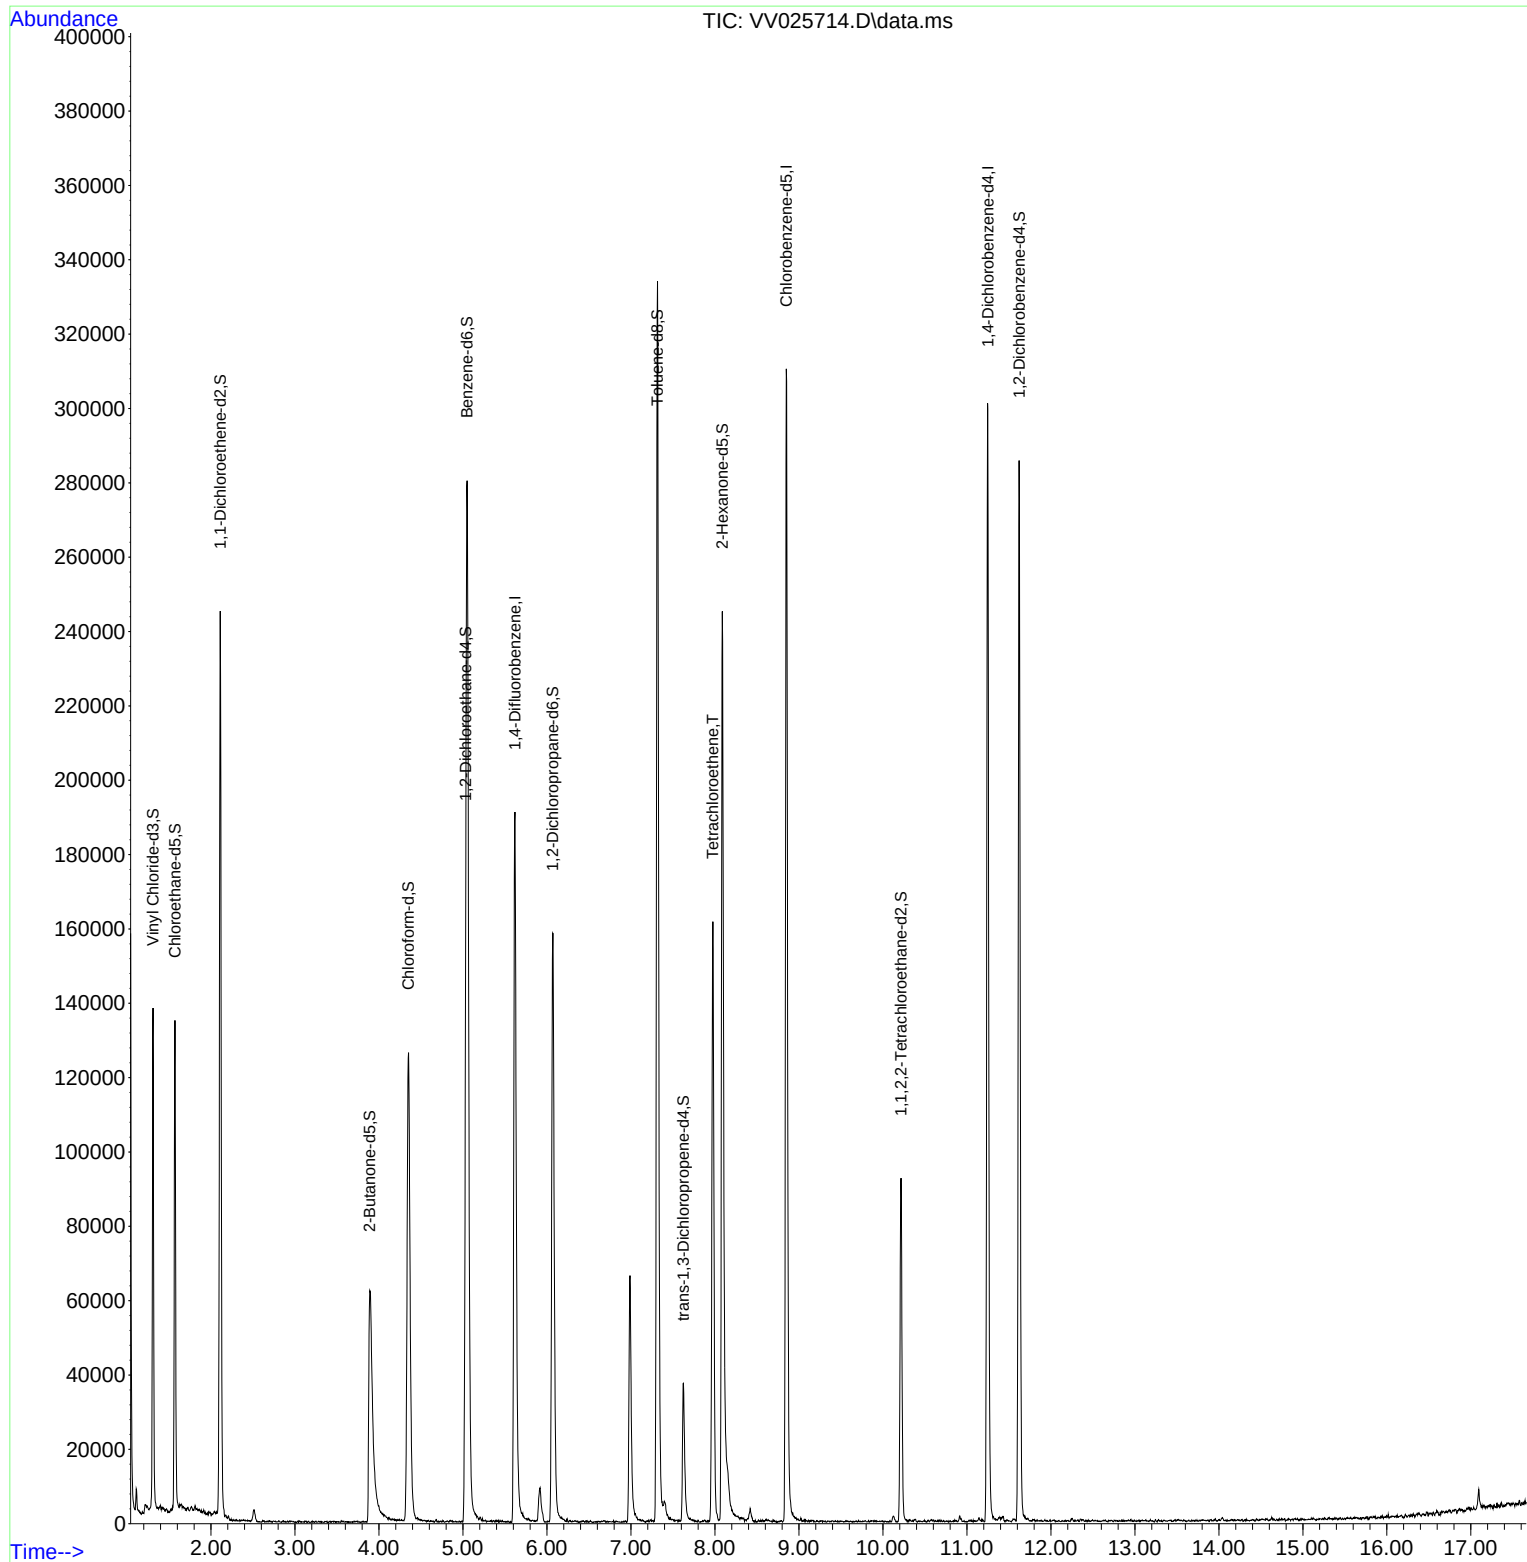

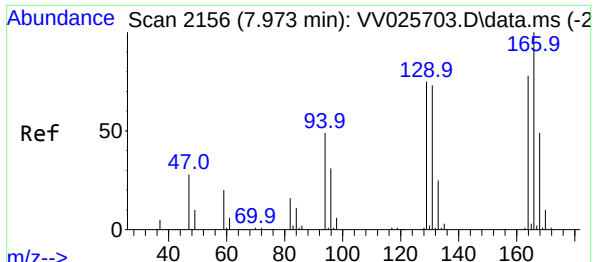

#47
 Tetrachloroethene
 Concen: 3.280 ug/L
 RT: 7.976 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV025714.D
 Acq: 25 Apr 2022 14:20

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W4DL

Tgt Ion:164 Resp: 34385

Ion	Ratio	Lower	Upper
164	100		
129	98.1	66.8	124.2
131	94.2	66.4	123.4
166	134.3	91.7	170.3

