

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042522\
 Data File : VW025715.D
 Acq On : 25 Apr 2022 14:44
 Operator : SY/MD
 Sample : N2492-17DL 400X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W5DL

Quant Time: Apr 26 06:35:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 26 06:32:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	131228	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	134764	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59522	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	61969	5.079	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.600%
7) Chloroethane-d5	1.571	69	62220	4.794	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.800%
11) 1,1-Dichloroethene-d2	2.111	63	93766	3.837	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.800%
20) 2-Butanone-d5	3.892	46	81539	54.943	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.880%
24) Chloroform-d	4.355	84	98434	5.339	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.800%
26) 1,2-Dichloroethane-d4	5.037	65	44773	5.636	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.800%
32) Benzene-d6	5.053	84	193673	4.967	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
36) 1,2-Dichloropropane-d6	6.069	67	58808	5.408	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.200%
41) Toluene-d8	7.317	98	162877	4.501	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%
43) trans-1,3-Dichloroprop...	7.625	79	16512	4.518	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%
46) 2-Hexanone-d5	8.088	63	58225	45.389	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.780%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32746	4.766	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	50945	5.105	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	35270	4.262	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025715.D
Acq On : 25 Apr 2022 14:44
Operator : SY/MD
Sample : N2492-17DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W5DL


Quant Time: Apr 26 06:35:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 26 06:32:17 2022
Response via : Initial Calibration

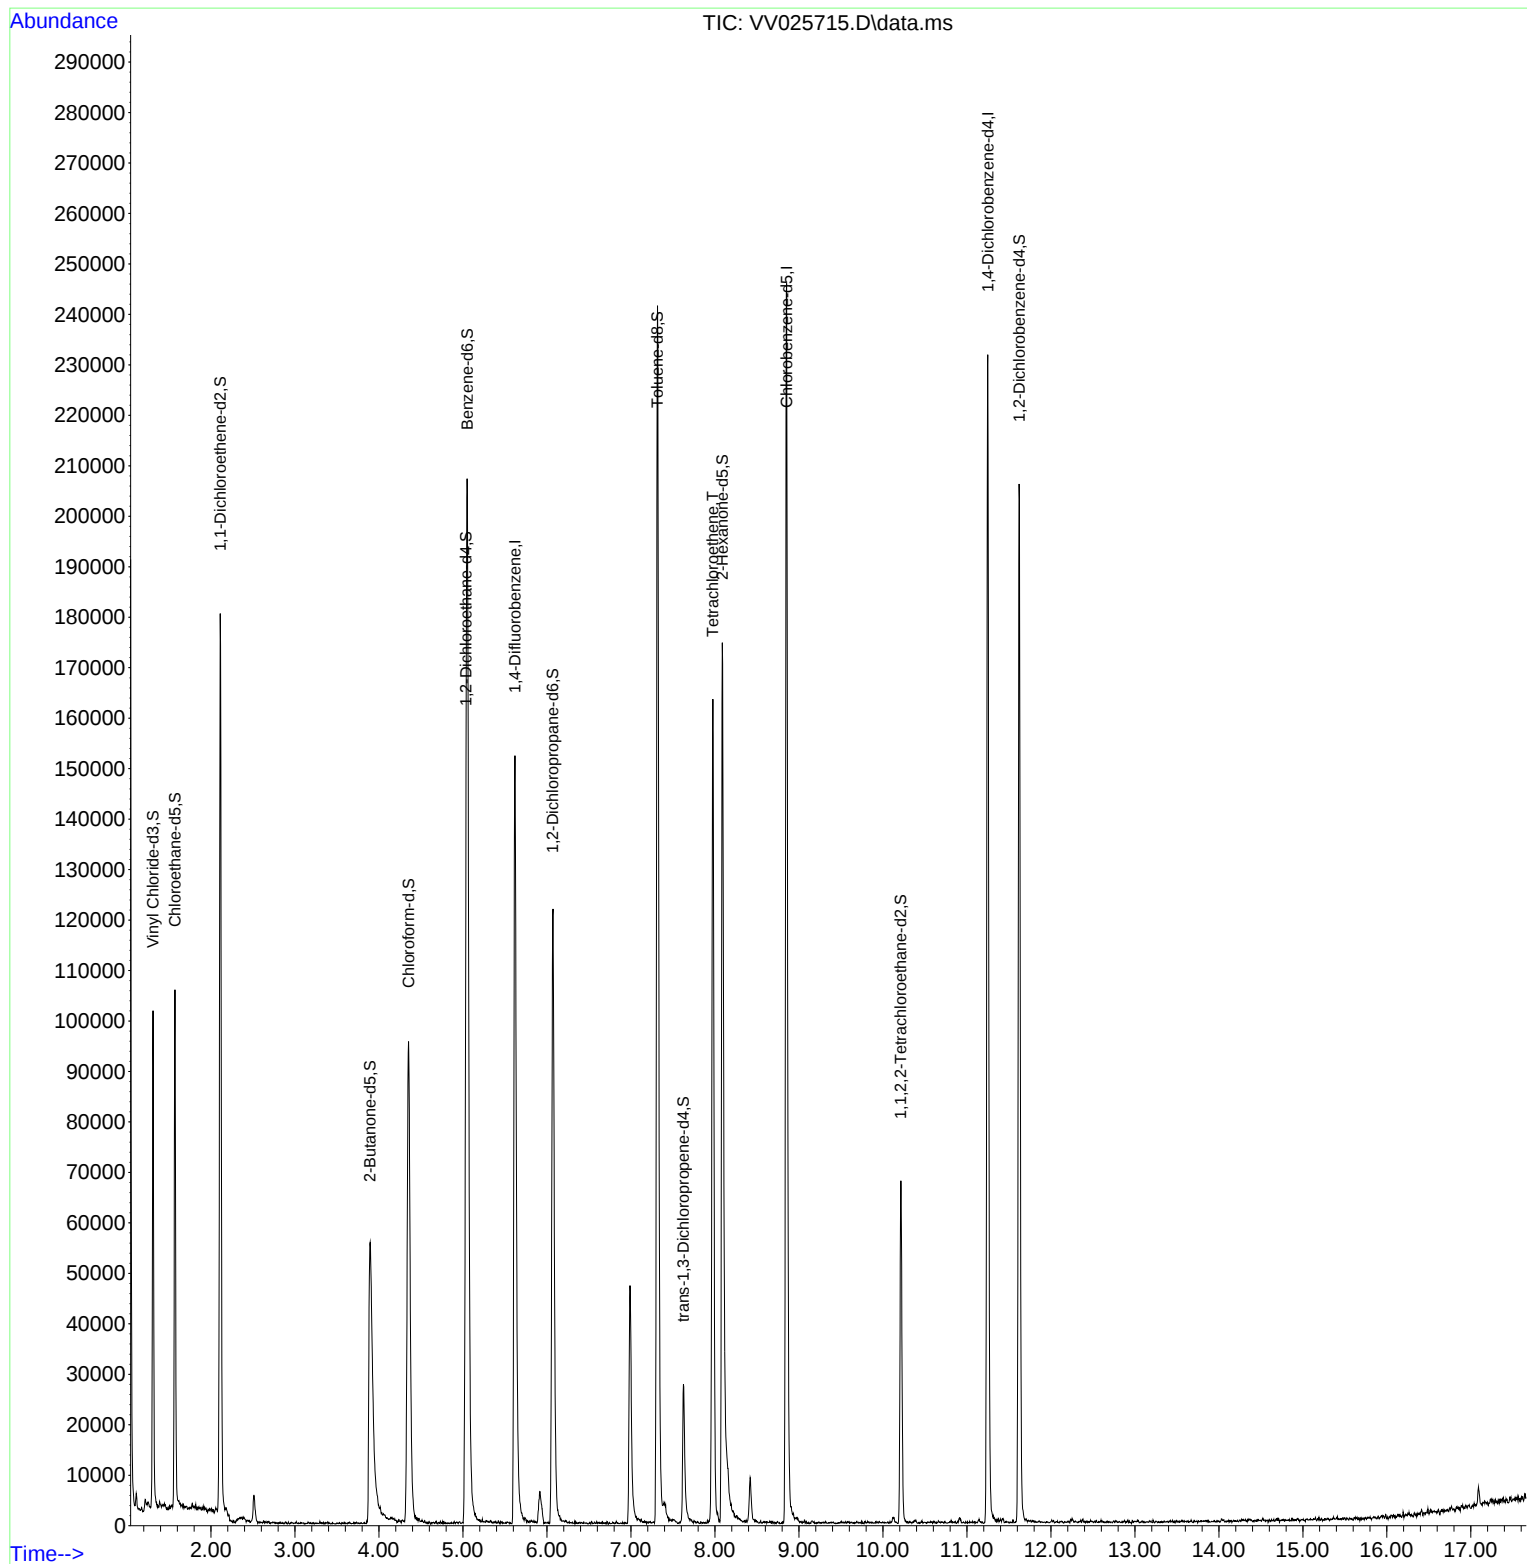

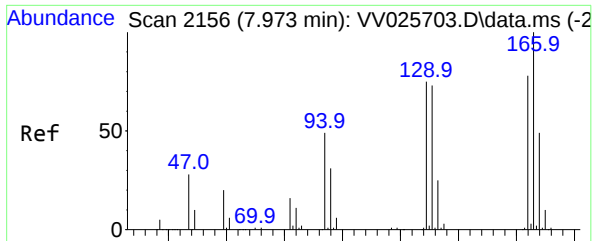

#47
Tetrachloroethene
Concen: 4.262 ug/L
RT: 7.976 min Scan# 2156
Delta R.T. 0.003 min
Lab File: VV025715.D
Acq: 25 Apr 2022 14:44

Instrument :
MSVOA_V
ClientSampleId :
EW6W5DL

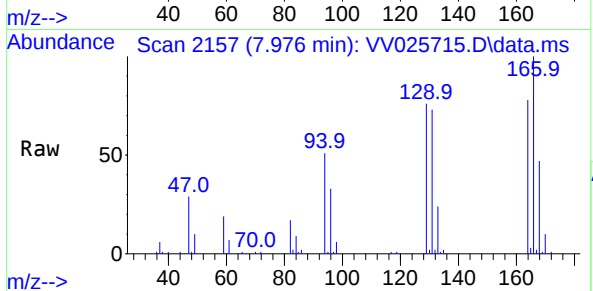

Tgt Ion:164 Resp: 35270

Ion	Ratio	Lower	Upper
164	100		
129	97.2	66.8	124.2
131	93.1	66.4	123.4
166	127.8	91.7	170.3

