

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042522\
 Data File : VW025716.D
 Acq On : 25 Apr 2022 15:07
 Operator : SY/MD
 Sample : N2492-18DL 400X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W6DL

Quant Time: Apr 26 06:35:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 26 06:32:17 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	130013	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	131959	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58840	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	65909	5.453	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 109.000%		
7) Chloroethane-d5	1.571	69	68438	5.322	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 106.400%		
11) 1,1-Dichloroethene-d2	2.111	63	101457	4.190	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 83.800%		
20) 2-Butanone-d5	3.892	46	86937	59.128	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 118.260%		
24) Chloroform-d	4.352	84	105624	5.783	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 115.600%		
26) 1,2-Dichloroethane-d4	5.034	65	47986	6.097	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 122.000%		
32) Benzene-d6	5.053	84	207326	5.430	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 108.600%		
36) 1,2-Dichloropropane-d6	6.069	67	60297	5.663	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 113.200%		
41) Toluene-d8	7.317	98	174302	4.919	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 98.400%		
43) trans-1,3-Dichloroprop...	7.625	79	17510	4.892	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 97.800%		
46) 2-Hexanone-d5	8.088	63	60774	48.383	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 96.760%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35376	5.259	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 105.200%		
66) 1,2-Dichlorobenzene-d4	11.622	152	55977	5.674	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 113.400%		
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	28867	3.563	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025716.D
Acq On : 25 Apr 2022 15:07
Operator : SY/MD
Sample : N2492-18DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W6DL

Quant Time: Apr 26 06:35:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 26 06:32:17 2022
Response via : Initial Calibration

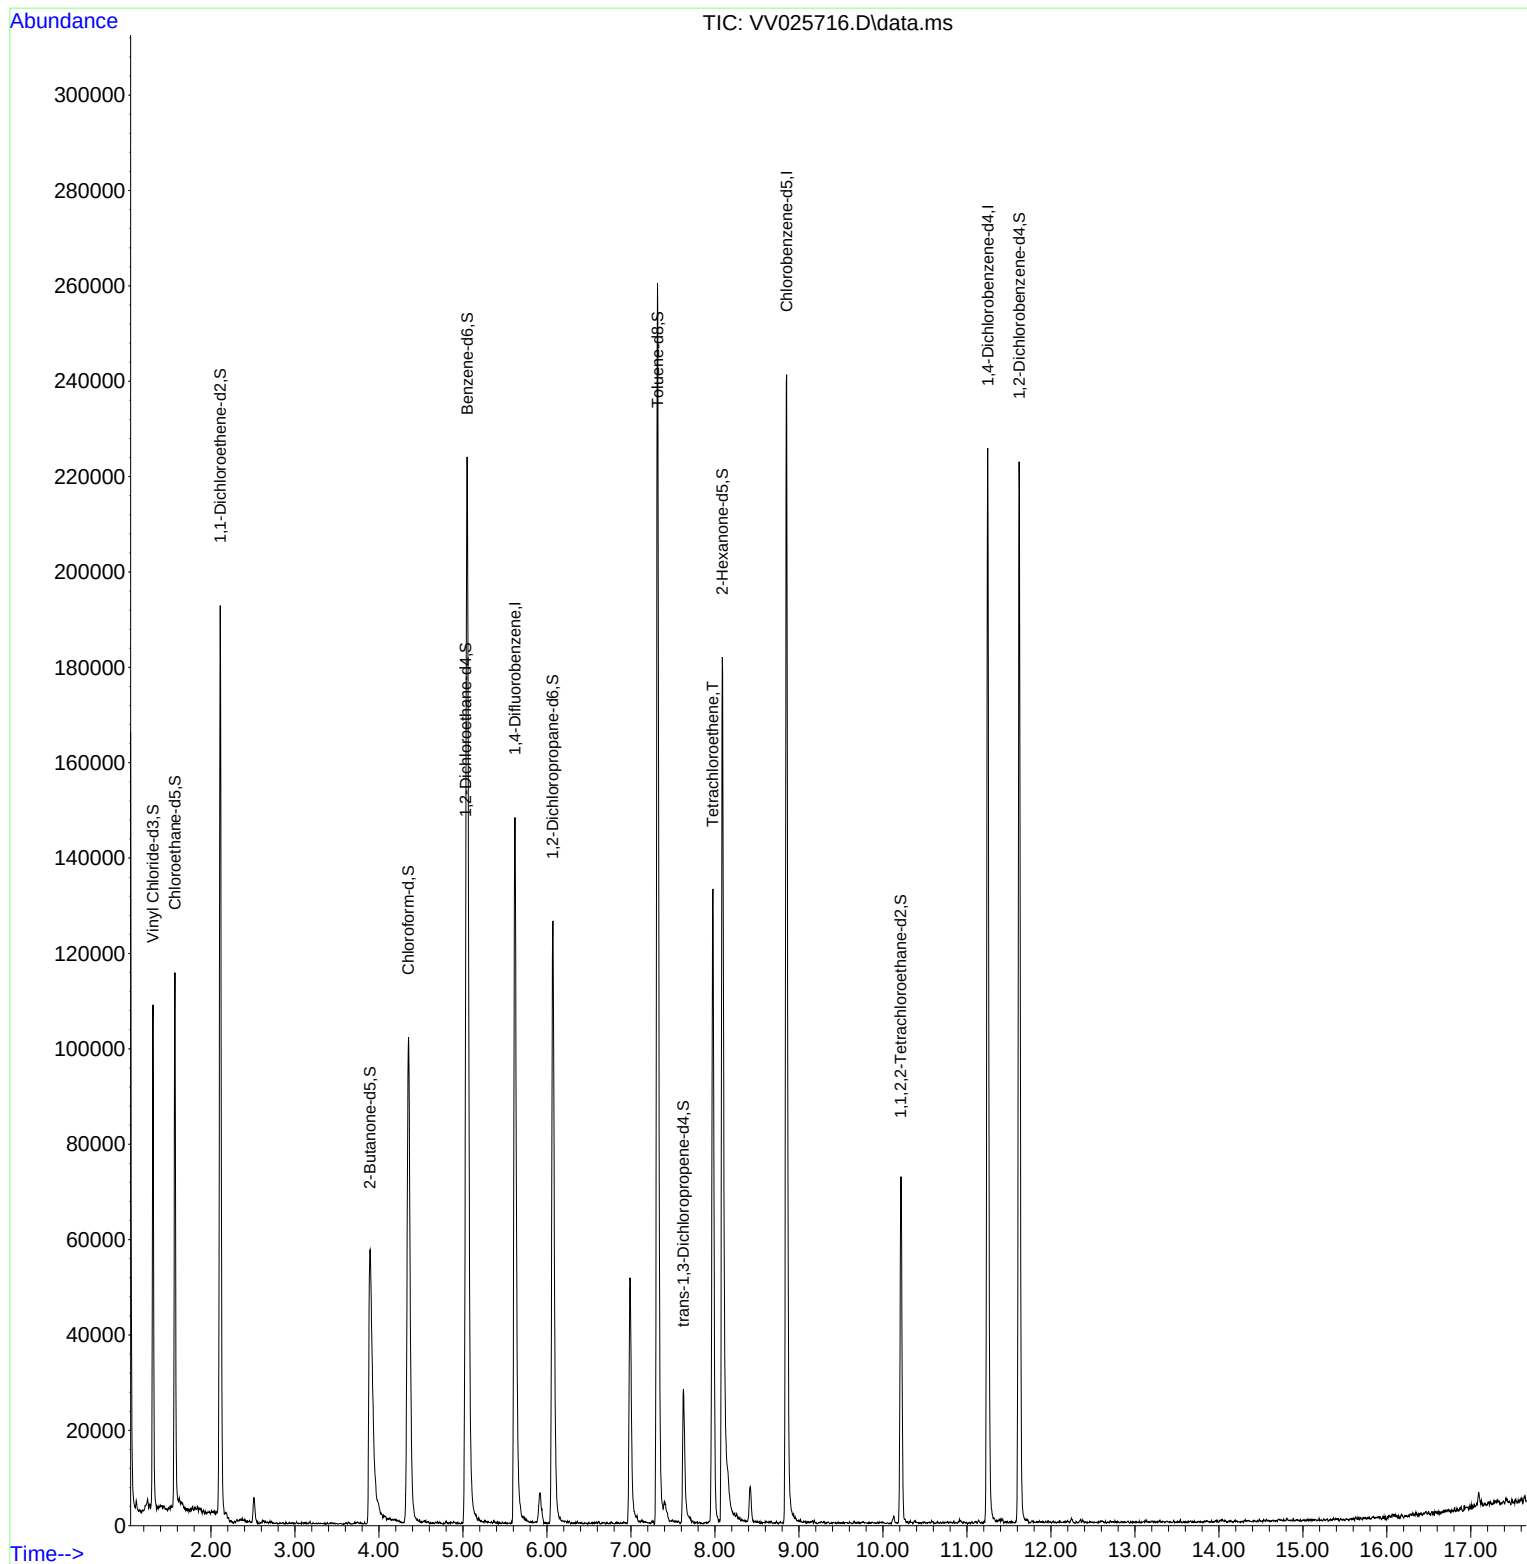


Abundance Scan 2156 (7.973 min): VV025703.D\data.ms (-2

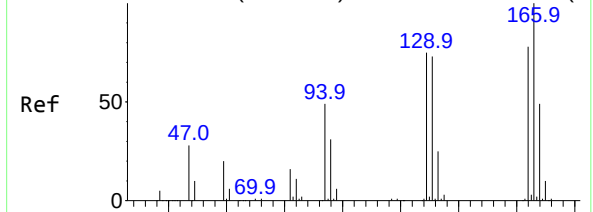

Abundance Scan 2157 (7.976 min): VV025716.D\data.ms



Abundance Scan 2157 (7.976 min): VV025716.D\data.ms (-2

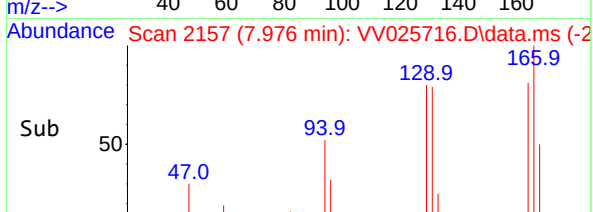

#47

Tetrachloroethene

Concen: 3.563 ug/L

RT: 7.976 min Scan# 21

Delta R.T. 0.003 min

Lab File: VV025716.D

Acq: 25 Apr 2022 15:07

Instrument :

MSVOA_V

ClientSampleId :

EW6W6DL

Tgt Ion:164 Resp: 28867

Ion Ratio Lower Upper

164 100

129 98.8 66.8 124.2

131 97.0 66.4 123.4

166 123.3 91.7 170.3

