

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042522\
 Data File : VW025717.D
 Acq On : 25 Apr 2022 15:31
 Operator : SY/MD
 Sample : N2492-22DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W8DL

Quant Time: Apr 26 06:36:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 26 06:32:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123912	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	129961	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56423	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	64011	5.556	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	111.200%	
7) Chloroethane-d5	1.571	69	66490	5.425	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.600%	
11) 1,1-Dichloroethene-d2	2.111	63	98384	4.263	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	85.200%	
20) 2-Butanone-d5	3.892	46	83059	59.272	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	118.540%	
24) Chloroform-d	4.352	84	103880	5.967	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	119.400%	
26) 1,2-Dichloroethane-d4	5.037	65	48096	6.412	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	128.200%	
32) Benzene-d6	5.053	84	203259	5.405	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	108.200%	
36) 1,2-Dichloropropane-d6	6.072	67	61310	5.846	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	117.000%	
41) Toluene-d8	7.317	98	168109	4.818	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	7.625	79	17116	4.856	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.200%	
46) 2-Hexanone-d5	8.088	63	62328	50.383	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.760%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	36119	5.452	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	109.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	54077	5.716	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	114.400%	
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	60675	7.603	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025717.D
Acq On : 25 Apr 2022 15:31
Operator : SY/MD
Sample : N2492-22DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W8DL


Quant Time: Apr 26 06:36:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 26 06:32:17 2022
Response via : Initial Calibration

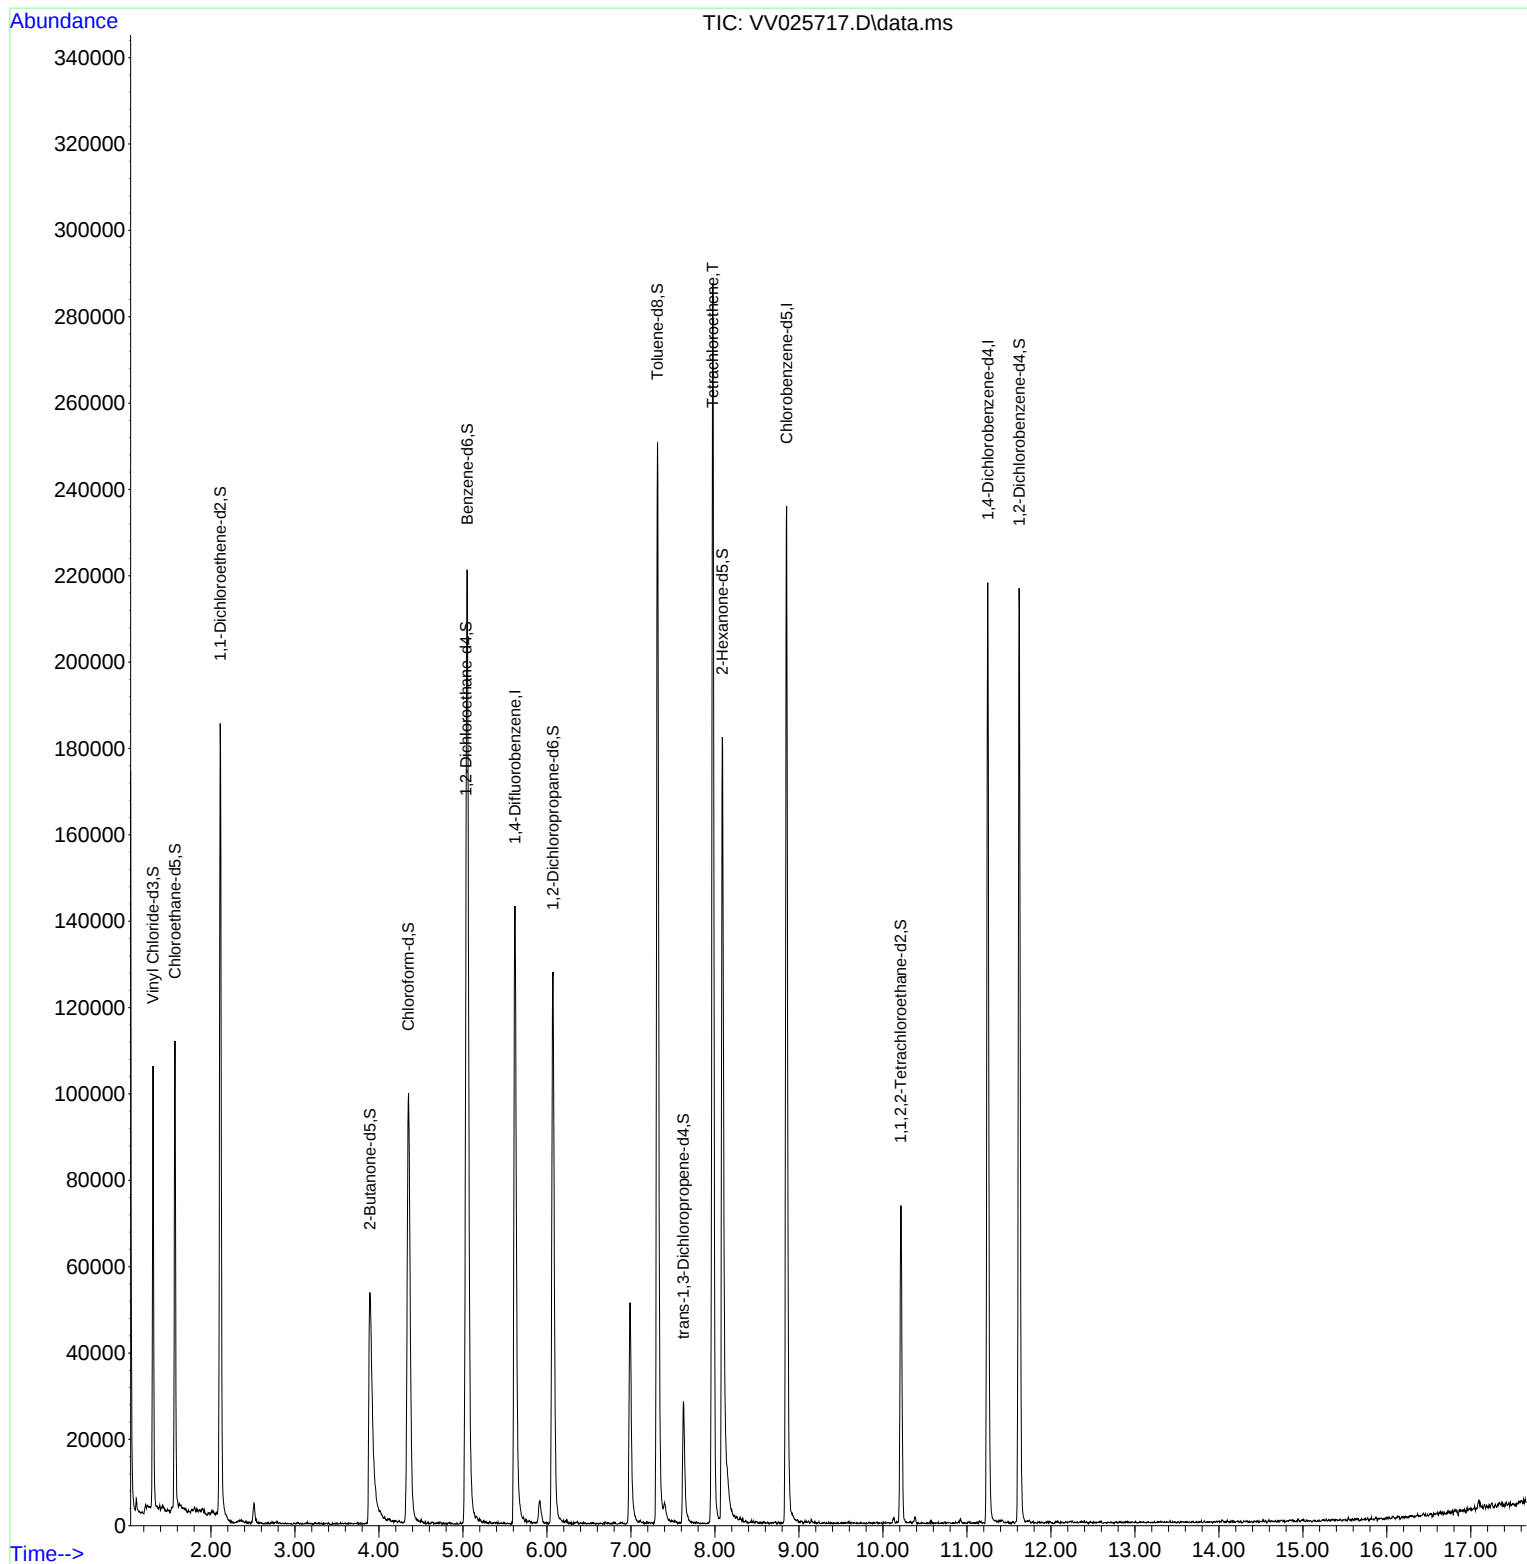

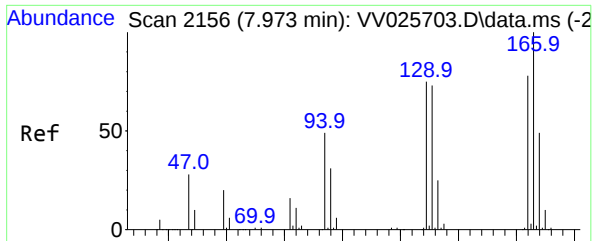

#47
 Tetrachloroethene
 Concen: 7.603 ug/L
 RT: 7.976 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV025717.D
 Acq: 25 Apr 2022 15:31

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W8DL

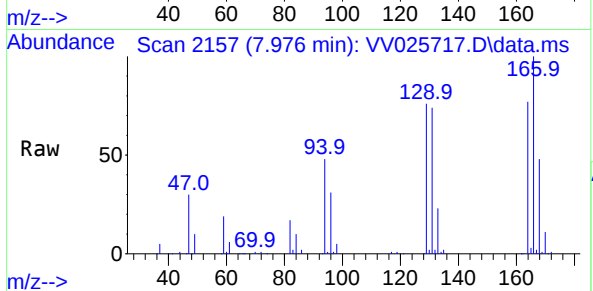

Tgt Ion:164 Resp: 60675

Ion	Ratio	Lower	Upper
164	100		
129	98.4	66.8	124.2
131	95.2	66.4	123.4
166	129.2	91.7	170.3

