

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042522\
 Data File : VW025718.D
 Acq On : 25 Apr 2022 15:54
 Operator : SY/MD
 Sample : N2492-23DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W9DL

Quant Time: Apr 26 06:36:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 26 06:32:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	186573	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	193428	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	84628	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	75864	4.374	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.400%
7) Chloroethane-d5	1.574	69	71272	3.862	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.200%
11) 1,1-Dichloroethene-d2	2.114	63	116442	3.351	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.000%
20) 2-Butanone-d5	3.902	46	103812	49.201	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.400%
24) Chloroform-d	4.352	84	124170	4.737	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	5.037	65	56970	5.044	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.800%
32) Benzene-d6	5.053	84	245227	4.382	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
36) 1,2-Dichloropropane-d6	6.069	67	73139	4.686	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.800%
41) Toluene-d8	7.317	98	206555	3.977	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	7.625	79	20759	3.957	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.088	63	75473	40.990	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.980%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42672	4.327	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	66043	4.655	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.000%
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	29291	2.466	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025718.D
Acq On : 25 Apr 2022 15:54
Operator : SY/MD
Sample : N2492-23DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W9DL


Quant Time: Apr 26 06:36:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 26 06:32:17 2022
Response via : Initial Calibration

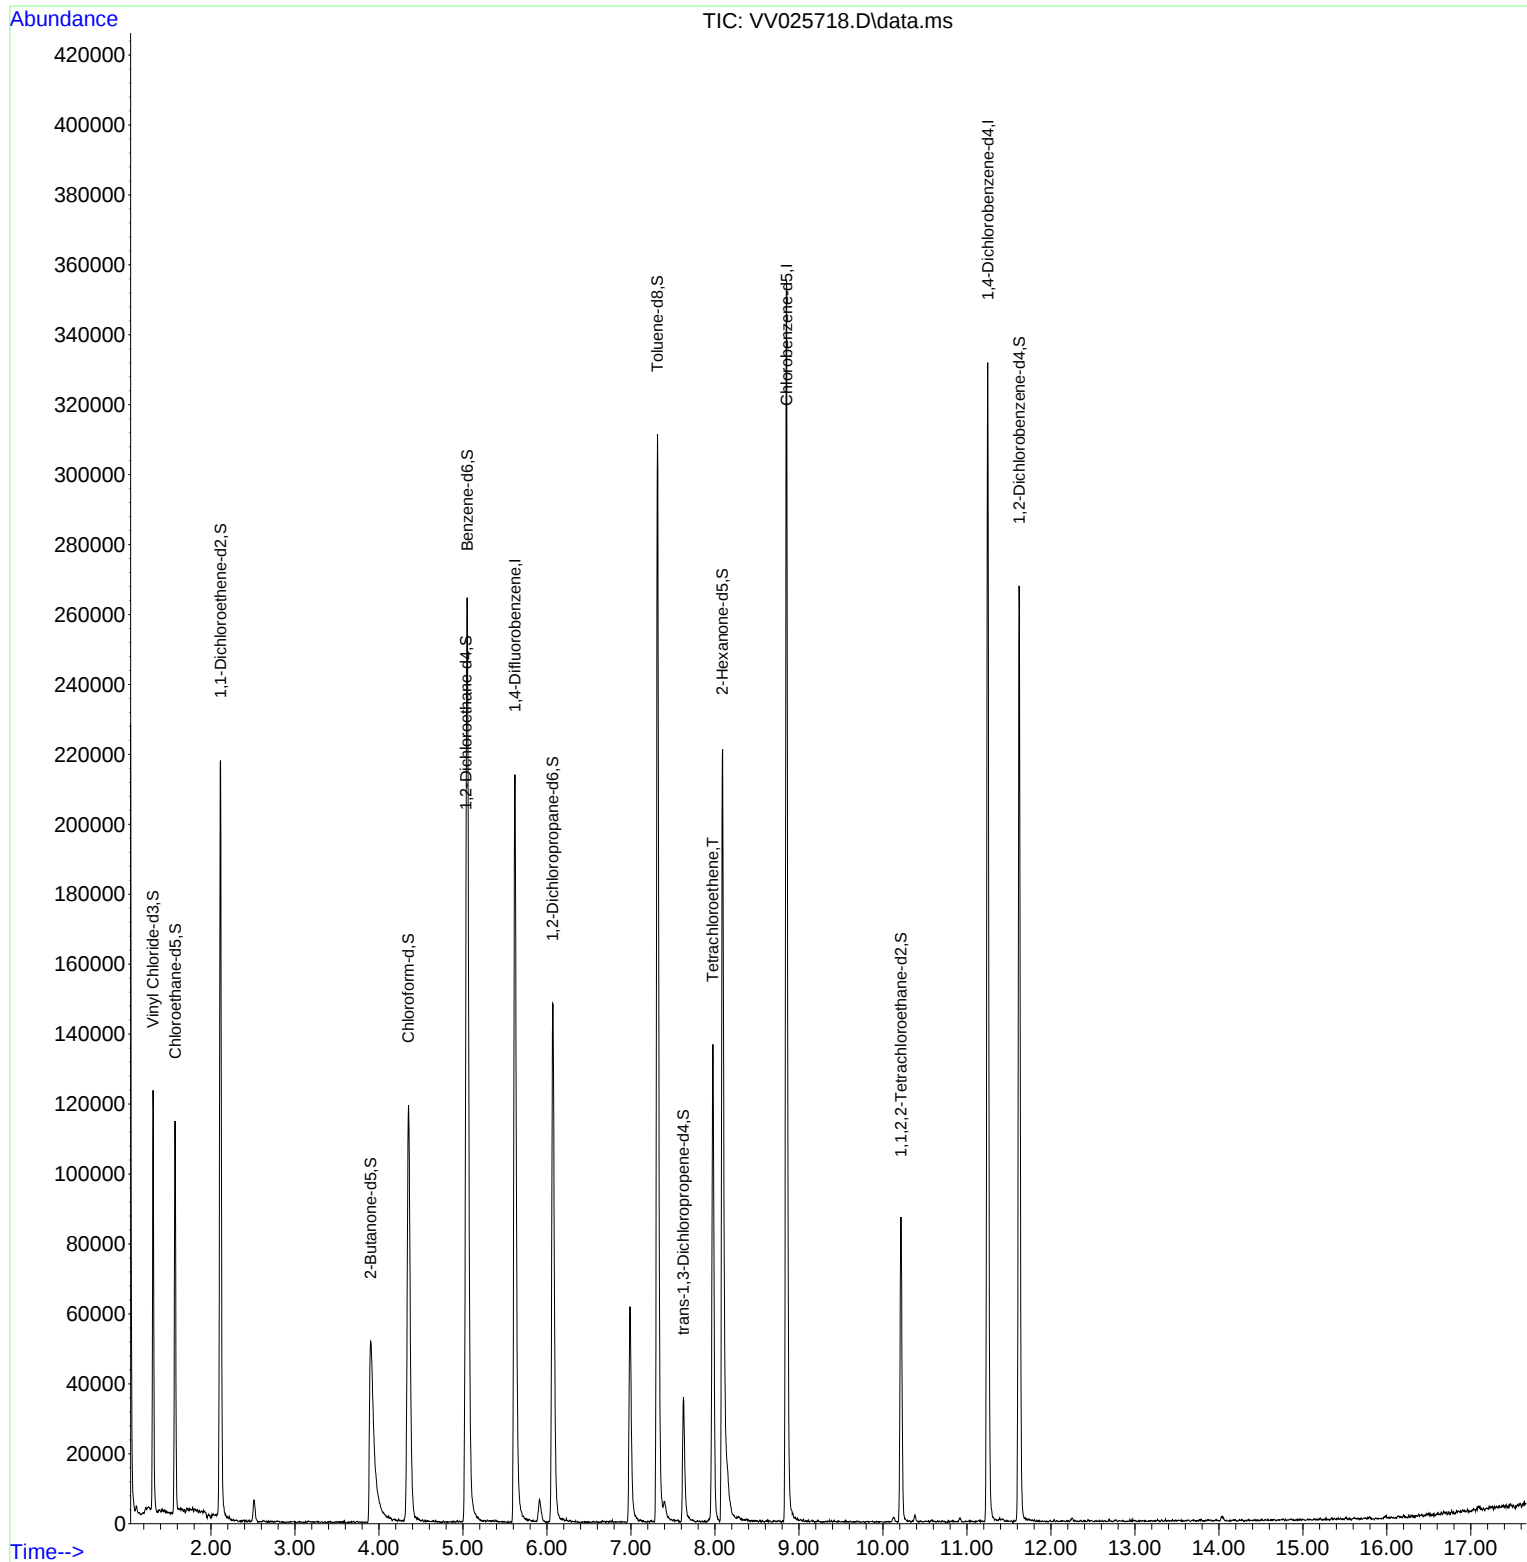

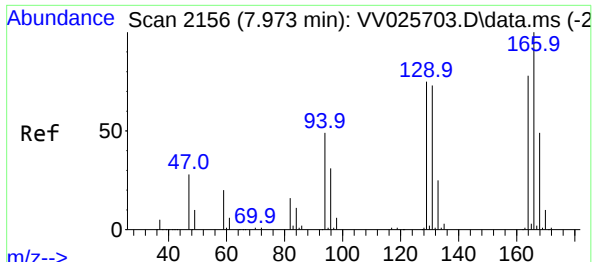

#47
Tetrachloroethene
Concen: 2.466 ug/L
RT: 7.976 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV025718.D
Acq: 25 Apr 2022 15:54

Instrument :
MSVOA_V
ClientSampleId :
EW6W9DL

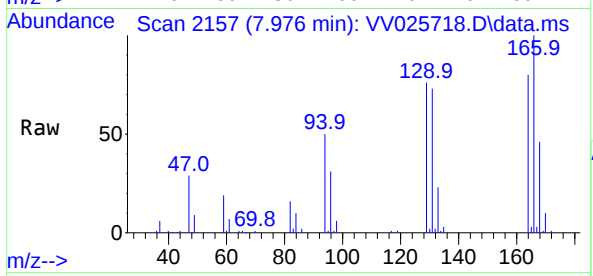

Tgt Ion:164 Resp: 29291

Ion	Ratio	Lower	Upper
164	100		
129	94.5	66.8	124.2
131	91.2	66.4	123.4
166	124.5	91.7	170.3

