

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
 Data File : VV025704.D
 Acq On : 25 Apr 2022 10:05
 Operator : SY/MD
 Sample : VV0425WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK351

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	102	rVB	120430	127713	19.60%	2.488%
2	1.568	156	164	175	rBV	128657	144441	22.17%	2.814%
3	2.104	320	331	351	rVB	215279	317177	48.68%	6.180%
4	3.886	873	885	915	rBV	53979	175793	26.98%	3.425%
5	4.342	1010	1027	1055	rBV2	117011	292547	44.90%	5.700%
6	5.040	1227	1244	1273	rBV2	260910	651557	100.00%	12.695%
7	5.612	1410	1422	1451	rBV	195144	398951	61.23%	7.773%
8	5.905	1503	1513	1532	rVB7	5882	12641	1.94%	0.246%
9	6.066	1547	1563	1590	rBV	148779	309843	47.55%	6.037%
10	6.982	1836	1848	1868	rBV	61556	118359	18.17%	2.306%
11	7.310	1935	1950	1970	rBV	305055	541467	83.10%	10.550%
12	7.619	2034	2046	2063	rBV2	34566	64035	9.83%	1.248%
13	7.976	2149	2157	2170	rVB6	4414	7835	1.20%	0.153%
14	8.085	2180	2191	2224	rBV	219299	430483	66.07%	8.387%
15	8.850	2416	2429	2450	rBV	309534	513057	78.74%	9.996%
16	10.213	2842	2853	2866	rBV	87615	135196	20.75%	2.634%
17	11.246	3162	3174	3195	rBV	302437	470609	72.23%	9.169%
18	11.622	3279	3291	3308	rBV	254789	405075	62.17%	7.892%
19	13.506	3868	3877	3890	rBV4	3742	6696	1.03%	0.130%
20	15.930	4620	4631	4632	rBV7	6245	9029	1.39%	0.176%




Sum of corrected areas: 5132504

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025704.D
Acq On : 25 Apr 2022 10:05
Operator : SY/MD
Sample : VV0425WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK351

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

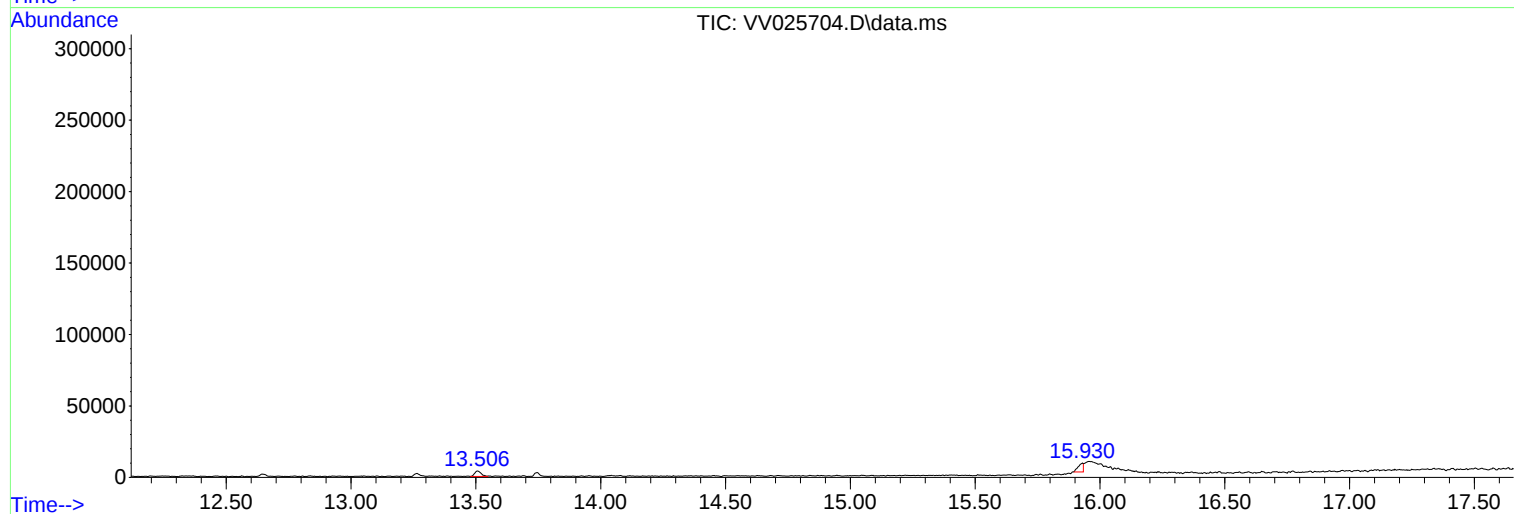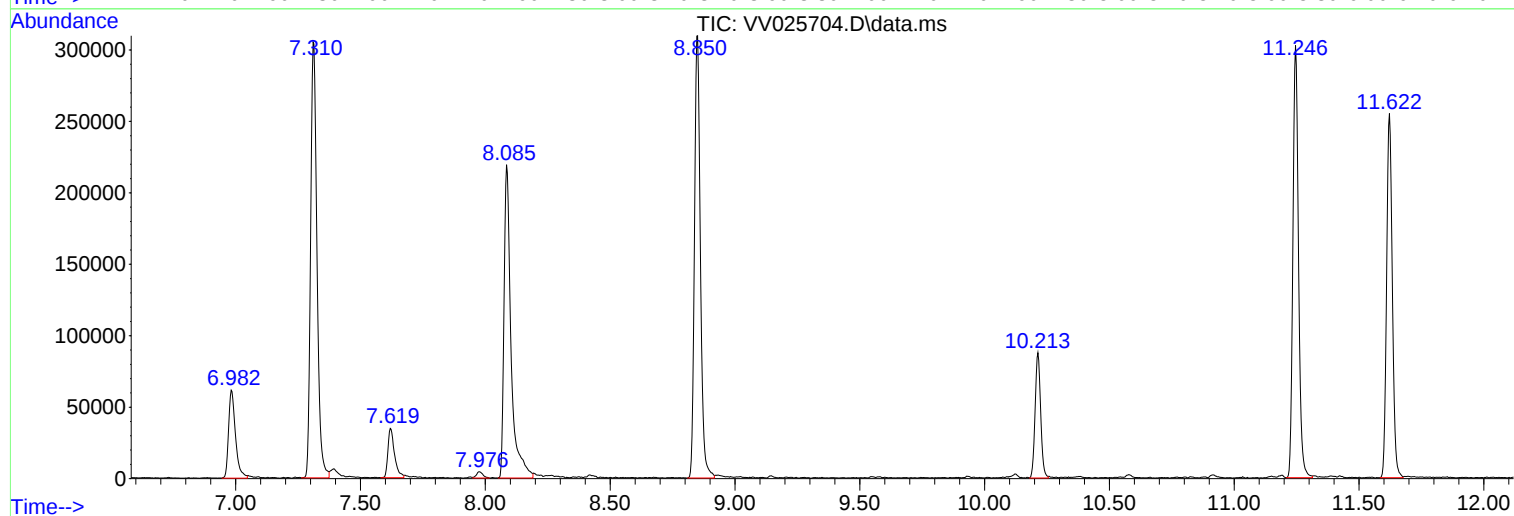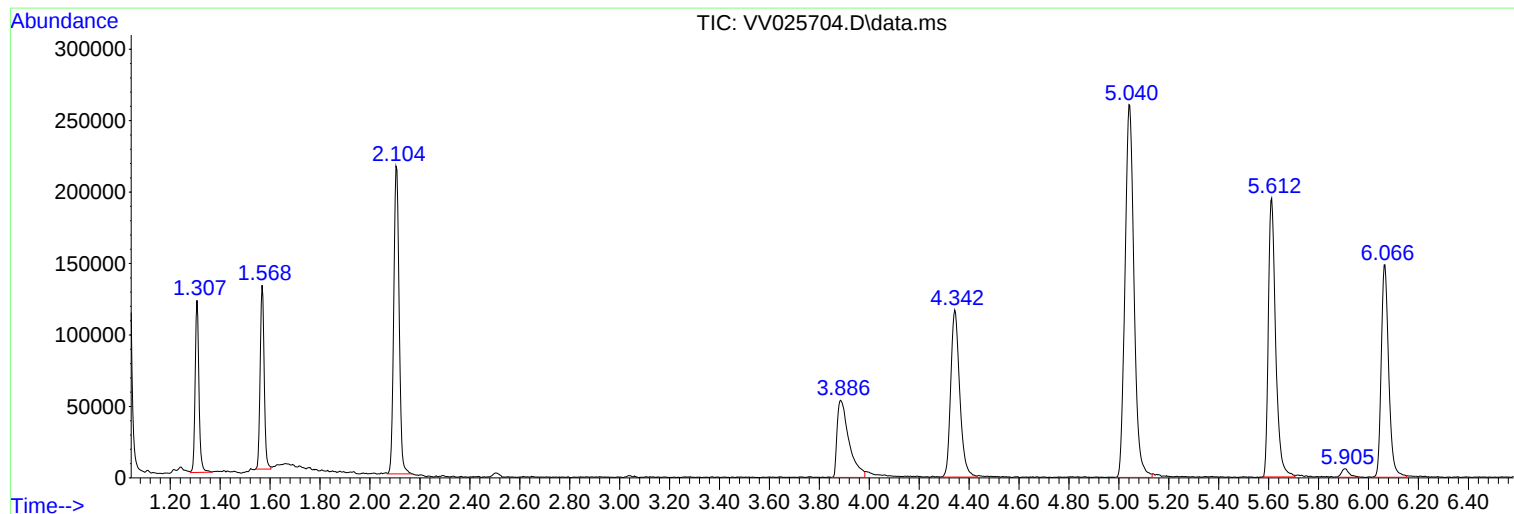

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025704.D
Acq On : 25 Apr 2022 10:05
Operator : SY/MD
Sample : VV0425WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK351

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025704.D
Acq On : 25 Apr 2022 10:05
Operator : SY/MD
Sample : VV0425WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK351

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
