

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
 Data File : VV025715.D
 Acq On : 25 Apr 2022 14:44
 Operator : SY/MD
 Sample : N2492-17DL 400X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	96	rBV	98515	104517	20.13%	2.367%
2	1.571	157	165	179	rBV	102540	116019	22.35%	2.628%
3	2.111	322	333	350	rBV	177851	255459	49.21%	5.786%
4	2.510	444	457	472	rVB3	5582	10534	2.03%	0.239%
5	3.896	876	888	923	rBV2	55481	184251	35.49%	4.173%
6	4.352	1016	1030	1060	rBV2	94998	237536	45.75%	5.380%
7	5.050	1232	1247	1275	rBV2	206952	519172	100.00%	11.758%
8	5.619	1413	1424	1448	rBV	152201	310167	59.74%	7.025%
9	5.915	1505	1516	1531	rVB9	6332	15254	2.94%	0.345%
10	6.072	1552	1565	1589	rBV	121823	251434	48.43%	5.695%
11	6.989	1840	1850	1871	rBV2	47129	92662	17.85%	2.099%
12	7.317	1941	1952	1971	rBV	241244	428075	82.45%	9.695%
13	7.625	2037	2048	2070	rBV	27377	50724	9.77%	1.149%
14	7.976	2144	2157	2173	rBV2	162854	276408	53.24%	6.260%
15	8.088	2183	2192	2223	rBV	174107	340660	65.62%	7.715%
16	8.419	2283	2295	2308	rBV2	8867	15438	2.97%	0.350%
17	8.854	2419	2430	2446	rBV	245607	405543	78.11%	9.185%
18	10.214	2842	2853	2869	rBV2	67920	109051	21.00%	2.470%
19	11.249	3160	3175	3194	rBV	231588	364565	70.22%	8.257%
20	11.622	3280	3291	3313	rBV	205632	327883	63.15%	7.426%


Sum of corrected areas: 4415352

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025715.D
Acq On : 25 Apr 2022 14:44
Operator : SY/MD
Sample : N2492-17DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

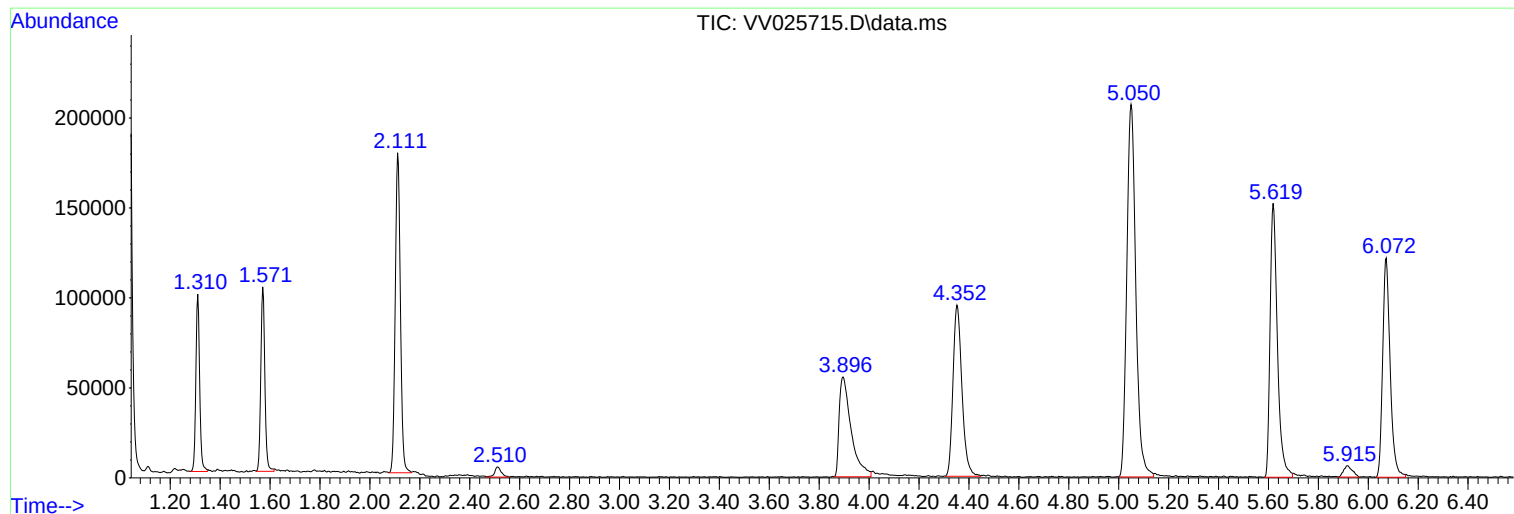

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025715.D
Acq On : 25 Apr 2022 14:44
Operator : SY/MD
Sample : N2492-17DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025715.D
Acq On : 25 Apr 2022 14:44
Operator : SY/MD
Sample : N2492-17DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------