

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
 Data File : VV025716.D
 Acq On : 25 Apr 2022 15:07
 Operator : SY/MD
 Sample : N2492-18DL 400X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	97	rVB	105936	110668	19.84%	2.432%
2	1.571	157	165	179	rBV	112067	128514	23.04%	2.824%
3	2.111	322	333	349	rVB	190594	273896	49.10%	6.018%
4	2.513	449	458	468	rBV2	5291	8427	1.51%	0.185%
5	3.895	875	888	926	rBV3	57494	190273	34.11%	4.181%
6	4.352	1013	1030	1061	rBV	101877	257562	46.18%	5.659%
7	5.050	1231	1247	1275	rBV2	223630	557790	100.00%	12.256%
8	5.619	1413	1424	1453	rBV	148036	307429	55.12%	6.755%
9	5.918	1505	1517	1531	rVB9	6395	14745	2.64%	0.324%
10	6.072	1552	1565	1588	rBV	126301	263002	47.15%	5.779%
11	6.989	1839	1850	1866	rBV2	51613	97482	17.48%	2.142%
12	7.317	1940	1952	1973	rBV	260285	461249	82.69%	10.135%
13	7.625	2039	2048	2071	rBV2	27930	53104	9.52%	1.167%
14	7.976	2145	2157	2178	rBV2	132699	226638	40.63%	4.980%
15	8.088	2182	2192	2229	rBV	181311	362412	64.97%	7.963%
16	8.423	2285	2296	2306	rVB4	7343	12475	2.24%	0.274%
17	8.853	2419	2430	2455	rBV	240705	399210	71.57%	8.772%
18	10.217	2843	2854	2867	rBV	72619	116138	20.82%	2.552%
19	11.249	3164	3175	3195	rBV	225225	357818	64.15%	7.862%
20	11.622	3279	3291	3312	rBV	222369	352349	63.17%	7.742%




Sum of corrected areas: 4551181

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025716.D
Acq On : 25 Apr 2022 15:07
Operator : SY/MD
Sample : N2492-18DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

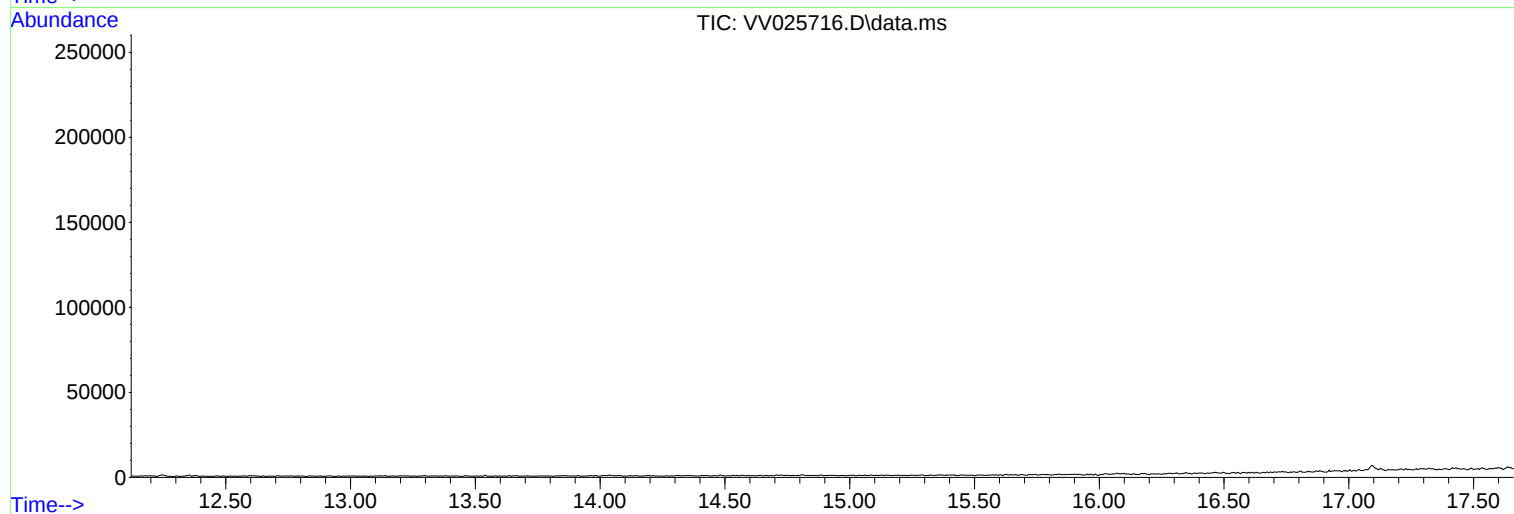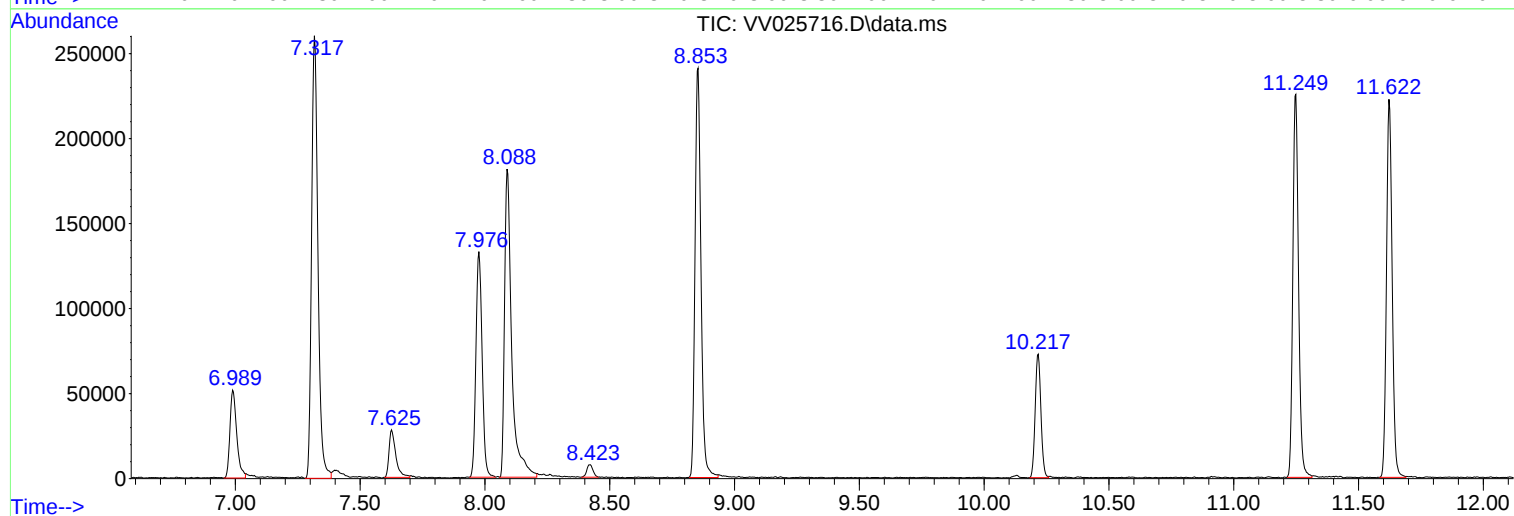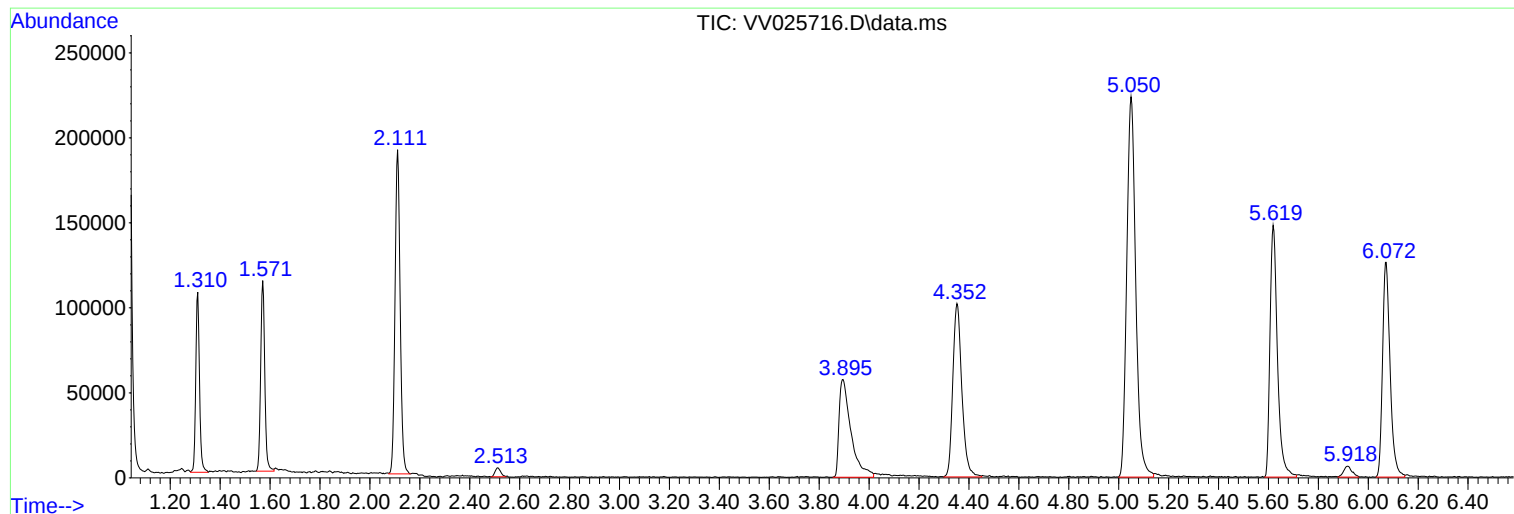

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025716.D
Acq On : 25 Apr 2022 15:07
Operator : SY/MD
Sample : N2492-18DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025716.D
Acq On : 25 Apr 2022 15:07
Operator : SY/MD
Sample : N2492-18DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------