

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
 Data File : VV025718.D
 Acq On : 25 Apr 2022 15:54
 Operator : SY/MD
 Sample : N2492-23DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	99	rVB	120735	126196	19.06%	2.253%
2	1.574	157	166	176	rBV	112247	130595	19.72%	2.332%
3	2.114	320	334	351	rBV	215897	318479	48.10%	5.687%
4	2.513	449	458	473	rVB	6282	11109	1.68%	0.198%
5	3.902	877	890	937	rBV	51773	202717	30.61%	3.620%
6	4.352	1013	1030	1055	rBV	118919	298500	45.08%	5.330%
7	5.050	1230	1247	1284	rBV2	264317	662173	100.00%	11.824%
8	5.619	1412	1424	1455	rBV	213896	443096	66.92%	7.912%
9	5.911	1504	1515	1531	rBV4	6444	14170	2.14%	0.253%
10	6.069	1551	1564	1585	rBV	148185	312392	47.18%	5.578%
11	6.989	1838	1850	1869	rBV2	61738	118143	17.84%	2.110%
12	7.317	1940	1952	1972	rBV	311173	550358	83.11%	9.827%
13	7.625	2038	2048	2063	rBV2	35692	65546	9.90%	1.170%
14	7.976	2145	2157	2182	rVB	136561	234460	35.41%	4.187%
15	8.091	2182	2193	2241	rBV	220903	452730	68.37%	8.084%
16	8.853	2418	2430	2451	rBV	354686	577310	87.18%	10.309%
17	10.214	2842	2853	2867	rBV	87311	141055	21.30%	2.519%
18	11.249	3162	3175	3194	rBV	331491	521884	78.81%	9.319%
19	11.622	3279	3291	3310	rBV	267405	419327	63.33%	7.488%




Sum of corrected areas: 5600240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025718.D
Acq On : 25 Apr 2022 15:54
Operator : SY/MD
Sample : N2492-23DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

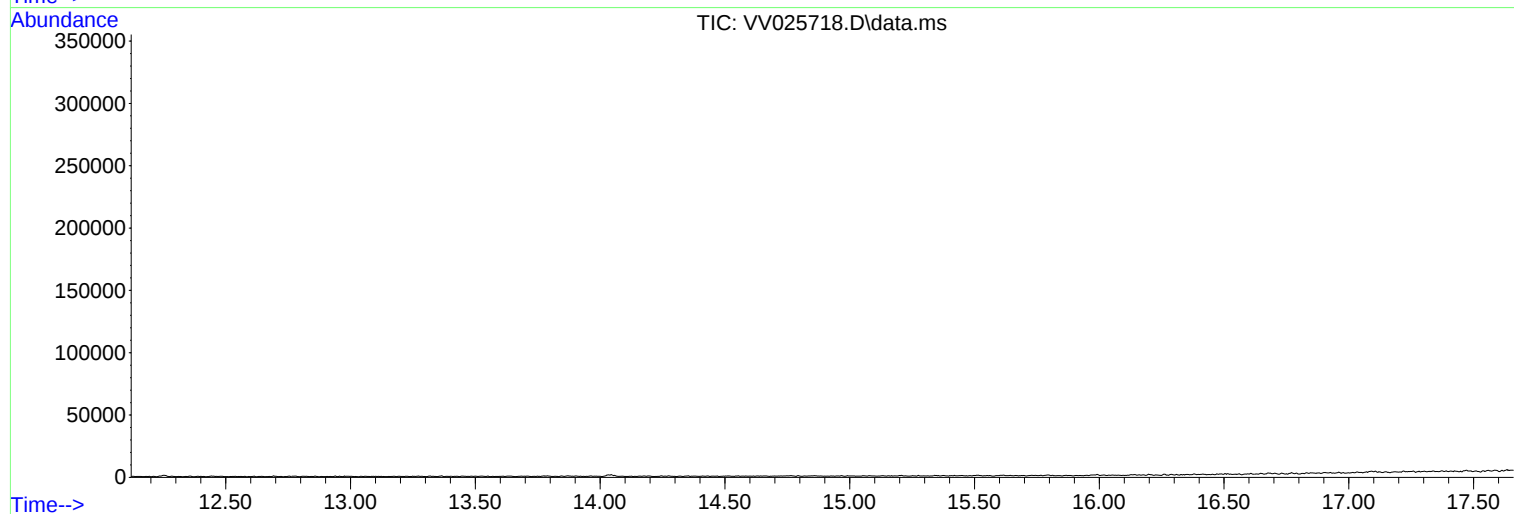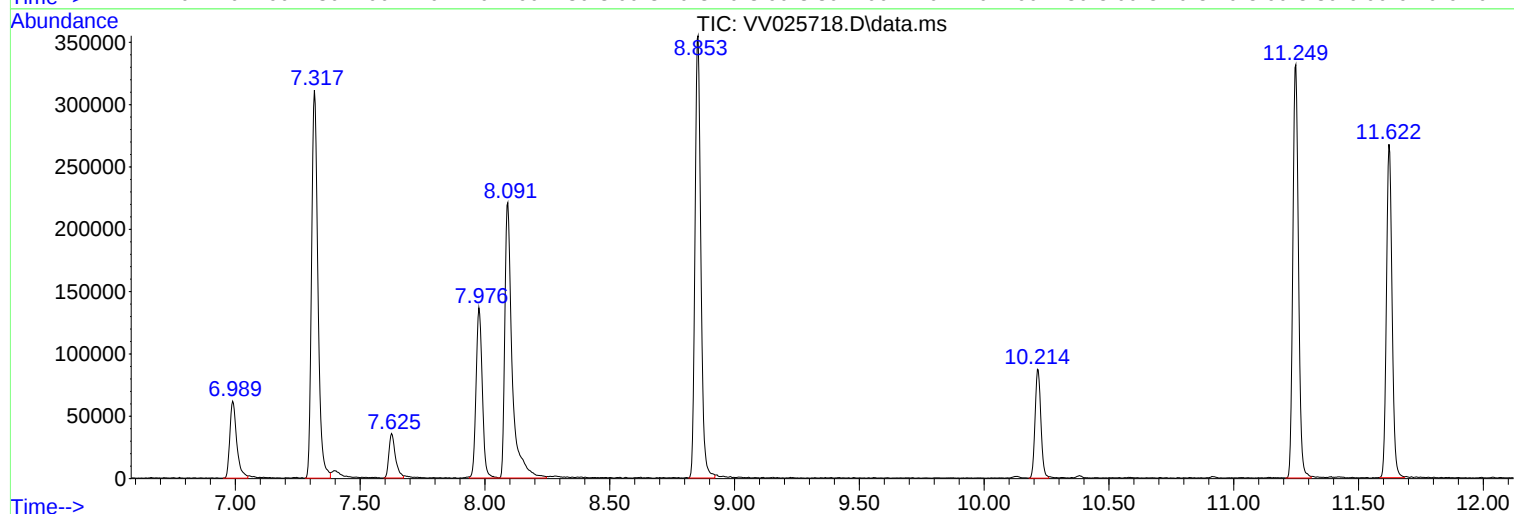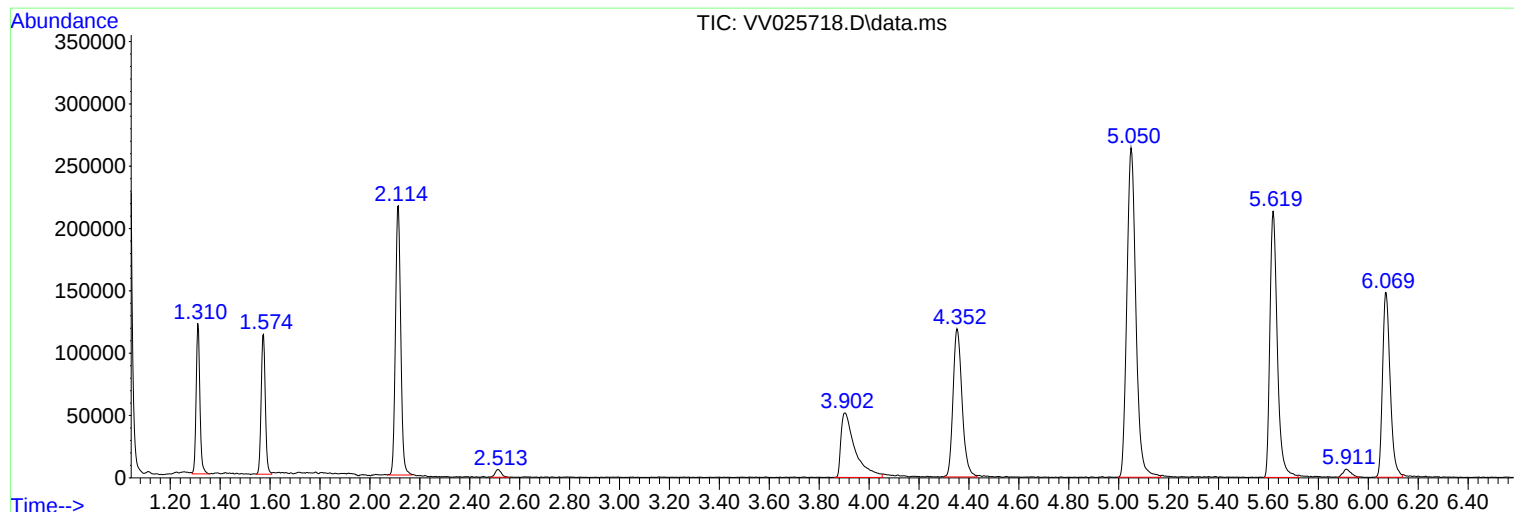

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025718.D
Acq On : 25 Apr 2022 15:54
Operator : SY/MD
Sample : N2492-23DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025718.D
Acq On : 25 Apr 2022 15:54
Operator : SY/MD
Sample : N2492-23DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc