
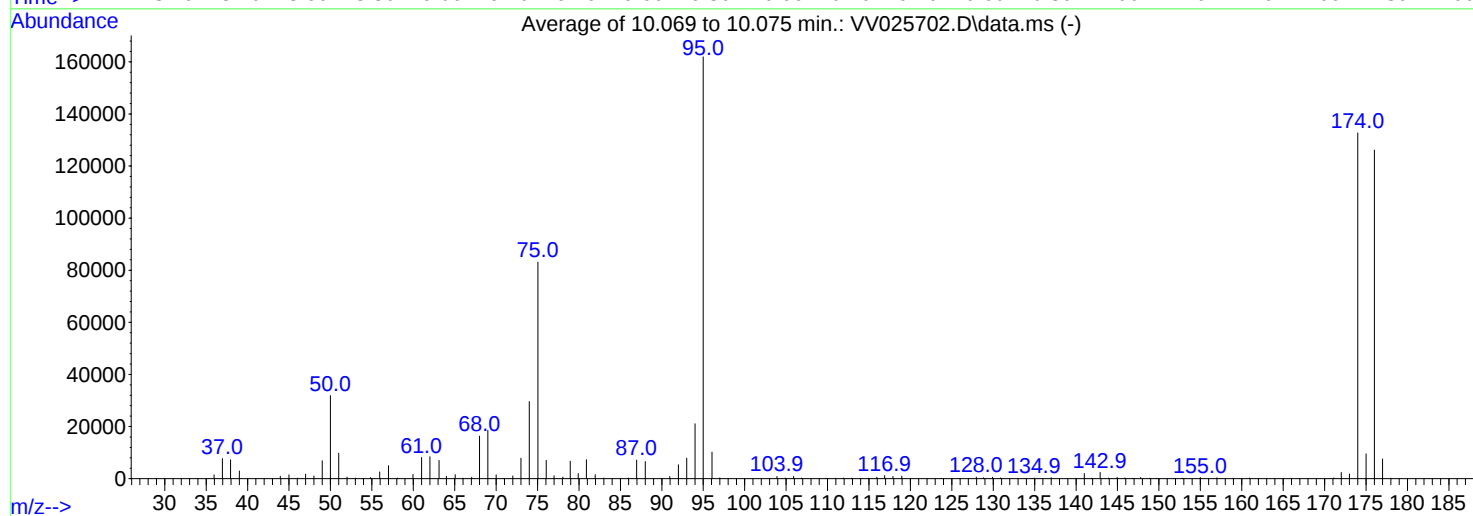


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042522\
Data File : VV025702.D
Acq On : 25 Apr 2022 08:51
Operator : SY/MD
Sample : BFB309
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB309

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 27 05:32:04 2022

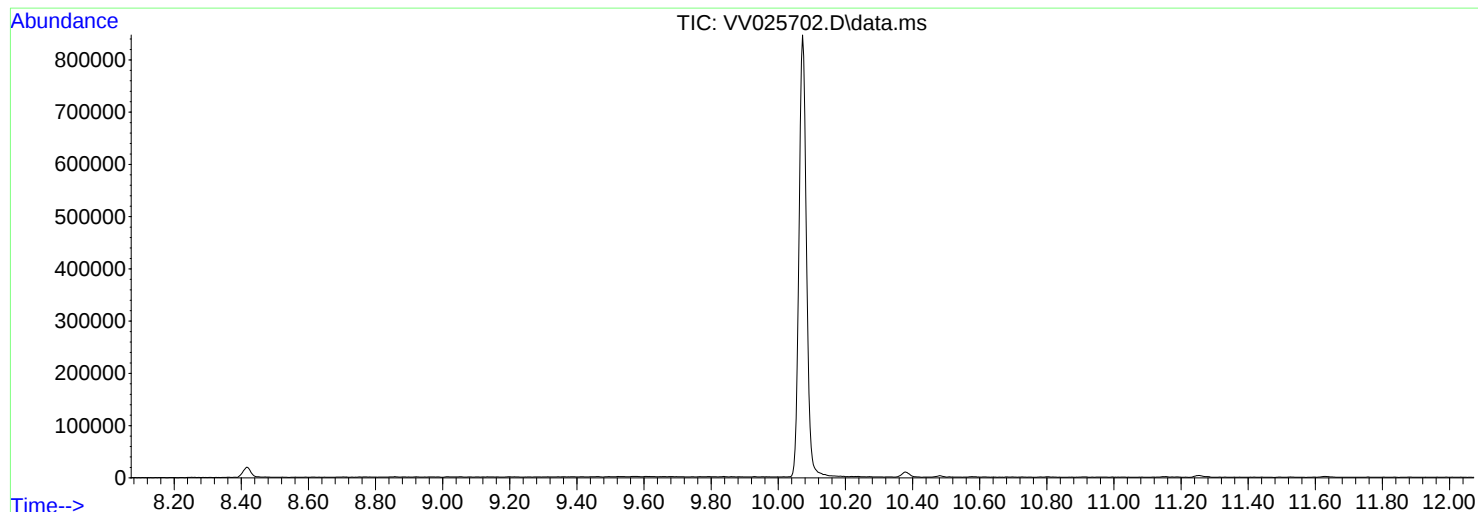

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	31896	PASS
75	95	30	80	51.3	83088	PASS
95	95	100	100	100.0	161920	PASS
96	95	5	9	6.3	10194	PASS
173	174	0.00	2	1.3	1786	PASS
174	95	50	120	82.0	132739	PASS
175	174	5	9	7.2	9527	PASS
176	174	95	105	95.1	126184	PASS
177	176	5	10	6.0	7551	PASS

m/z	Abundance
35.90	881.0
36.90	140.0
37.90	439.0
39.10	112.0
40.00	162.0
43.90	314.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	2566.0
37.00	8008.0
38.00	7603.0
39.00	2970.0
39.90	309.0
43.00	168.0
44.00	1180.0
45.00	1522.0
46.10	239.0
47.00	1711.0
48.00	1105.0
49.00	6932.0
50.00	31568.0
51.00	9860.0
52.00	583.0
53.00	271.0
54.80	419.0
56.00	2633.0
57.00	4964.0
58.10	290.0
60.00	1630.0
61.00	8278.0
62.00	8445.0
63.10	7040.0
64.00	952.0
65.00	1572.0
66.00	187.0
67.10	588.0
68.00	16020.0
69.00	18440.0
70.00	1480.0
70.90	105.0
72.00	1138.0
73.00	7951.0
74.00	28848.0
75.10	81384.0
76.00	6959.0
77.00	1054.0
78.10	590.0
78.90	6716.0
79.90	1880.0
80.90	7209.0
82.00	1515.0
83.00	261.0
86.00	228.0
86.90	7155.0
88.00	6380.0
91.00	829.0
92.00	5222.0
93.00	7582.0
94.00	20568.0
95.00	158528.0
96.10	10023.0
97.00	320.0
103.90	878.0
104.90	281.0
105.90	792.0
106.90	229.0
109.80	163.0
111.00	216.0
111.90	256.0
112.90	168.0
114.90	214.0
116.00	523.0
116.90	1253.0
117.90	848.0
118.90	1070.0
123.70	132.0
128.00	583.0
128.80	413.0
129.90	509.0
130.90	268.0
134.70	187.0
135.00	203.0
137.00	363.0
141.00	1804.0
142.90	2339.0
143.90	237.0
144.90	501.0
145.90	272.0
146.80	119.0
147.80	468.0
148.80	143.0
149.70	146.0
152.80	212.0
155.00	436.0
156.90	330.0
159.00	173.0
160.90	228.0
171.10	306.0
172.00	2160.0
173.00	1799.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

174.00	126856.0
175.00	9450.0
176.00	120216.0
177.00	7588.0
178.00	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	2443.0
37.00	8070.0
38.00	7907.0
39.00	3183.0
40.00	293.0
43.00	160.0
44.00	1235.0
45.00	1544.0
46.10	259.0
47.00	1731.0
48.00	1067.0
49.00	7168.0
50.00	33016.0
51.00	10115.0
52.00	671.0
53.00	257.0
53.90	104.0
54.80	436.0
55.90	2712.0
57.00	5179.0
58.10	301.0
59.90	1651.0
61.00	8442.0
62.00	8781.0
63.10	7312.0
64.00	1003.0
65.00	1568.0
66.00	216.0
67.00	577.0
68.00	16848.0
69.00	19360.0
70.00	1511.0
70.90	113.0
72.00	1095.0
73.00	8123.0
74.00	30648.0
75.00	85856.0
76.10	7248.0
77.00	1193.0
78.00	660.0
78.90	6964.0
79.90	2054.0
80.90	7433.0
82.00	1601.0
83.00	253.0
86.00	255.0
87.00	7398.0
88.00	6787.0
91.00	792.0
92.00	5612.0
93.00	8229.0
94.00	21936.0
95.00	168000.0
96.10	10577.0
97.00	333.0
103.90	901.0
104.90	260.0
105.90	888.0
106.80	237.0
109.80	157.0
111.00	207.0
111.90	271.0
112.90	185.0
115.00	228.0
116.00	585.0
116.90	1167.0
117.90	850.0
118.90	1029.0
123.80	128.0
125.90	103.0
128.00	649.0
128.80	405.0
129.90	561.0
130.90	324.0
135.00	247.0
137.00	373.0
139.90	169.0
141.00	2037.0
141.80	283.0
142.90	2542.0
143.90	260.0
145.00	501.0
145.90	298.0
146.80	161.0
147.80	458.0
148.80	132.0
149.70	136.0
151.80	138.0
152.90	213.0
155.00	471.0
157.00	294.0
159.00	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

161.00	249.0
171.10	281.0
172.00	2552.0
173.00	1856.0
174.00	137536.0
175.00	9925.0
176.00	131032.0
177.00	7713.0
178.00	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	2166.0
37.00	7346.0
38.00	7503.0
39.00	3041.0
40.00	265.0
43.00	140.0
44.00	1223.0
45.00	1415.0
46.00	279.0
47.00	1672.0
48.00	959.0
49.00	6556.0
50.00	31104.0
51.00	9337.0
52.00	598.0
53.00	232.0
54.90	417.0
56.00	2497.0
57.00	4841.0
58.10	241.0
60.00	1455.0
61.00	7680.0
62.00	8083.0
63.10	6586.0
64.00	904.0
65.10	1543.0
66.00	203.0
67.00	507.0
68.00	16140.0
69.00	17808.0
70.00	1357.0
71.00	102.0
72.00	971.0
73.00	7507.0
74.00	29416.0
75.00	82024.0
76.10	6759.0
77.00	1135.0
78.00	657.0
79.00	6467.0
79.90	2057.0
80.90	7036.0
81.90	1573.0
83.00	226.0
86.00	262.0
87.00	6767.0
88.00	6561.0
90.90	725.0
92.00	5269.0
93.00	7801.0
94.00	20792.0
95.00	159232.0
96.00	9983.0
97.00	359.0
103.90	862.0
104.90	264.0
105.90	892.0
106.80	223.0
109.80	135.0
111.00	180.0
111.90	242.0
112.90	200.0
115.00	212.0
115.90	592.0
116.90	1049.0
117.90	817.0
119.00	918.0
123.80	116.0
125.90	124.0
127.90	643.0
128.80	345.0
129.90	564.0
130.90	327.0
134.90	301.0
137.00	308.0
139.90	219.0
141.00	2094.0
141.90	233.0
142.90	2269.0
143.90	241.0
144.90	441.0
145.90	311.0
146.80	158.0
147.80	415.0
148.90	108.0
149.70	103.0
150.00	115.0
151.80	161.0
152.80	153.0
155.00	472.0
157.10	252.0
158.90	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

161.00	247.0
171.10	285.0
172.00	2536.0
173.00	1703.0
174.00	133824.0
175.00	9205.0
176.00	127304.0
177.00	7353.0
178.00	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309