




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025736.D
 Acq On : 29 Apr 2022 11:28
 Operator : SY/MD
 Sample : N2615-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D7

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

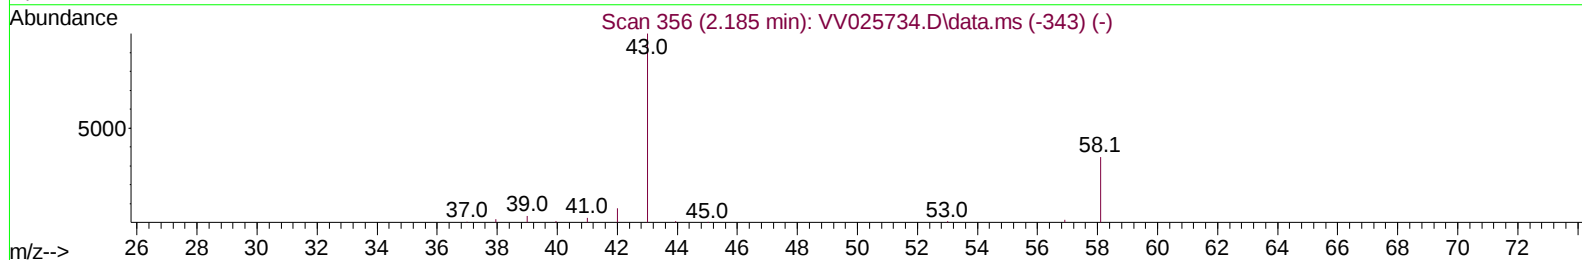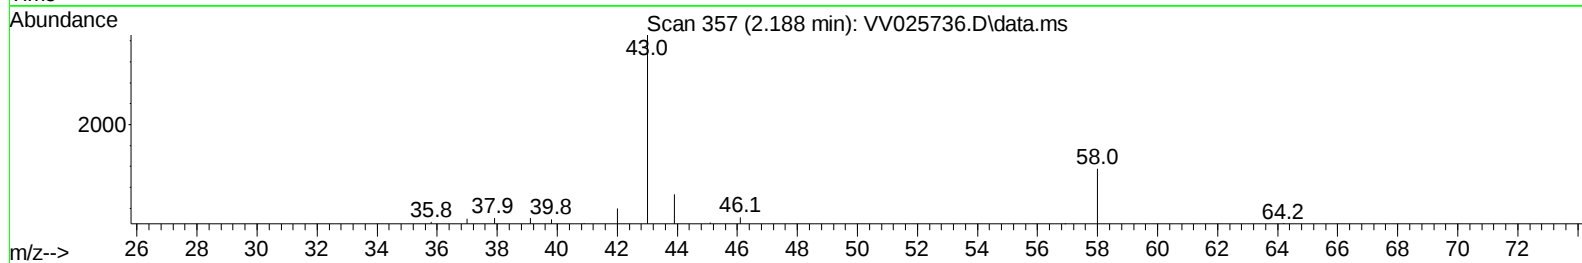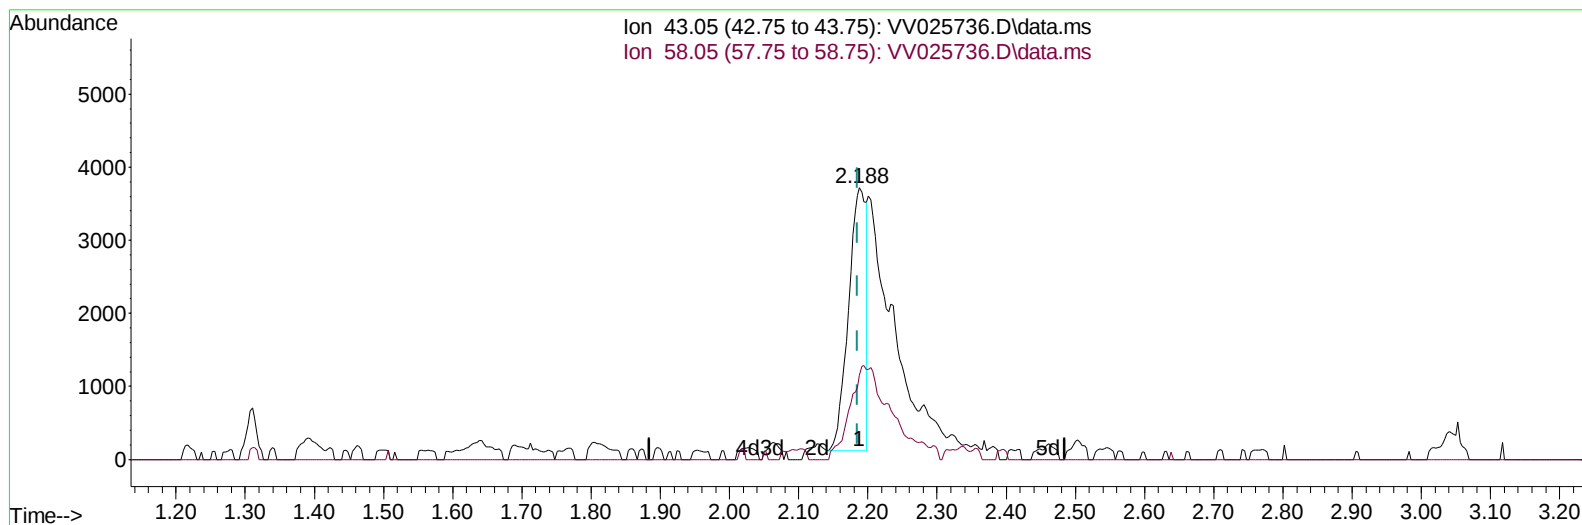

TIC: VV025736.D\data.ms

(13) Acetone (T)

2.188min (+ 0.003) 5.23 ug/L

response 6348

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	82.91#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025736.D
 Acq On : 29 Apr 2022 11:28
 Operator : SY/MD
 Sample : N2615-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D7

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

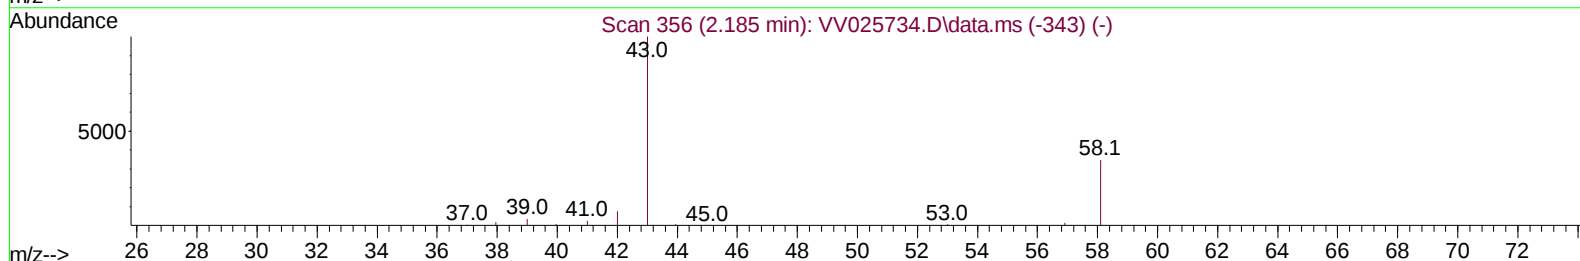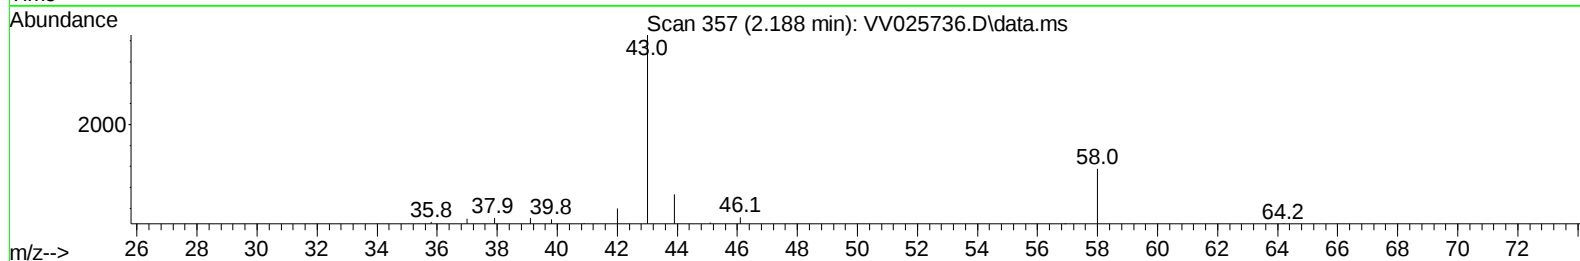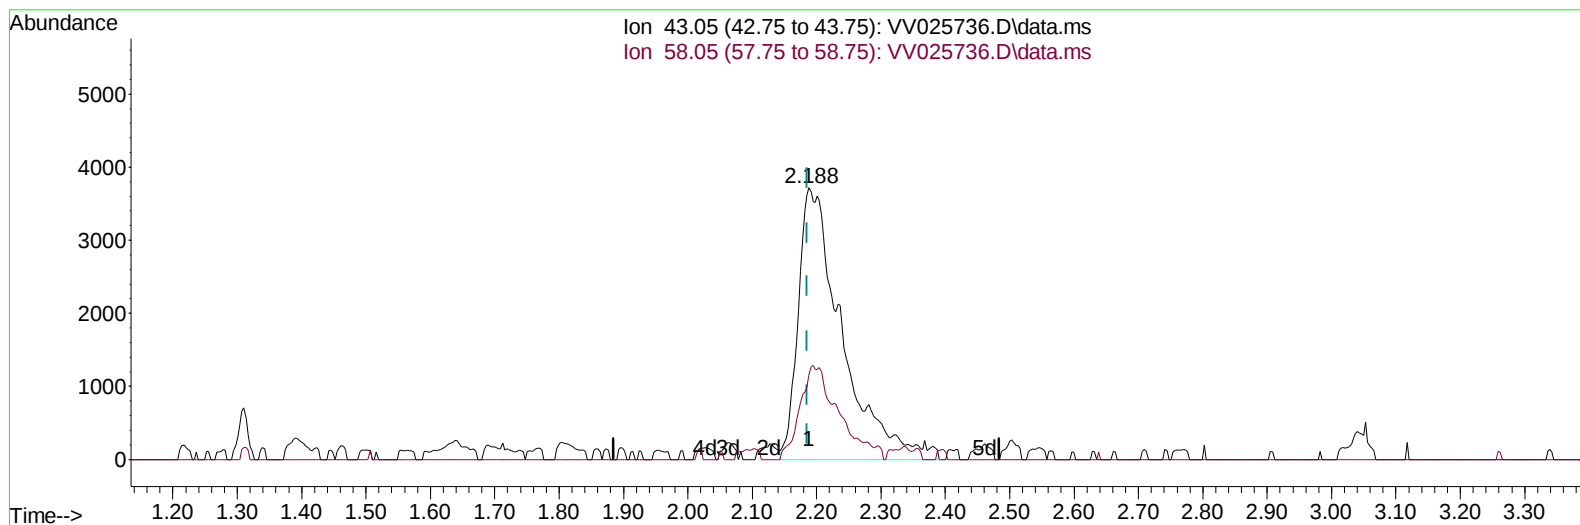

TIC: VV025736.D\data.ms

(13) Acetone (T)

2.188min (+ 0.003) 14.36 ug/L m

response 17428

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	30.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025736.D
 Acq On : 29 Apr 2022 11:28
 Operator : SY/MD
 Sample : N2615-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D7

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

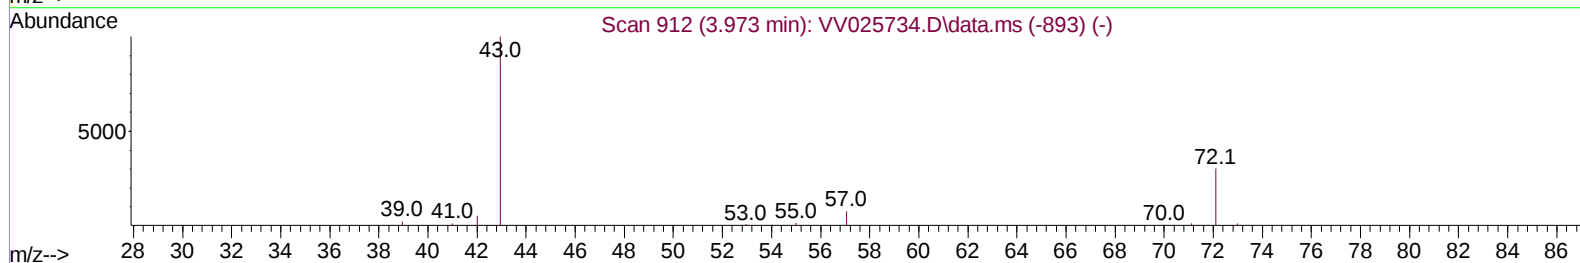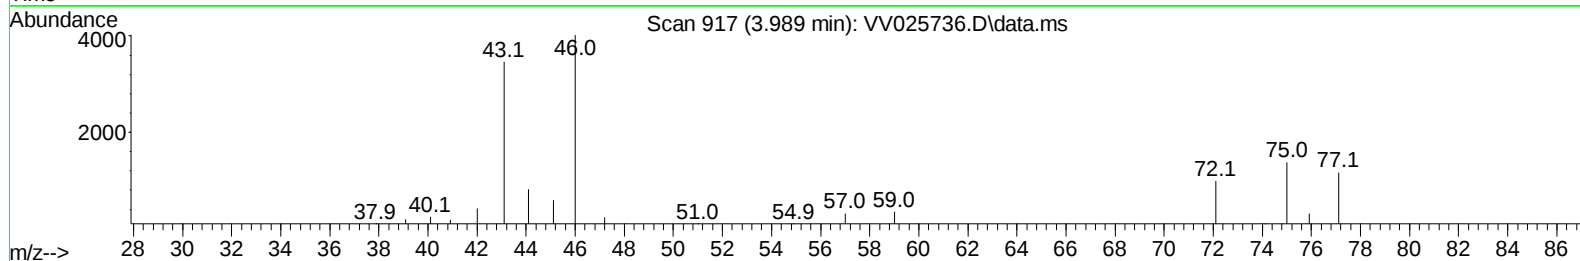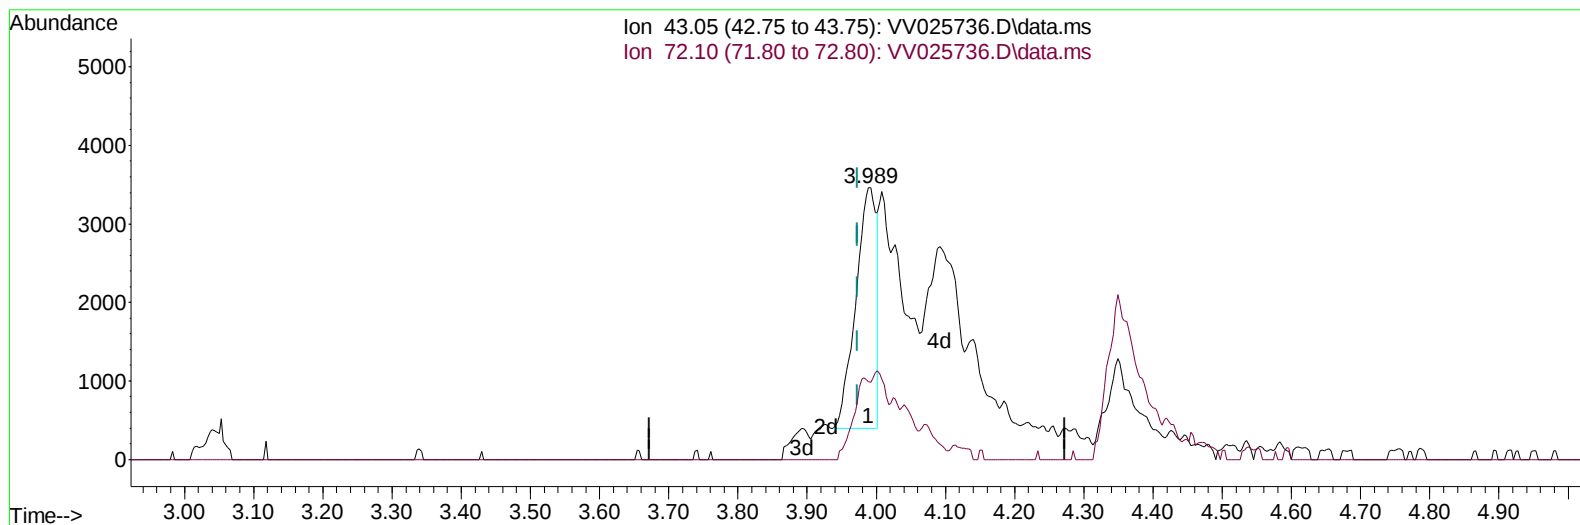

TIC: VV025736.D\data.ms

(21) 2-Butanone (T)

3.989min (+ 0.016) 3.82 ug/L

response 6409

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	27.93
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025736.D
Acq On : 29 Apr 2022 11:28
Operator : SY/MD
Sample : N2615-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D7

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon May 02 01:22:31 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

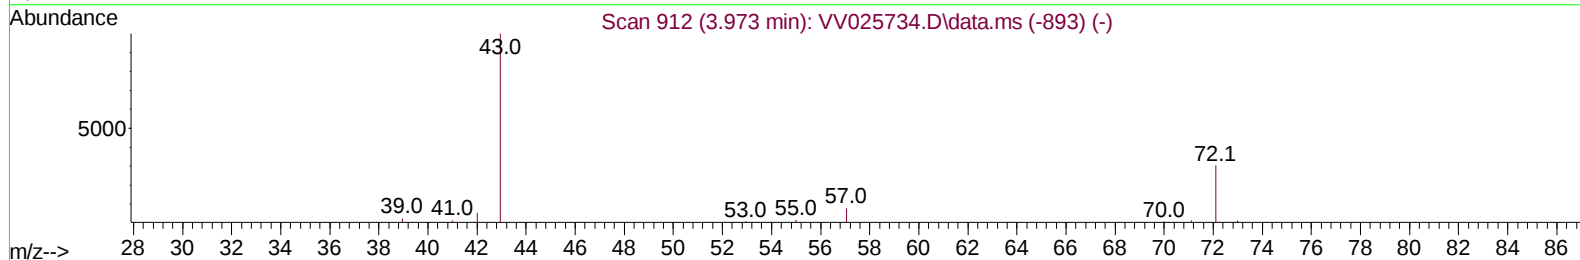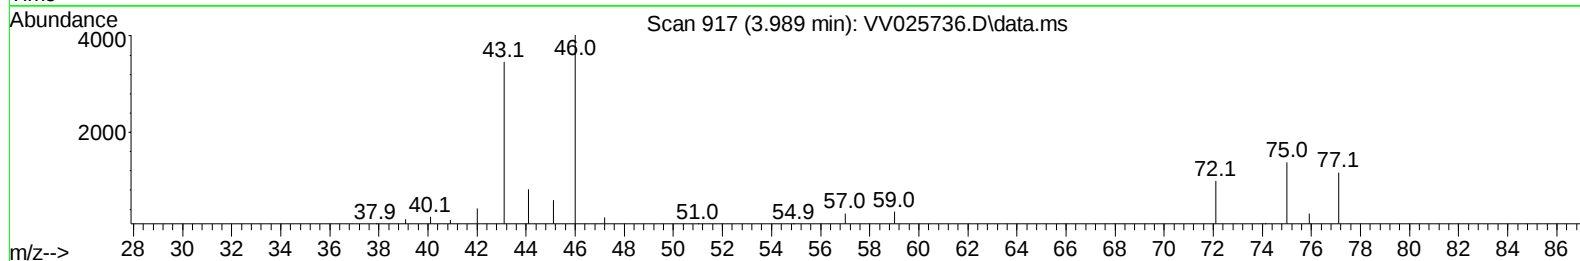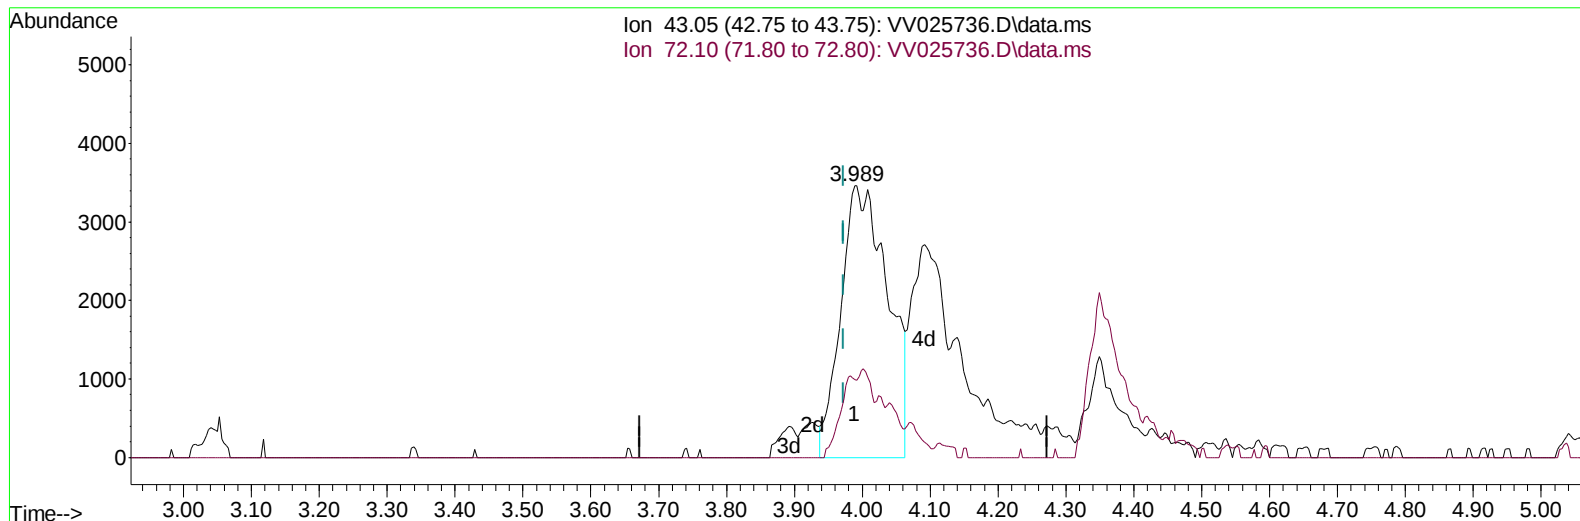

TIC: VV025736.D\data.ms

(21) 2-Butanone (T)

3.989min (+ 0.016) 9.90 ug/L m

response 16602

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	10.78#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025736.D
 Acq On : 29 Apr 2022 11:28
 Operator : SY/MD
 Sample : N2615-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D7

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	158095	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	160794	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	75402	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	57879	3.938	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	78.800%	
7) Chloroethane-d5	1.568	69	61514	3.934	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	78.600%	
11) 1,1-Dichloroethene-d2	2.108	63	95773	3.253	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	65.000%	
20) 2-Butanone-d5	3.895	46	109282	61.123	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	122.240%	
24) Chloroform-d	4.346	84	117502	5.290	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	105.800%	
26) 1,2-Dichloroethane-d4	5.030	65	55478	5.797	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	116.000%	
32) Benzene-d6	5.043	84	221801	4.767	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	95.400%	
36) 1,2-Dichloropropane-d6	6.063	67	69592	5.364	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	107.200%	
41) Toluene-d8	7.313	98	183769	4.256	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.622	79	19982	4.582	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	91.600%	
46) 2-Hexanone-d5	8.085	63	80325	52.480	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	104.960%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	40801	4.977	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	99.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	66353	5.249	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	105.000%	
Target Compounds						
					Qvalue	
13) Acetone	2.188	43	17428m	14.362	ug/L	
16) Methylene chloride	2.506	84	33561	2.524	ug/L	95
21) 2-Butanone	3.989	43	16602m	9.901	ug/L	
25) Chloroform	4.368	83	4973	0.242	ug/L	96
33) Benzene	5.098	78	14825	0.312	ug/L	100
42) Toluene	7.387	91	28311	0.548	ug/L	96
52) Ethylbenzene	9.014	91	2327	0.042	ug/L	98
53) m,p-Xylene	9.140	106	2630	0.126	ug/L	86
54) o-Xylene	9.545	106	2521	0.124	ug/L	98
62) 1,3,5-Trimethylbenzene	10.538	105	1198	0.058	ug/L	90
63) 1,2,4-Trimethylbenzene	10.914	105	5039	0.134	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025736.D
Acq On : 29 Apr 2022 11:28
Operator : SY/MD
Sample : N2615-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D7

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon May 02 01:22:31 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

