




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025737.D
 Acq On : 29 Apr 2022 11:51
 Operator : SY/MD
 Sample : N2615-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

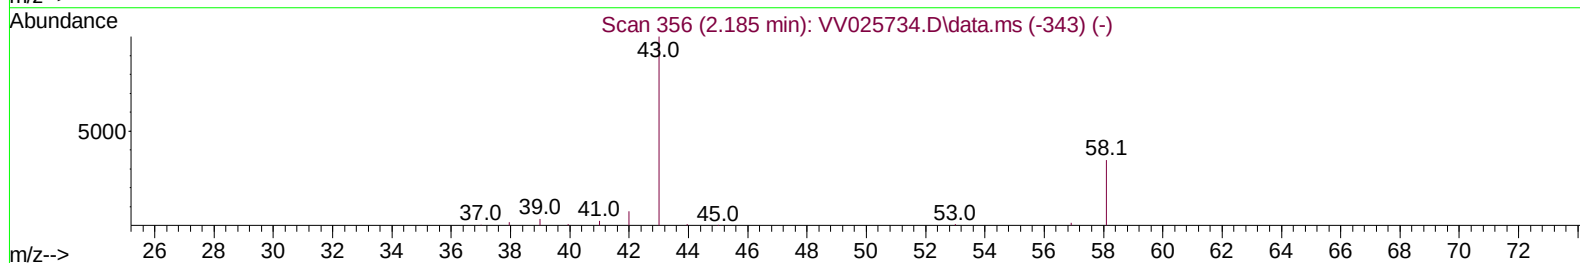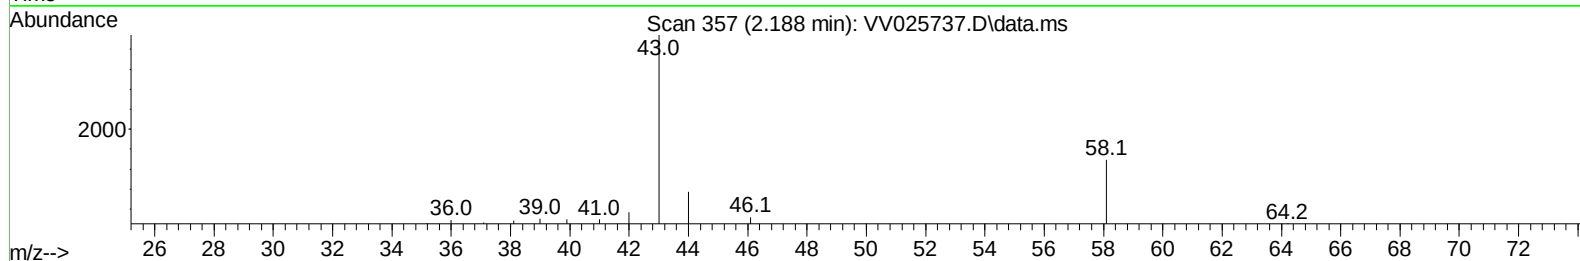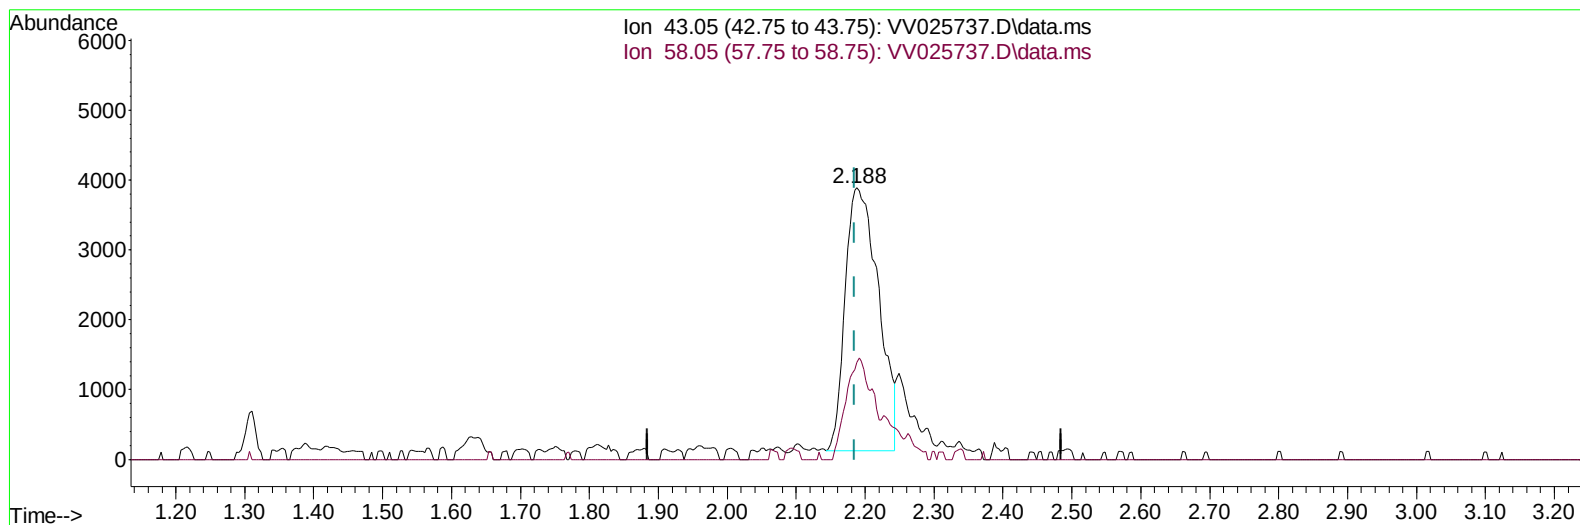

TIC: VV025737.D\data.ms

(13) Acetone (T)

2.188min (+ 0.003) 10.00 ug/L

response 12586

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	30.68
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025737.D
 Acq On : 29 Apr 2022 11:51
 Operator : SY/MD
 Sample : N2615-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

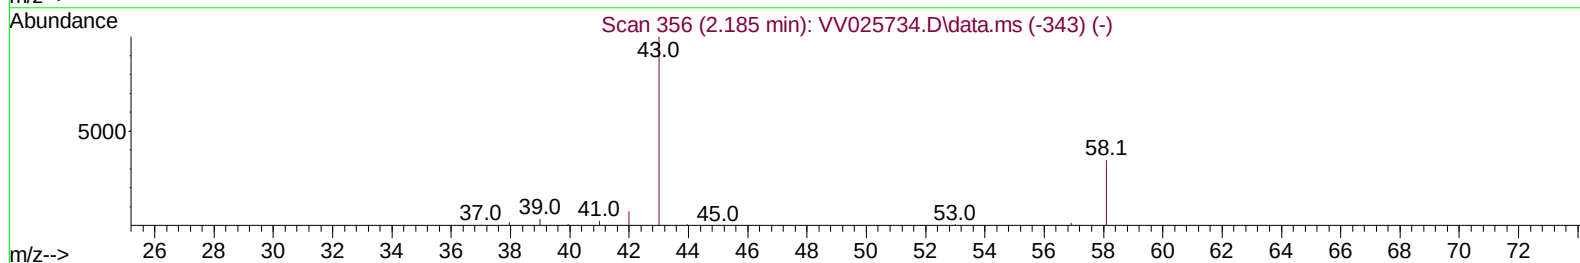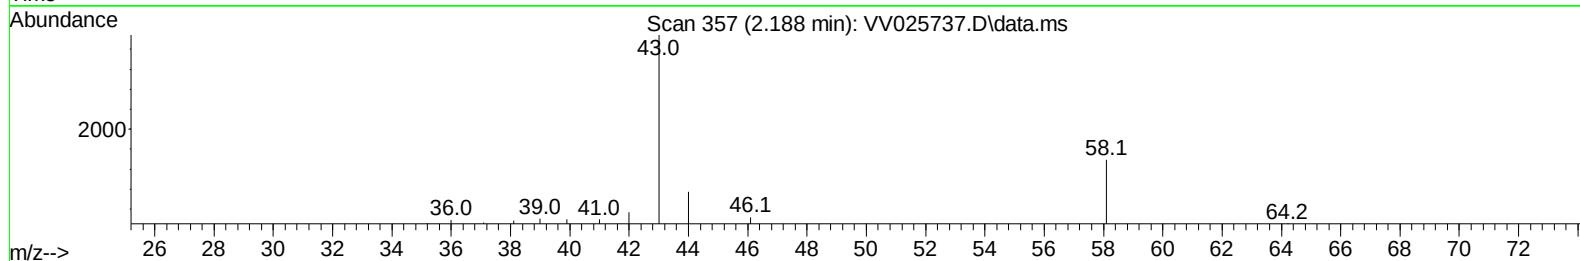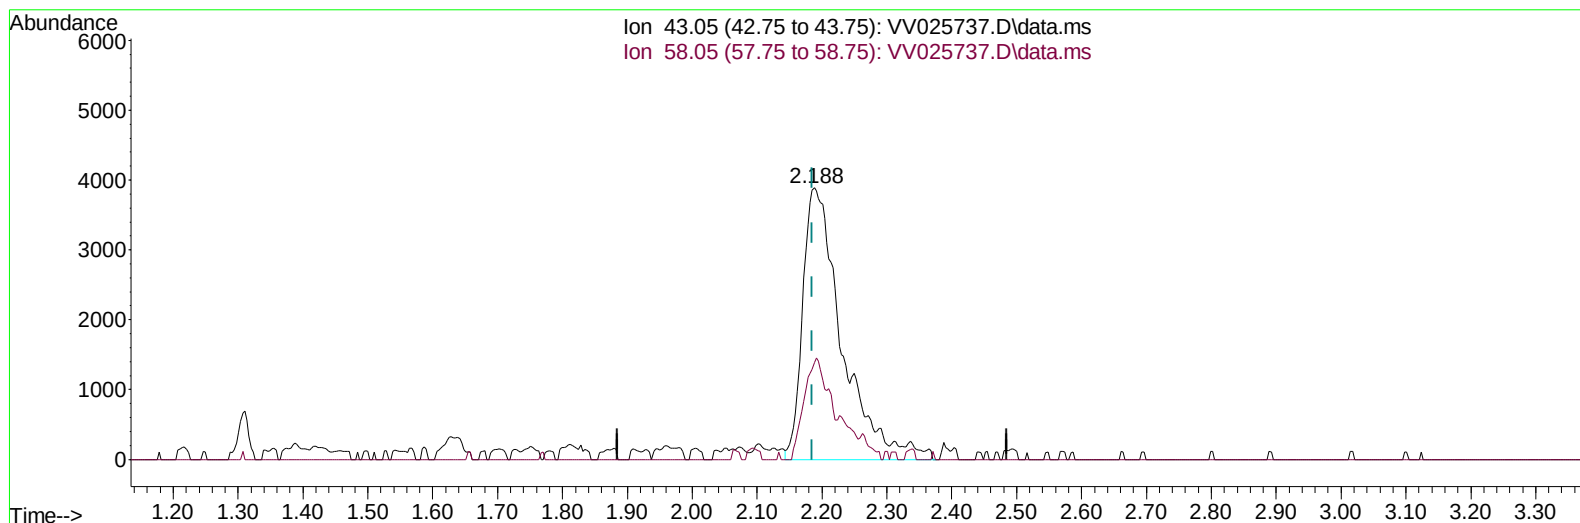

TIC: VV025737.D\data.ms

(13) Acetone (T)

2.188min (+ 0.003) 12.94 ug/L m

response 16284

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	23.72
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025737.D
 Acq On : 29 Apr 2022 11:51
 Operator : SY/MD
 Sample : N2615-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

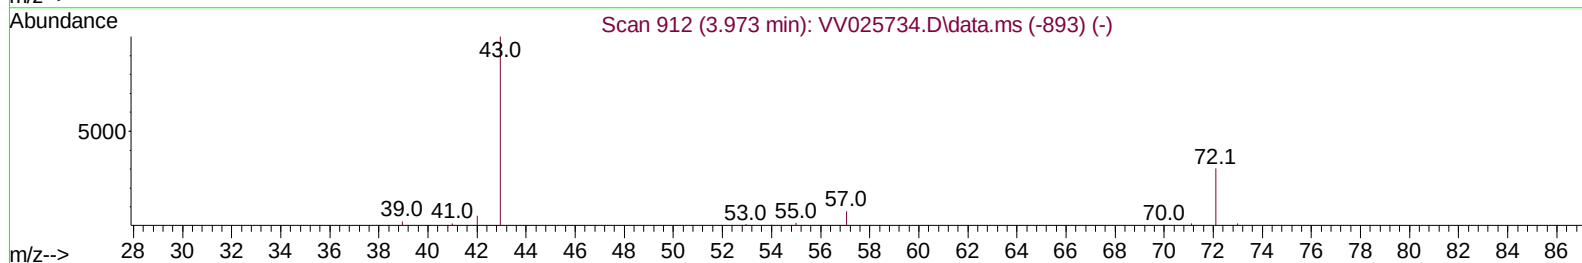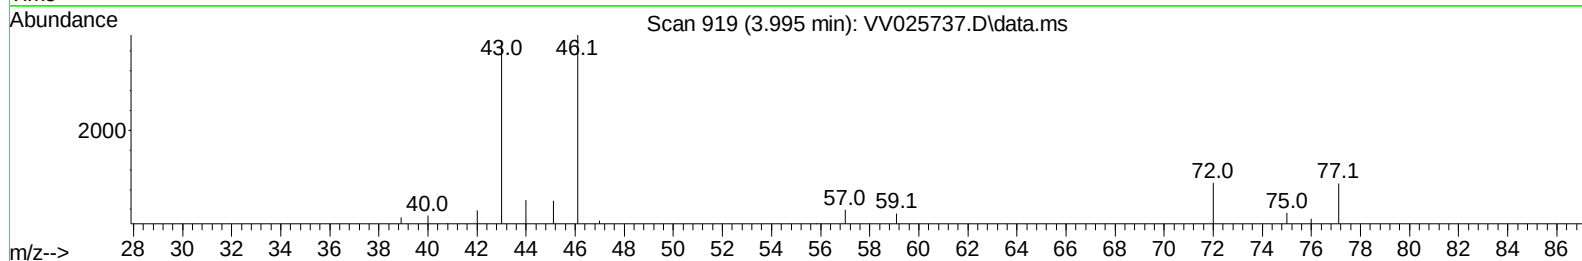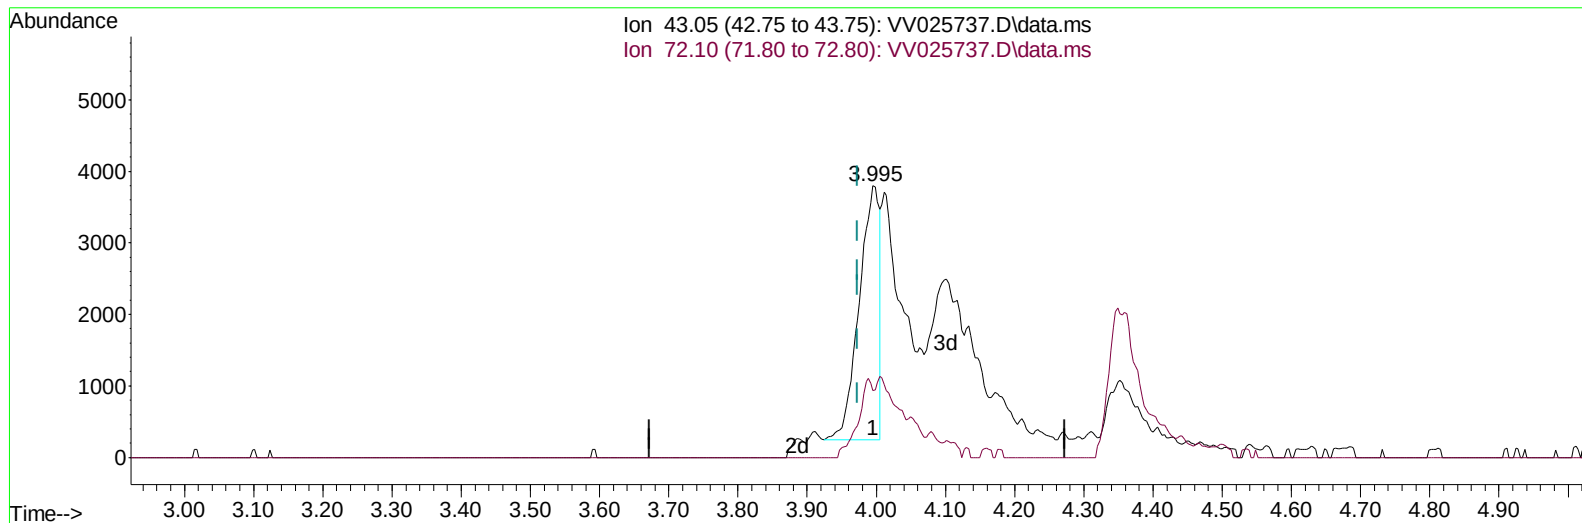

TIC: VV025737.D\data.ms

(21) 2-Butanone (T)

3.995min (+ 0.022) 4.14 ug/L

response 7203

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	22.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025737.D
 Acq On : 29 Apr 2022 11:51
 Operator : SY/MD
 Sample : N2615-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

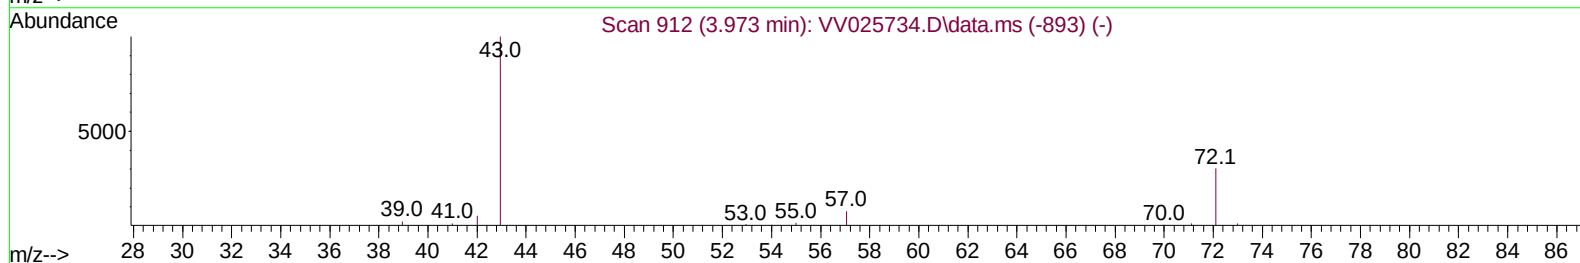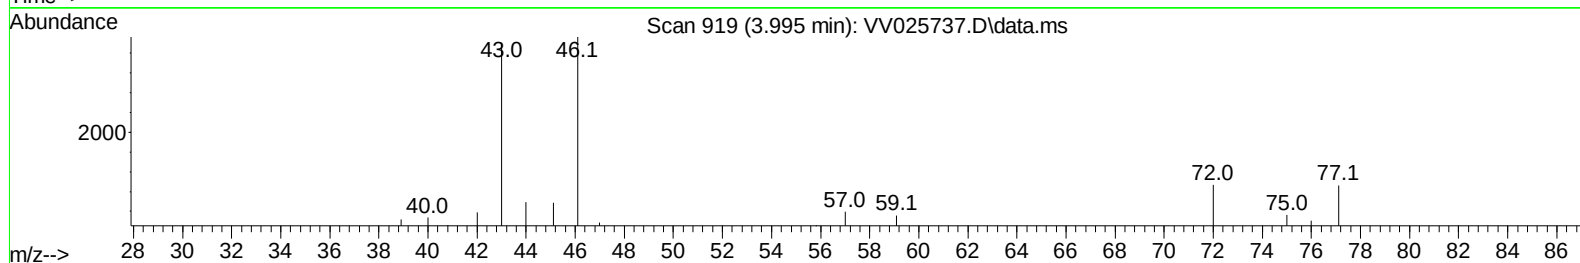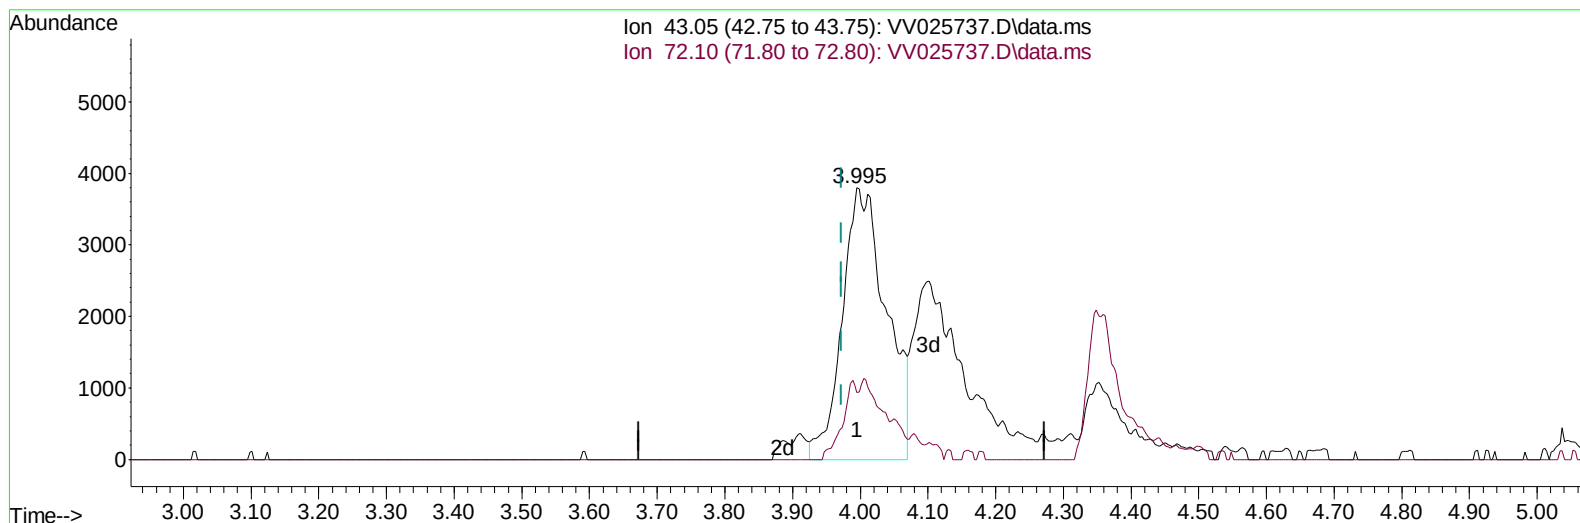

TIC: VV025737.D\data.ms

(21) 2-Butanone (T)

3.995min (+ 0.022) 9.88 ug/L m

response 17172

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	30.40	9.53#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025737.D
 Acq On : 29 Apr 2022 11:51
 Operator : SY/MD
 Sample : N2615-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 05/04/2022
 Supervised By : Mahesh Dadoda 05/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	163949	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	172491	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	80231	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56963	3.737	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	74.800%	
7) Chloroethane-d5	1.568	69	59649	3.678	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	73.600%	
11) 1,1-Dichloroethene-d2	2.108	63	92417	3.027	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	60.600%	
20) 2-Butanone-d5	3.895	46	110814	59.767	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	119.540%	
24) Chloroform-d	4.346	84	115758	5.026	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.600%	
26) 1,2-Dichloroethane-d4	5.034	65	54143	5.456	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	109.200%	
32) Benzene-d6	5.050	84	221157	4.431	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	88.600%	
36) 1,2-Dichloropropane-d6	6.069	67	70078	5.035	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	100.600%	
41) Toluene-d8	7.313	98	183521	3.962	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	79.200%	
43) trans-1,3-Dichloroprop...	7.625	79	19845	4.242	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	84.800%	
46) 2-Hexanone-d5	8.088	63	79526	48.434	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	96.860%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	41352	4.703	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	94.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	67910	5.048	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	101.000%	
Target Compounds						
					Qvalue	
13) Acetone	2.188	43	16284m	12.940	ug/L	
16) Methylene chloride	2.510	84	3234	0.235	ug/L	95
21) 2-Butanone	3.995	43	17172m	9.875	ug/L	
25) Chloroform	4.371	83	5605	0.263	ug/L	99
33) Benzene	5.101	78	18547	0.364	ug/L	100
42) Toluene	7.390	91	34104	0.615	ug/L	100
52) Ethylbenzene	9.021	91	2861	0.048	ug/L	95
53) m,p-Xylene	9.143	106	3874	0.172	ug/L	92
54) o-Xylene	9.548	106	3054	0.140	ug/L	100
62) 1,3,5-Trimethylbenzene	10.545	105	1136	0.051	ug/L	88
63) 1,2,4-Trimethylbenzene	10.918	105	5234	0.131	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025737.D
Acq On : 29 Apr 2022 11:51
Operator : SY/MD
Sample : N2615-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D5

Manual IntegrationsAPPROVED

Quant Time: May 02 01:23:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon May 02 01:22:31 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

