

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042922\
 Data File : VW025747.D
 Acq On : 29 Apr 2022 15:46
 Operator : SY/MD
 Sample : N2612-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0B2

Quant Time: May 02 01:25:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	149687	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	153818	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69832	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	49264	3.540	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	70.800%	
7) Chloroethane-d5	1.571	69	54138	3.657	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	73.200%	
11) 1,1-Dichloroethene-d2	2.114	63	80271	2.879	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	57.600%#	
20) 2-Butanone-d5	3.895	46	105047	62.055	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	124.100%	
24) Chloroform-d	4.352	84	106490	5.064	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
26) 1,2-Dichloroethane-d4	5.034	65	49154	5.425	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	108.400%	
32) Benzene-d6	5.053	84	195827	4.400	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.000%	
36) 1,2-Dichloropropane-d6	6.072	67	63660	5.129	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.600%	
41) Toluene-d8	7.317	98	162245	3.928	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.600%	
43) trans-1,3-Dichloroprop...	7.625	79	16371	3.924	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.400%	
46) 2-Hexanone-d5	8.088	63	73572	50.248	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.500%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	42640	5.438	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	108.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	59072	5.045	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.000%	
Target Compounds						Qvalue
14) Carbon disulfide	2.301	76	4573	0.147	ug/L #	91
17) Methyl tert-butyl Ether	2.773	73	1798	0.089	ug/L #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025747.D
Acq On : 29 Apr 2022 15:46
Operator : SY/MD
Sample : N2612-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0B2

Quant Time: May 02 01:25:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon May 02 01:22:31 2022
Response via : Initial Calibration




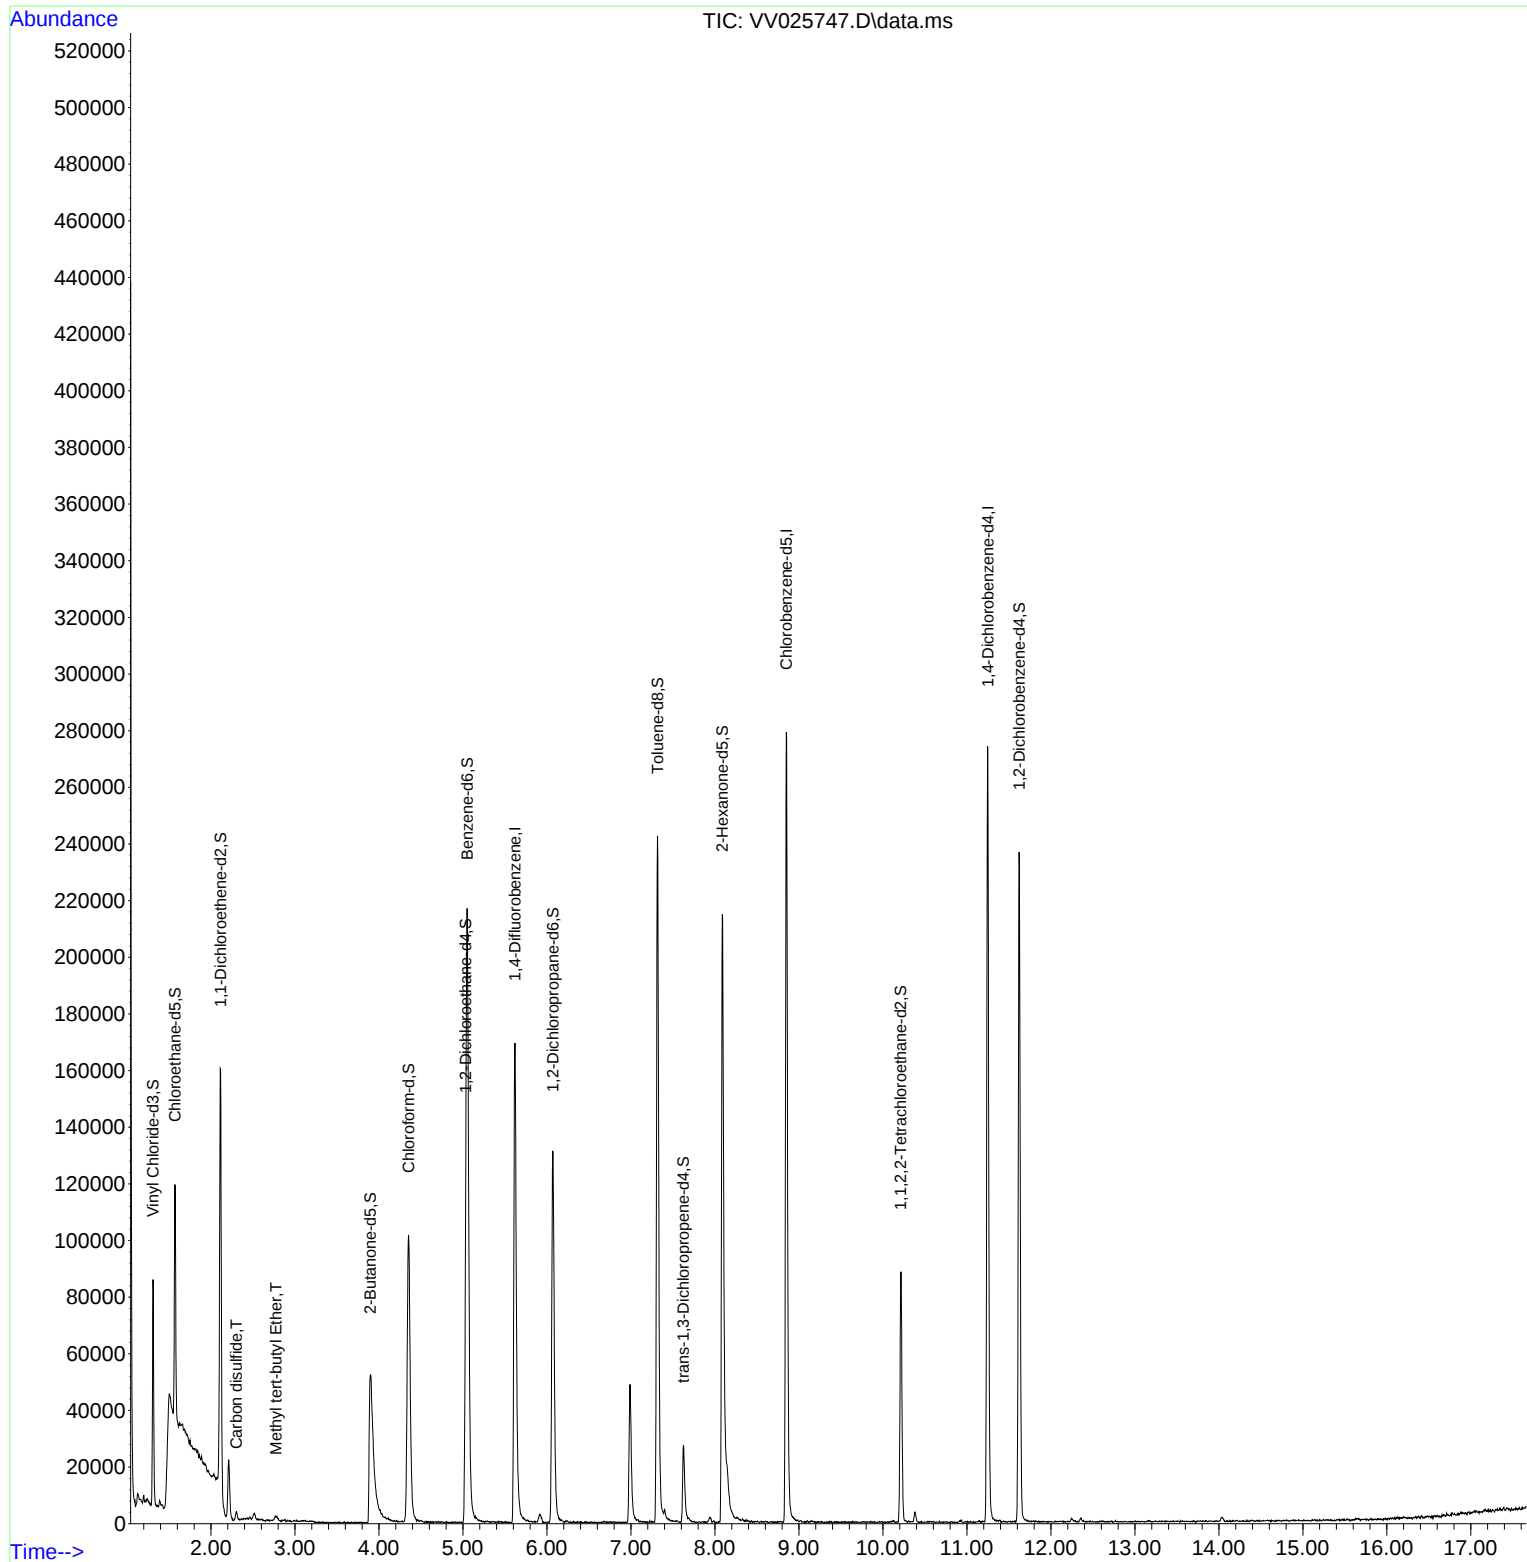


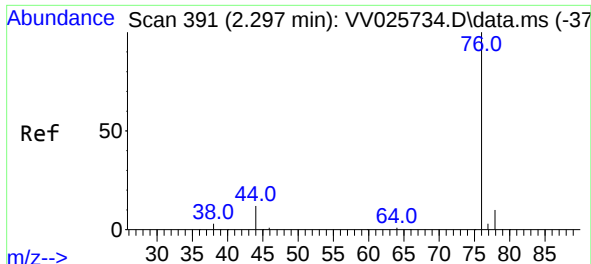

#14
Carbon disulfide
Concen: 0.147 ug/L
RT: 2.301 min Scan# 391
Delta R.T. 0.003 min
Lab File: VV025747.D
Acq: 29 Apr 2022 15:46

Instrument :
MSVOA_V
ClientSampleId :
BH0B2

Tgt Ion: 76 Resp: 4573
Ion Ratio Lower Upper
76 100
78 12.4 7.3 10.9#

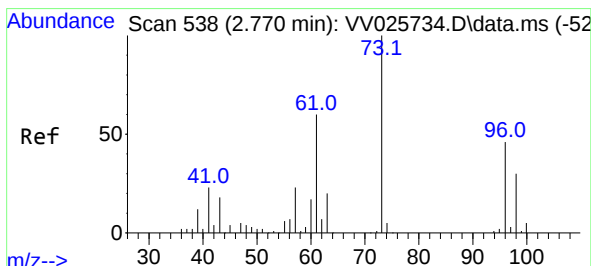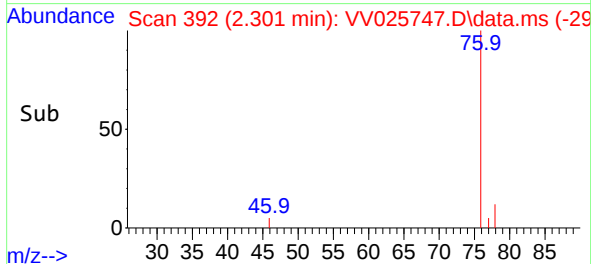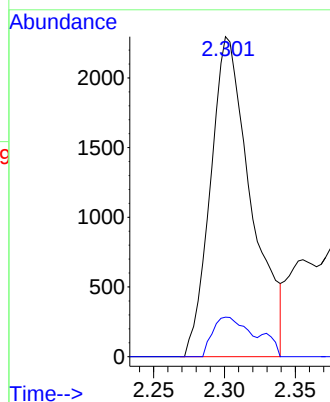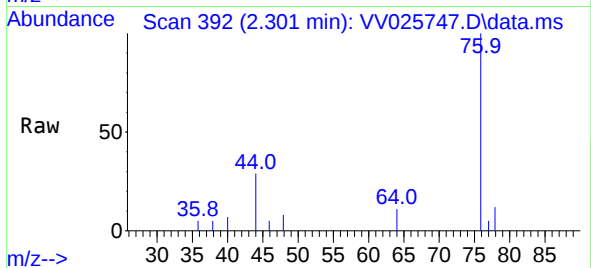

#17
Methyl tert-butyl Ether
Concen: 0.089 ug/L
RT: 2.773 min Scan# 539
Delta R.T. 0.003 min
Lab File: VV025747.D
Acq: 29 Apr 2022 15:46

Tgt Ion: 73 Resp: 1798
Ion Ratio Lower Upper
73 100
43 17.4 14.2 21.4
57 11.5 16.1 24.1#

