

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042922\
 Data File : VW025754.D
 Acq On : 29 Apr 2022 18:30
 Operator : SY/MD
 Sample : N2612-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D1

Quant Time: May 02 01:27:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon May 02 01:22:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	152291	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	157817	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71243	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	50368	3.557	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.200%
7) Chloroethane-d5	1.571	69	54236	3.601	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	72.000%
11) 1,1-Dichloroethene-d2	2.111	63	81127	2.860	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.200%#
20) 2-Butanone-d5	3.895	46	104929	60.925	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.860%
24) Chloroform-d	4.355	84	107888	5.043	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.800%
26) 1,2-Dichloroethane-d4	5.034	65	50762	5.506	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.200%
32) Benzene-d6	5.053	84	200287	4.386	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	6.069	67	64248	5.045	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.000%
41) Toluene-d8	7.317	98	164950	3.893	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.800%
43) trans-1,3-Dichloroprop...	7.625	79	17480	4.084	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.600%
46) 2-Hexanone-d5	8.088	63	75481	50.245	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.500%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	43515	5.409	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	59782	5.005	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.000%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.979	164	5488	0.566	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025754.D
Acq On : 29 Apr 2022 18:30
Operator : SY/MD
Sample : N2612-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D1

Quant Time: May 02 01:27:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon May 02 01:22:31 2022
Response via : Initial Calibration

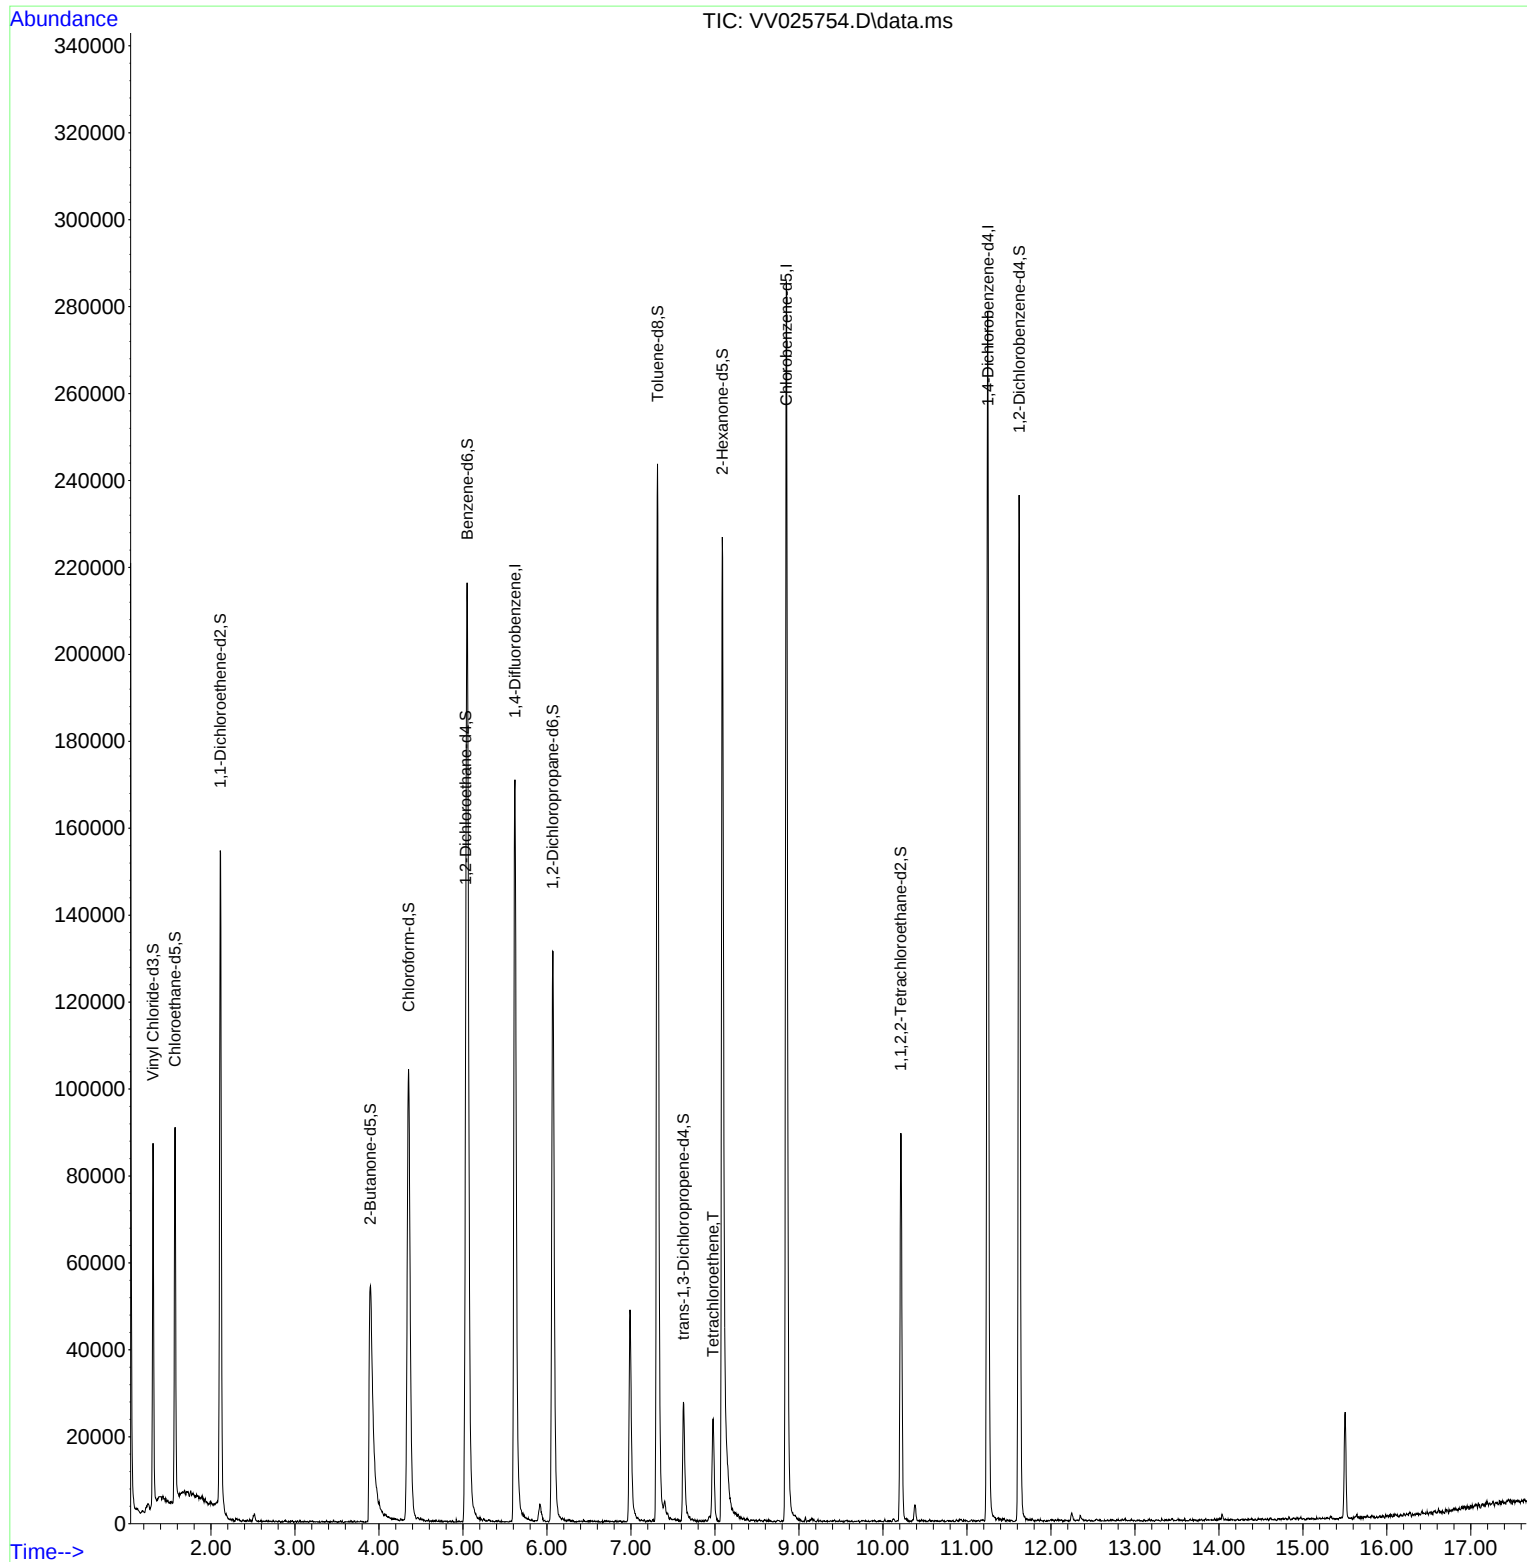

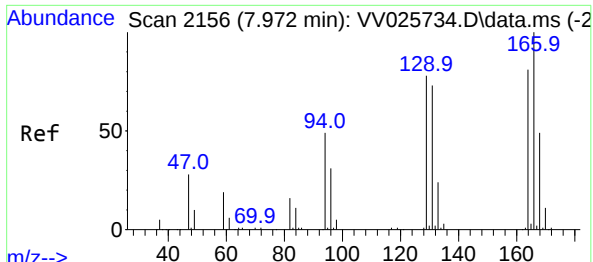

#47
Tetrachloroethene
Concen: 0.566 ug/L
RT: 7.979 min Scan# 21
Delta R.T. 0.006 min
Lab File: VV025754.D
Acq: 29 Apr 2022 18:30

Instrument :
MSVOA_V
ClientSampleId :
BH0D1

Tgt Ion:164 Resp: 5488

Ion	Ratio	Lower	Upper
164	100		
129	97.3	66.8	124.2
131	87.6	66.4	123.4
166	120.7	91.7	170.3

