

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025740.D
 Acq On : 29 Apr 2022 13:02
 Operator : SY/MD
 Sample : N2612-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH096

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	74	84	95	rBV	89957	90414	15.95%	1.945%
2	1.571	157	165	180	rBV	96165	109300	19.28%	2.352%
3	2.111	321	333	355	rVB	161927	242558	42.78%	5.219%
4	3.892	878	887	928	rBV	56318	179642	31.68%	3.865%
5	4.352	1014	1030	1054	rBV	106319	264691	46.68%	5.695%
6	5.050	1231	1247	1270	rBV2	225839	567000	100.00%	12.200%
7	5.619	1411	1424	1449	rBV2	178009	367257	64.77%	7.902%
8	5.911	1503	1515	1526	rBV8	6338	13624	2.40%	0.293%
9	6.069	1550	1564	1586	rBV2	134328	278531	49.12%	5.993%
10	6.989	1840	1850	1876	rBV2	55039	105283	18.57%	2.265%
11	7.317	1941	1952	1971	rBV	261255	459245	81.00%	9.882%
12	7.625	2038	2048	2064	rBV2	30266	56618	9.99%	1.218%
13	7.937	2138	2145	2155	rBV3	4092	7216	1.27%	0.155%
14	8.088	2182	2192	2223	rBV	218712	438580	77.35%	9.437%
15	8.850	2418	2429	2458	rBV	287165	484091	85.38%	10.416%
16	10.214	2842	2853	2871	rBV	83827	134766	23.77%	2.900%
17	10.381	2896	2905	2917	rVB4	9905	15756	2.78%	0.339%
18	11.246	3164	3174	3196	rBV	280938	444414	78.38%	9.562%
19	11.622	3279	3291	3308	rBV	240454	380632	67.13%	8.190%
20	12.249	3476	3486	3500	rVB3	4654	7878	1.39%	0.170%




Sum of corrected areas: 4647496

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025740.D
Acq On : 29 Apr 2022 13:02
Operator : SY/MD
Sample : N2612-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

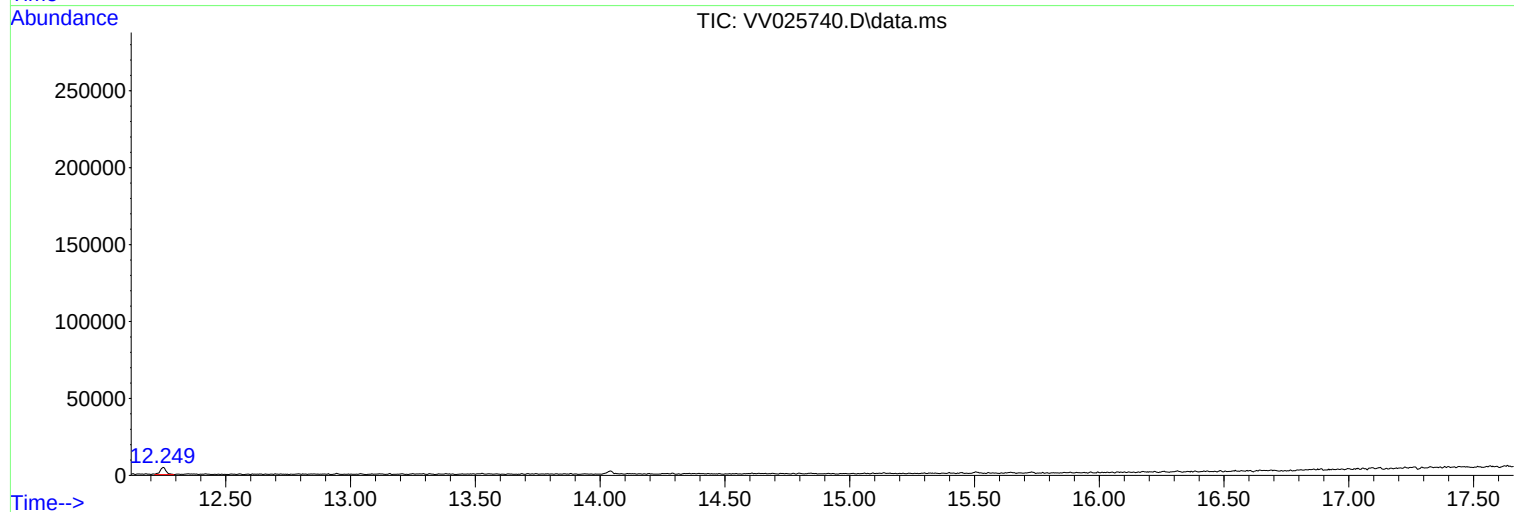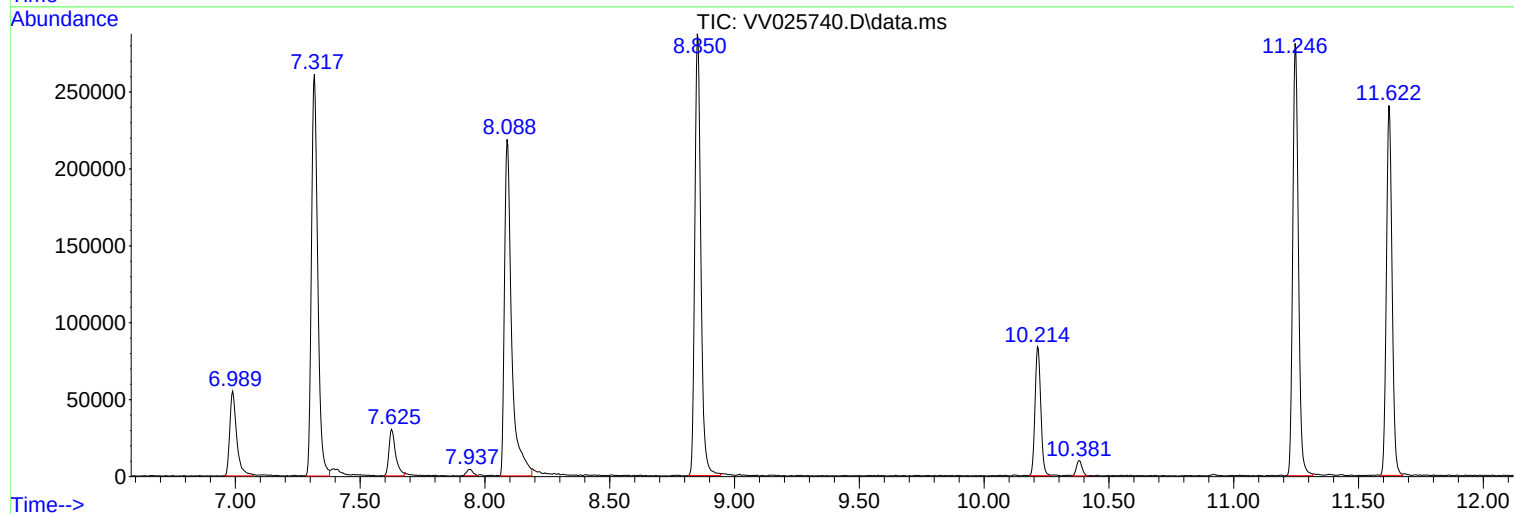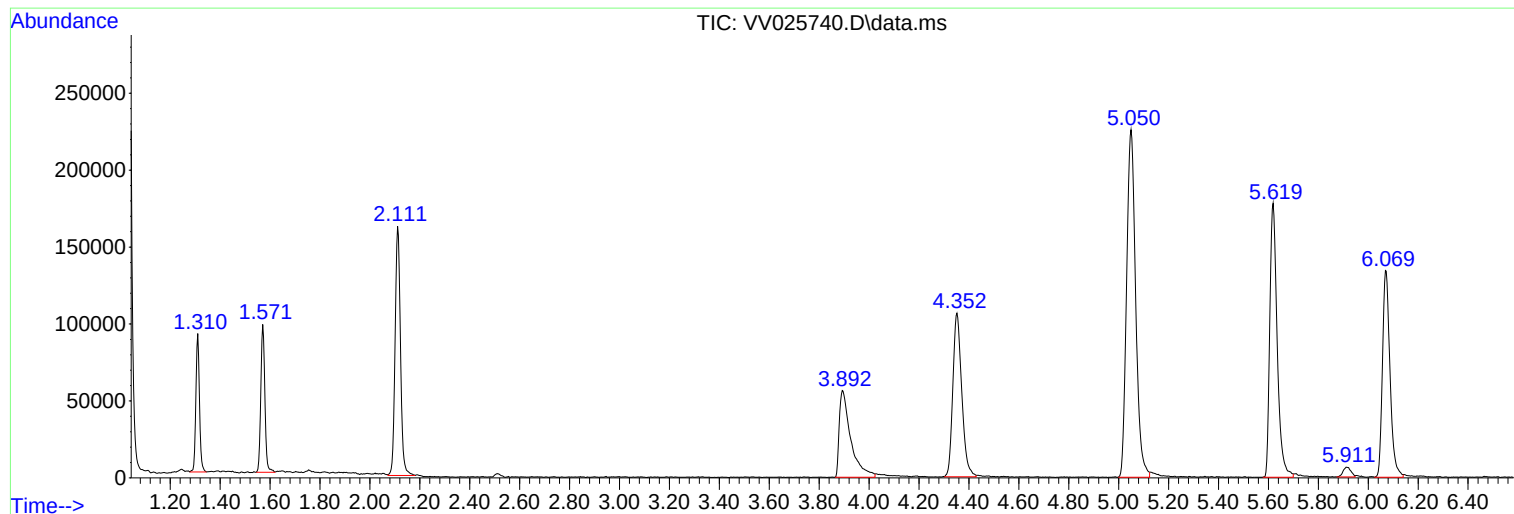

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025740.D
Acq On : 29 Apr 2022 13:02
Operator : SY/MD
Sample : N2612-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025740.D
Acq On : 29 Apr 2022 13:02
Operator : SY/MD
Sample : N2612-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH096

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc