

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025752.D
 Acq On : 29 Apr 2022 17:43
 Operator : SY/MD
 Sample : N2612-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	97	rBV	82943	87072	15.65%	1.711%
2	1.571	158	165	175	rBV	90755	106496	19.14%	2.093%
3	2.111	323	333	353	rVB	153828	232609	41.81%	4.572%
4	2.513	449	458	467	rVB6	3176	5629	1.01%	0.111%
5	3.908	876	892	923	rBV3	99929	343603	61.76%	6.753%
6	4.352	1013	1030	1055	rBV	104199	263012	47.27%	5.169%
7	5.050	1231	1247	1276	rBV2	220731	556364	100.00%	10.935%
8	5.619	1412	1424	1449	rBV	176405	365089	65.62%	7.176%
9	5.921	1506	1518	1538	rBV6	17411	38723	6.96%	0.761%
10	6.069	1552	1564	1587	rBV2	130813	272292	48.94%	5.352%
11	6.989	1838	1850	1868	rBV	49060	92928	16.70%	1.826%
12	7.316	1940	1952	1974	rBV	246980	434793	78.15%	8.546%
13	7.625	2036	2048	2069	rBV2	27710	51664	9.29%	1.015%
14	7.976	2140	2157	2177	rBV	197687	332691	59.80%	6.539%
15	8.088	2183	2192	2229	rBV	225559	449158	80.73%	8.828%
16	8.850	2418	2429	2456	rBV	290265	481415	86.53%	9.462%
17	10.213	2841	2853	2871	rBV	90146	144755	26.02%	2.845%
18	10.381	2897	2905	2914	rVB4	4371	6994	1.26%	0.137%
19	11.249	3162	3175	3194	rBV	284350	445791	80.13%	8.762%
20	11.622	3278	3291	3308	rBV	238454	376868	67.74%	7.407%




Sum of corrected areas: 5087946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025752.D
Acq On : 29 Apr 2022 17:43
Operator : SY/MD
Sample : N2612-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

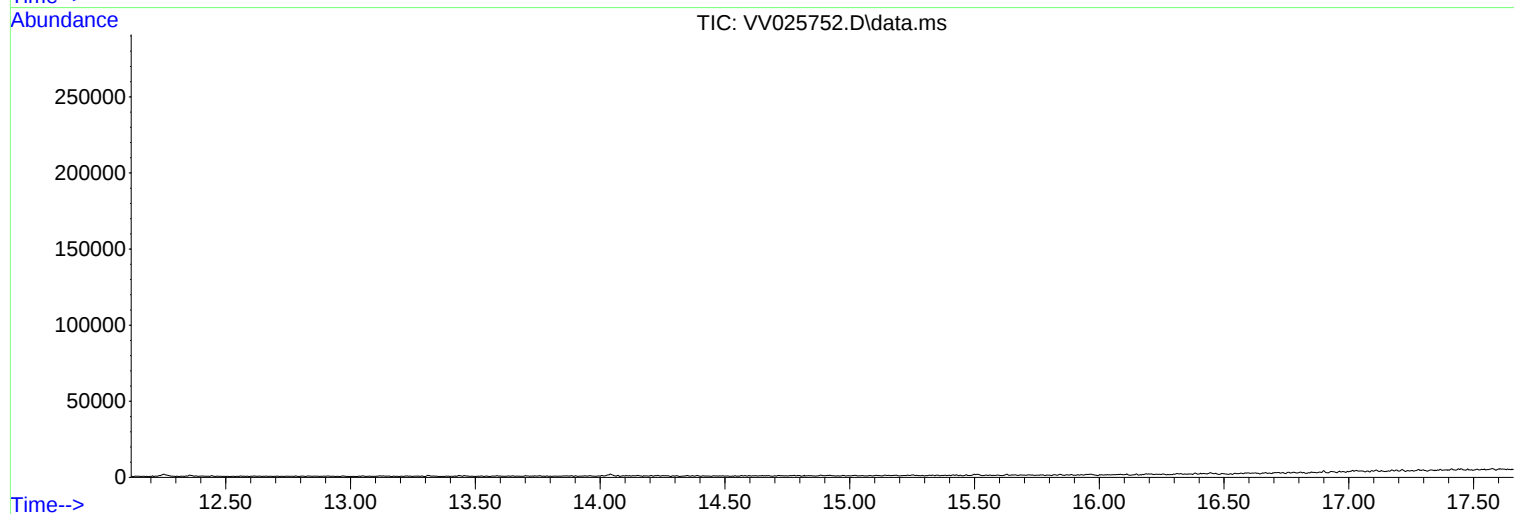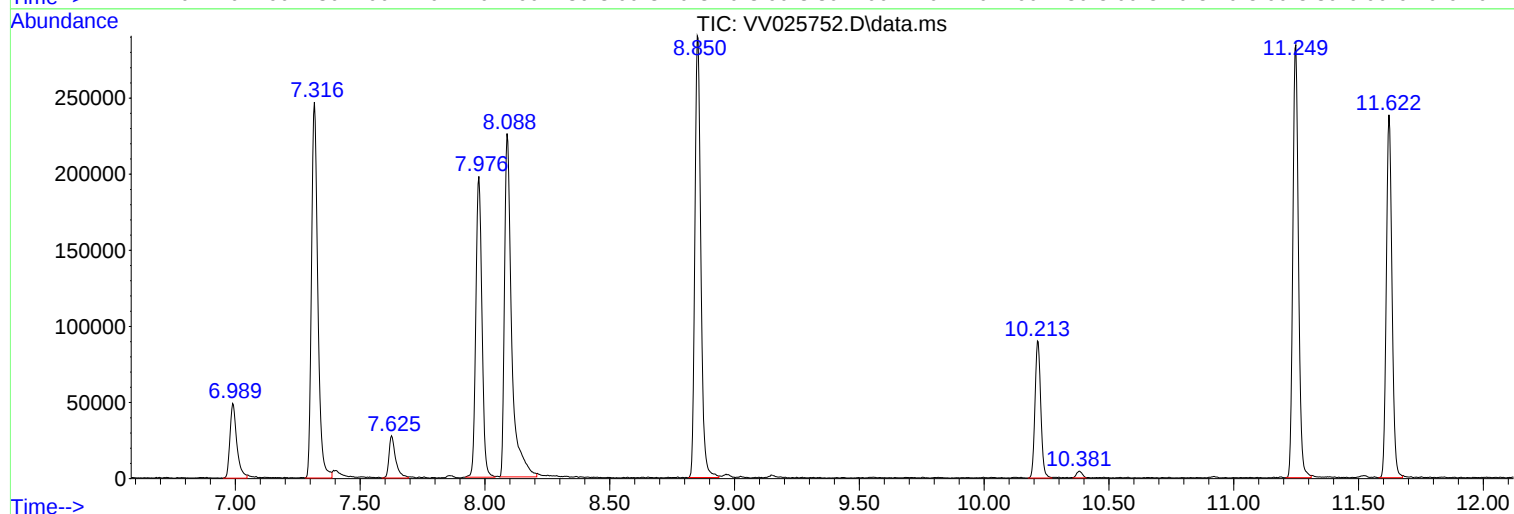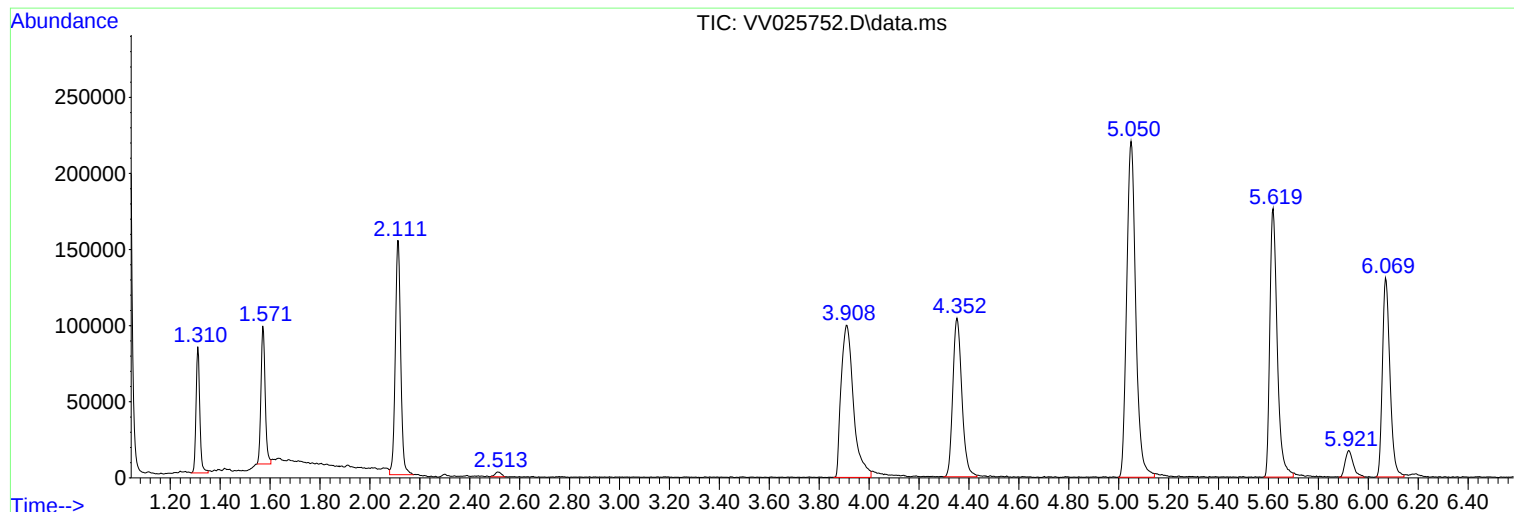

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025752.D
Acq On : 29 Apr 2022 17:43
Operator : SY/MD
Sample : N2612-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025752.D
Acq On : 29 Apr 2022 17:43
Operator : SY/MD
Sample : N2612-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc