

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025754.D
 Acq On : 29 Apr 2022 18:30
 Operator : SY/MD
 Sample : N2612-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	97	rBV	83493	85329	15.53%	1.867%
2	1.574	157	166	181	rBV	86465	102348	18.63%	2.239%
3	2.111	323	333	354	rVB	152917	228641	41.61%	5.003%
4	3.899	879	889	918	rBV2	54233	175464	31.94%	3.839%
5	4.352	1014	1030	1059	rBV2	103643	257773	46.92%	5.640%
6	5.050	1231	1247	1278	rBV2	216092	549430	100.00%	12.022%
7	5.619	1412	1424	1450	rBV	170623	354969	64.61%	7.767%
8	5.915	1506	1516	1529	rVB7	3924	8344	1.52%	0.183%
9	6.069	1549	1564	1585	rBV	131366	272602	49.62%	5.965%
10	6.989	1837	1850	1869	rBV2	48789	92775	16.89%	2.030%
11	7.317	1940	1952	1973	rBV	243308	434124	79.01%	9.499%
12	7.625	2039	2048	2061	rBV	27330	49060	8.93%	1.073%
13	7.979	2148	2158	2172	rVB2	23288	40880	7.44%	0.894%
14	8.088	2182	2192	2228	rBV	226559	452389	82.34%	9.899%
15	8.850	2418	2429	2451	rBV	285141	472453	85.99%	10.338%
16	10.214	2843	2853	2868	rBV	89279	141887	25.82%	3.105%
17	10.381	2899	2905	2916	rVB3	3699	5649	1.03%	0.124%
18	11.249	3163	3175	3195	rBV	278278	437795	79.68%	9.579%
19	11.622	3280	3291	3310	rBV	235914	371968	67.70%	8.139%
20	15.503	4488	4498	4511	rVB2	24395	36370	6.62%	0.796%




Sum of corrected areas: 4570250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025754.D
Acq On : 29 Apr 2022 18:30
Operator : SY/MD
Sample : N2612-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

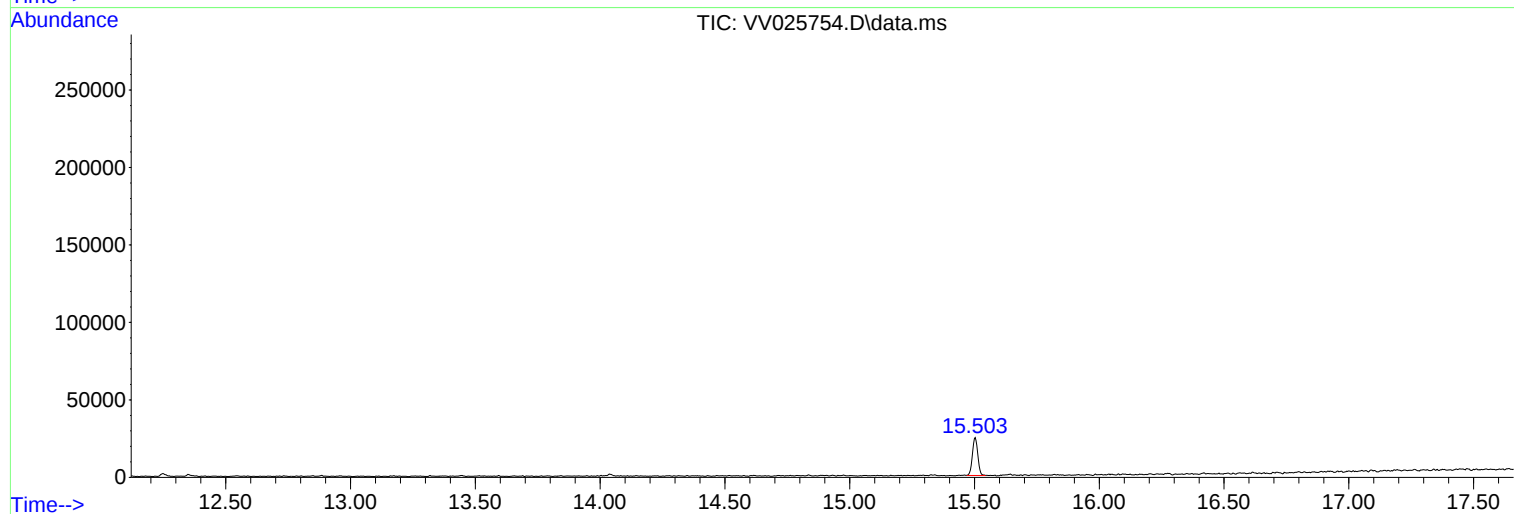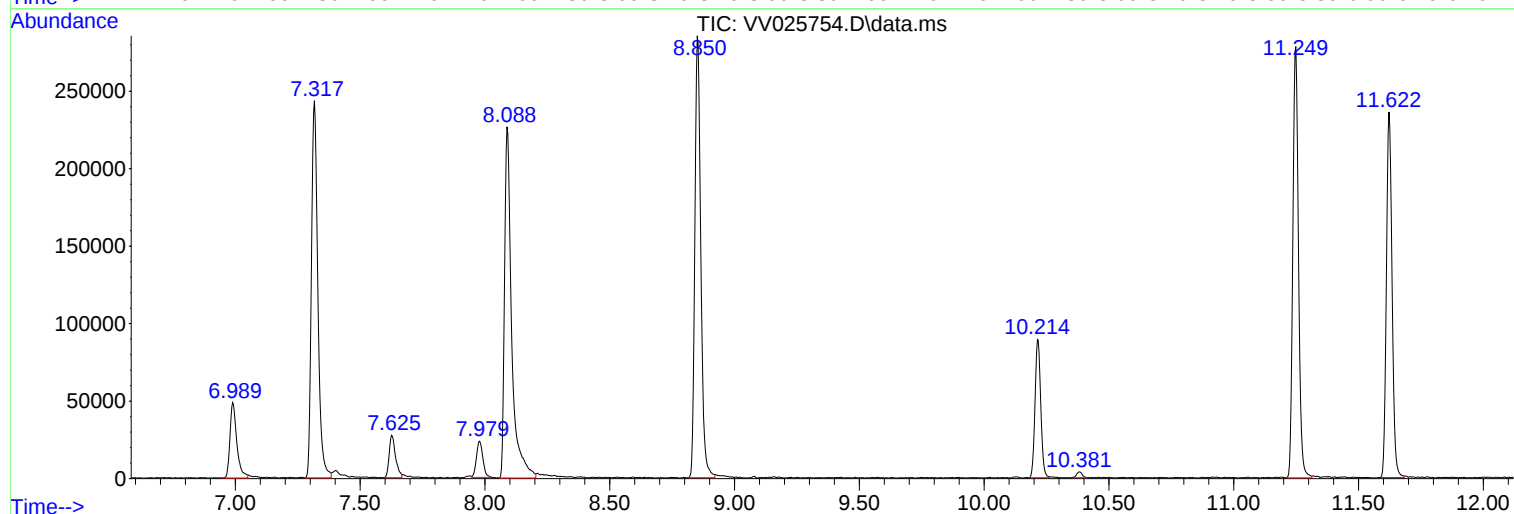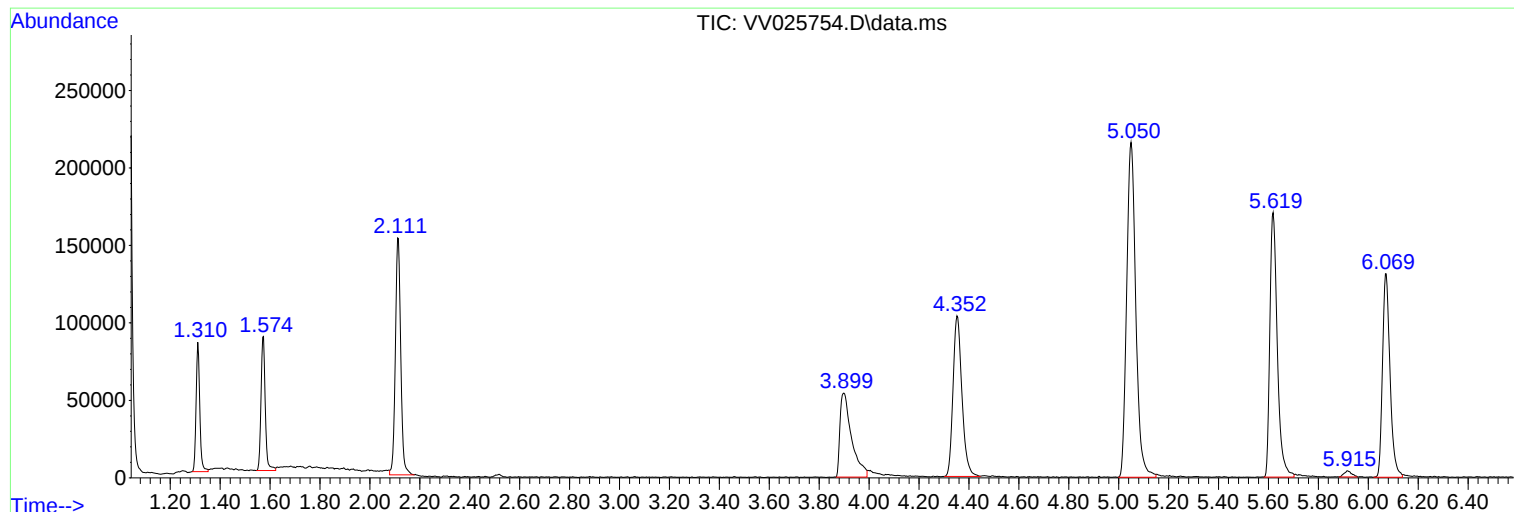

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025754.D
Acq On : 29 Apr 2022 18:30
Operator : SY/MD
Sample : N2612-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025754.D
Acq On : 29 Apr 2022 18:30
Operator : SY/MD
Sample : N2612-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc