

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
 Data File : VV025755.D
 Acq On : 29 Apr 2022 18:54
 Operator : SY/MD
 Sample : N2612-22
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0D3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	94	rBV	80678	80316	14.79%	1.602%
2	1.571	157	165	177	rBV	86675	104043	19.16%	2.075%
3	2.111	324	333	351	rVB	152441	228024	41.98%	4.547%
4	3.912	879	893	923	rBV3	99560	325676	59.96%	6.495%
5	4.352	1013	1030	1054	rBV	101085	253324	46.64%	5.052%
6	5.050	1232	1247	1278	rBV2	213868	543145	100.00%	10.832%
7	5.619	1411	1424	1455	rBV	177539	365717	67.33%	7.293%
8	5.921	1506	1518	1537	rBV6	18005	40854	7.52%	0.815%
9	6.069	1550	1564	1584	rBV	129370	269525	49.62%	5.375%
10	6.989	1839	1850	1873	rBV	46555	89704	16.52%	1.789%
11	7.317	1941	1952	1971	rBV	249050	430648	79.29%	8.588%
12	7.625	2038	2048	2073	rBV	26414	50000	9.21%	0.997%
13	7.976	2145	2157	2176	rVB	200482	335428	61.76%	6.689%
14	8.088	2182	2192	2228	rBV	219220	440205	81.05%	8.779%
15	8.850	2418	2429	2451	rBV	287395	479959	88.37%	9.572%
16	10.214	2842	2853	2868	rBV	88839	141642	26.08%	2.825%
17	10.381	2896	2905	2914	rVB4	4648	7125	1.31%	0.142%
18	11.246	3164	3174	3199	rBV	292051	445470	82.02%	8.884%
19	11.622	3280	3291	3309	rBV	235798	373839	68.83%	7.455%
20	15.500	4490	4497	4506	rBV5	6659	9724	1.79%	0.194%




Sum of corrected areas: 5014368

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025755.D
Acq On : 29 Apr 2022 18:54
Operator : SY/MD
Sample : N2612-22
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

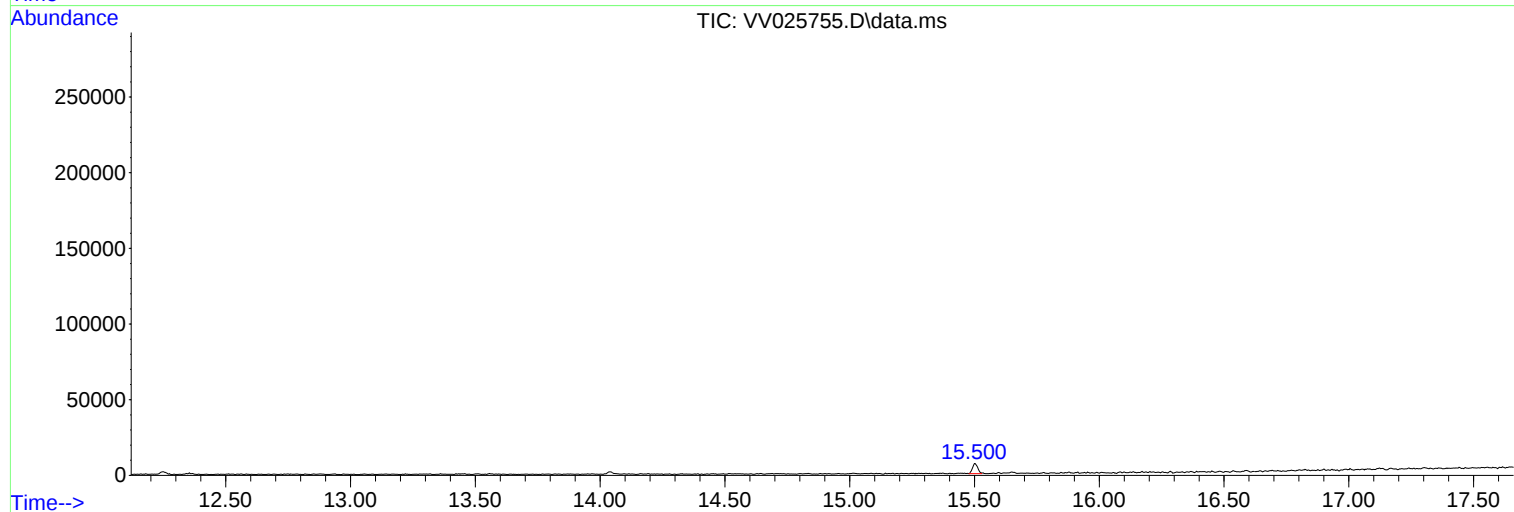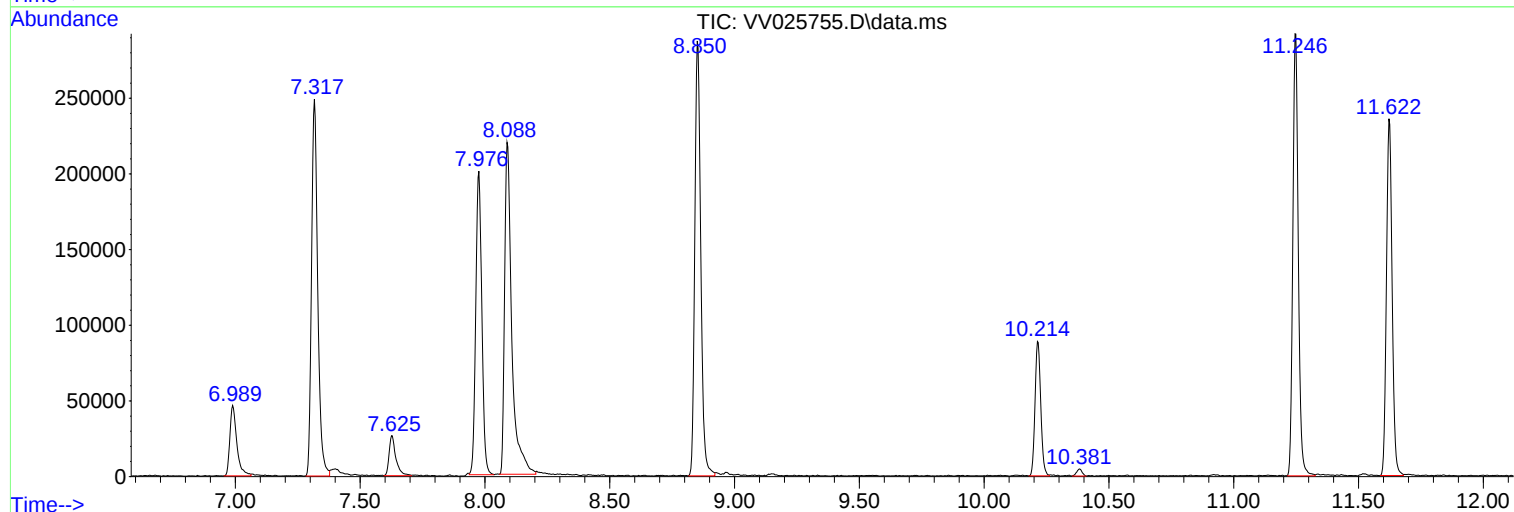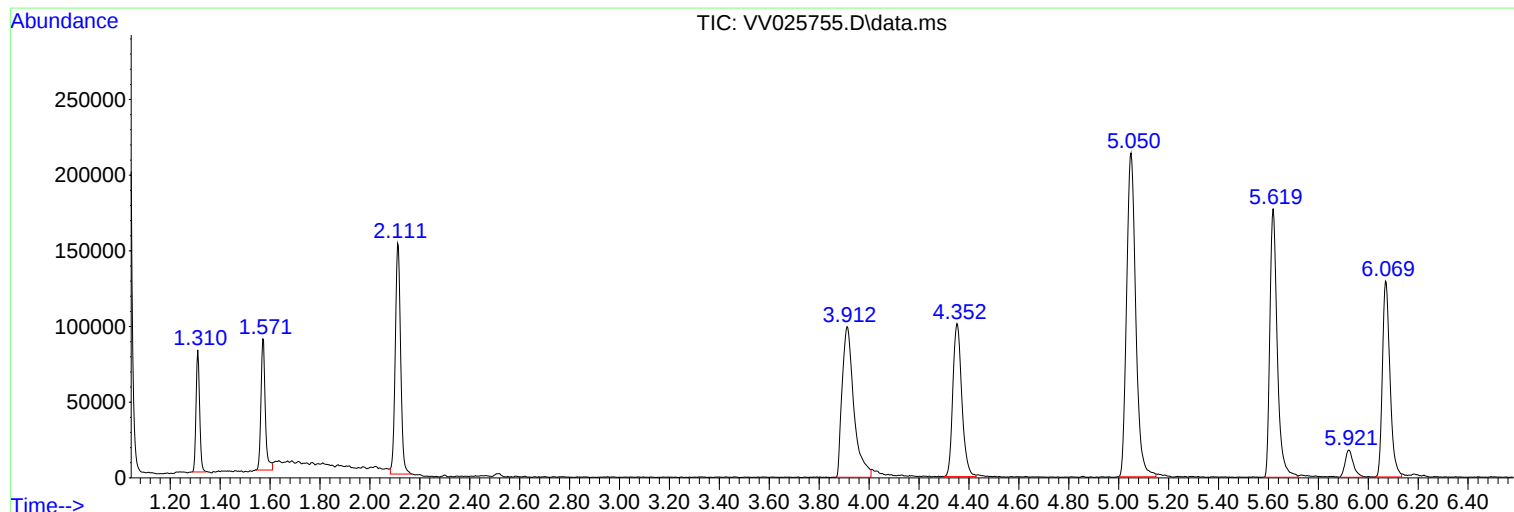

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025755.D
Acq On : 29 Apr 2022 18:54
Operator : SY/MD
Sample : N2612-22
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042922\
Data File : VV025755.D
Acq On : 29 Apr 2022 18:54
Operator : SY/MD
Sample : N2612-22
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0D3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc