

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035495.D
 Acq On : 01 May 2024 14:44
 Operator : SY/MD
 Sample : P2279-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ7

Quant Time: May 02 01:27:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 02 01:07:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	508174	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	485409	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	213930	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	179581	45.831	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.660%
7) Chloroethane-d5	1.526	69	132781	45.985	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.960%
11) 1,1-Dichloroethene-d2	2.053	65	77256	45.931	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.860%
21) 2-Butanone-d5	3.796	46	248324	93.904	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.900%
24) Chloroform-d	4.246	84	331556	46.132	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.260%
26) 1,2-Dichloroethane-d4	4.937	65	210039	49.624	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.240%
32) Benzene-d6	4.953	84	675705	49.455	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.900%
36) 1,2-Dichloropropane-d6	5.985	67	214302	50.304	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.600%
41) Toluene-d8	7.239	98	580991	46.716	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.440%
43) trans-1,3-Dichloroprop...	7.551	79	96626	46.538	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.080%
47) 2-Hexanone-d5	8.027	63	196047	100.143	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.140%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	314230	48.407	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.820%
66) 1,2-Dichlorobenzene-d4	11.558	152	223997	52.701	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.400%
Target Compounds						
					Qvalue	
3) Chloromethane	1.214	50	17139	4.647	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035495.D
Acq On : 01 May 2024 14:44
Operator : SY/MD
Sample : P2279-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ7

Quant Time: May 02 01:27:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 02 01:07:15 2024
Response via : Initial Calibration

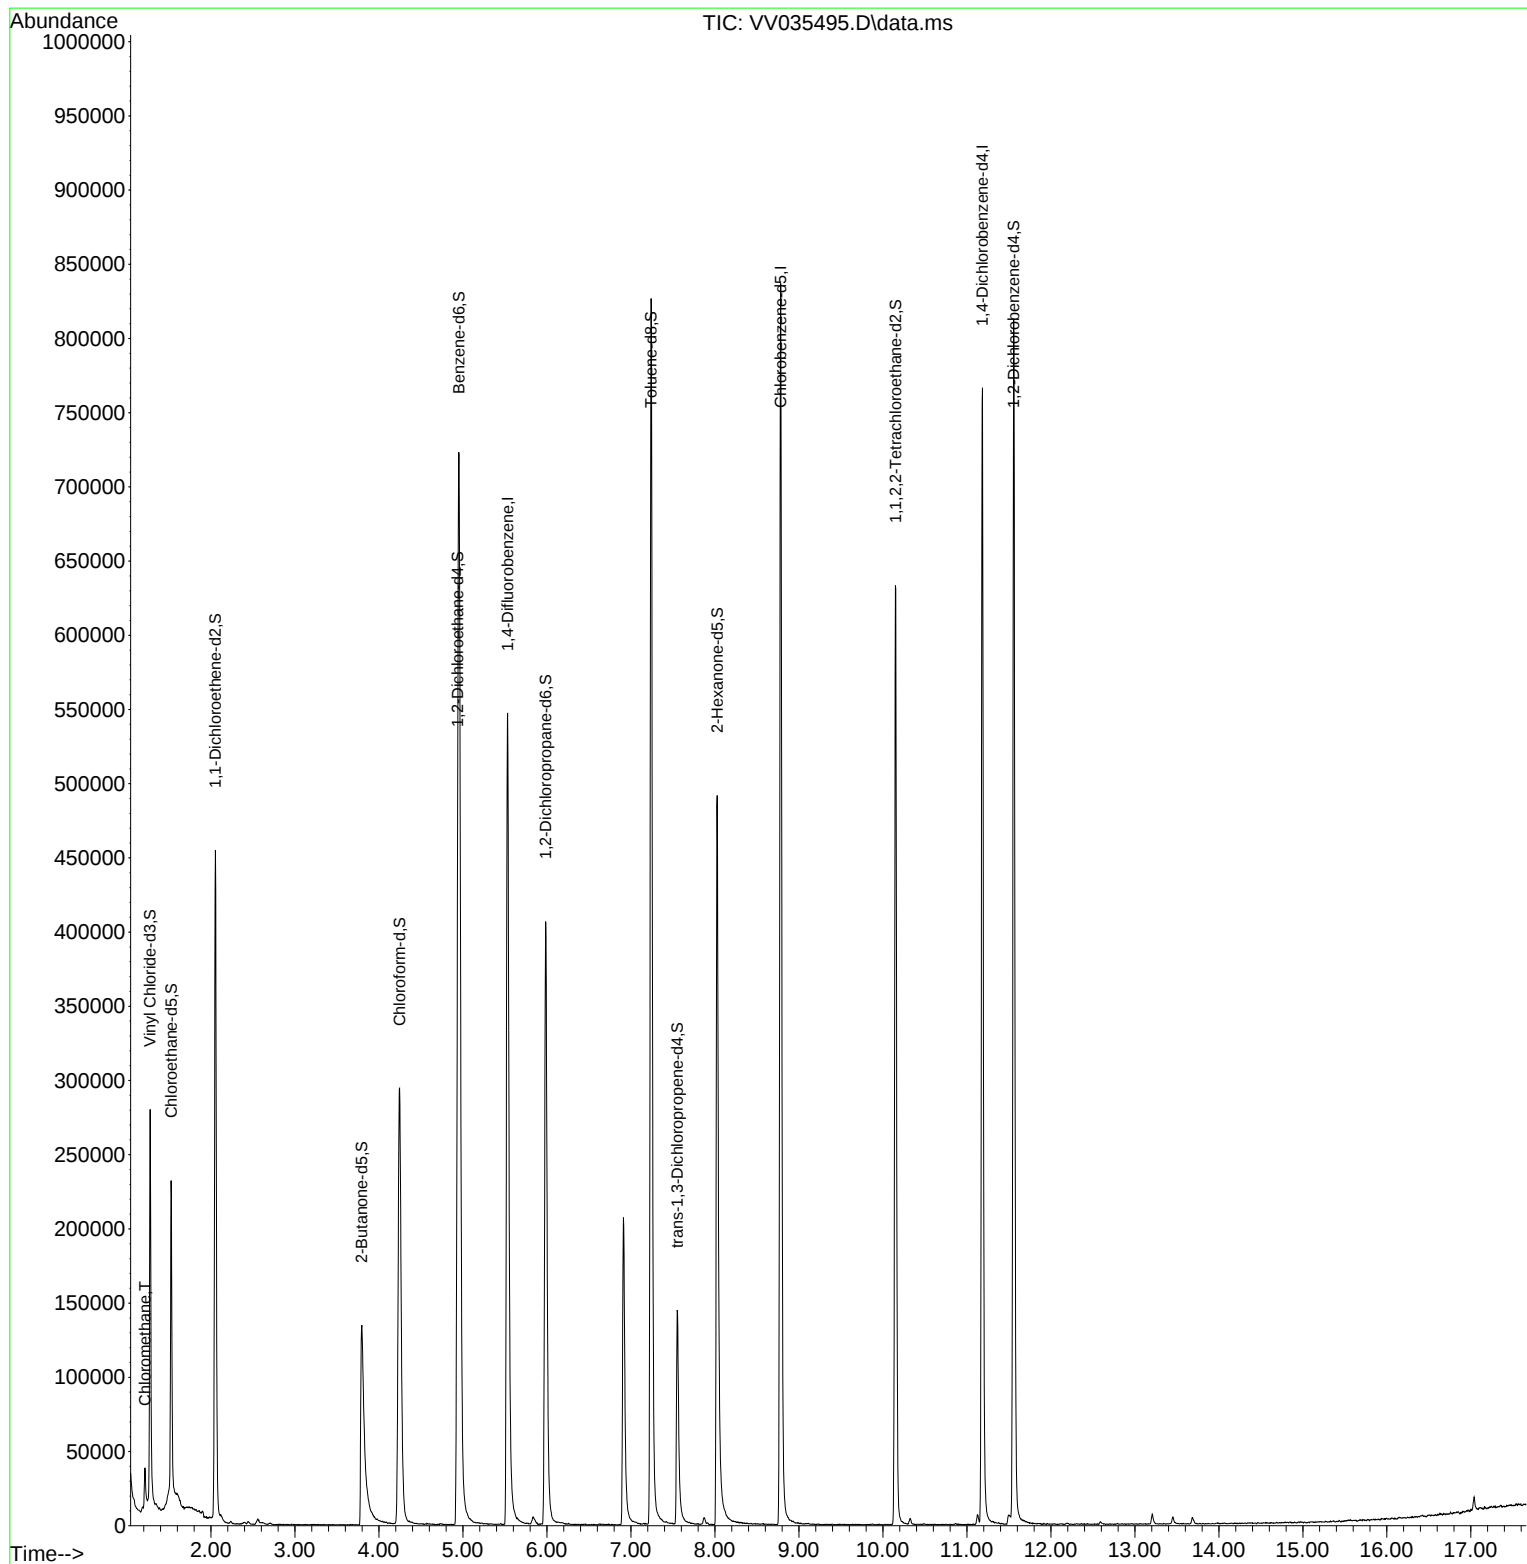

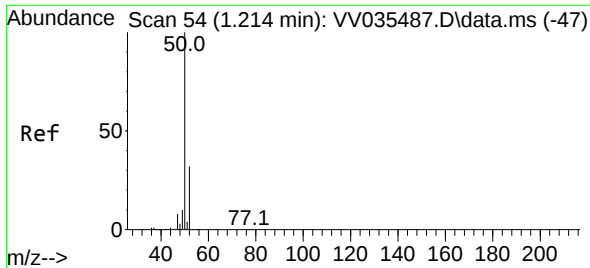

#3
 Chloromethane
 Concen: 4.647 ug/L
 RT: 1.214 min Scan# 54
 Delta R.T. -0.000 min
 Lab File: VV035495.D
 Acq: 01 May 2024 14:44

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ7

Tgt Ion: 50 Resp: 17139
 Ion Ratio Lower Upper
 50 100
 52 33.7 22.6 42.0

