

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035493.D
 Acq On : 01 May 2024 13:56
 Operator : SY/MD
 Sample : VV0501WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M

Title : VOC Analysis

Signal : TIC: VV035493.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	104	rVB	283457	328390	16.28%	2.159%
2	1.529	146	152	166	rVB	236418	263030	13.04%	1.729%
3	2.056	306	316	333	rVB	469642	681644	33.80%	4.482%
4	2.240	366	373	382	rVB	2843	4575	0.23%	0.030%
5	2.394	418	421	423	rBV	613	461	0.02%	0.003%
6	2.449	431	438	453	rVB3	4434	7147	0.35%	0.047%
7	2.532	461	464	467	rVB2	390	253	0.01%	0.002%
8	2.561	467	473	474	rBV2	524	423	0.02%	0.003%
9	2.648	496	500	504	rBV3	287	256	0.01%	0.002%
10	2.703	511	517	520	rBV4	1273	1272	0.06%	0.008%
11	3.024	611	617	619	rBV2	345	362	0.02%	0.002%
12	3.114	641	645	647	rBV4	377	280	0.01%	0.002%
13	3.513	766	769	775	rVV2	388	402	0.02%	0.003%
14	3.796	848	857	890	rBV	142391	425821	21.11%	2.800%
15	4.246	981	997	1031	rBV	311559	806617	39.99%	5.303%
16	4.478	1066	1069	1074	rBV4	500	463	0.02%	0.003%
17	4.651	1121	1123	1128	rVB3	366	243	0.01%	0.002%
18	4.728	1144	1147	1149	rBV2	330	252	0.01%	0.002%
19	4.815	1167	1174	1175	rBV2	388	370	0.02%	0.002%
20	4.953	1199	1217	1255	rBV2	770870	2016956	100.00%	13.261%
21	5.166	1280	1283	1287	rVB3	1109	837	0.04%	0.006%
22	5.188	1287	1290	1292	rBV4	645	304	0.02%	0.002%
23	5.439	1364	1368	1371	rVB3	419	407	0.02%	0.003%
24	5.461	1371	1375	1379	rBV4	492	394	0.02%	0.003%
25	5.532	1385	1397	1439	rBV	579520	1205937	59.79%	7.929%
26	5.764	1467	1469	1472	rVB3	609	271	0.01%	0.002%
27	5.838	1481	1492	1512	rBV8	6322	16509	0.82%	0.109%
28	5.985	1525	1538	1568	rBV	431300	899635	44.60%	5.915%
29	6.420	1670	1673	1678	rBV2	461	449	0.02%	0.003%
30	6.609	1727	1732	1735	rBV3	387	347	0.02%	0.002%
31	6.641	1738	1742	1744	rBV2	570	346	0.02%	0.002%
32	6.783	1779	1786	1788	rBV4	378	401	0.02%	0.003%
33	6.912	1813	1826	1862	rBV	225357	437616	21.70%	2.877%
34	7.149	1897	1900	1904	rBV4	406	305	0.02%	0.002%
35	7.188	1910	1912	1917	rVB2	674	575	0.03%	0.004%
36	7.239	1917	1928	1961	rBV	898058	1585730	78.62%	10.426%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035493.D
 Acq On : 01 May 2024 13:56
 Operator : SY/MD
 Sample : VV0501WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	7.506	2009	2011	2015	rBV2	410	343	0.02%	0.002%
38	7.551	2015	2025	2055	rBV	154590	295016	14.63%	1.940%
39	7.773	2092	2094	2098	rVB5	515	332	0.02%	0.002%
40	7.821	2107	2109	2113	rVB3	486	303	0.02%	0.002%
41	7.870	2122	2124	2126	rBV	393	282	0.01%	0.002%
42	7.905	2132	2135	2136	rBV	857	408	0.02%	0.003%
43	7.915	2136	2138	2146	rVB5	1292	1145	0.06%	0.008%
44	8.027	2163	2173	2218	rBV	514822	981718	48.67%	6.454%
45	8.362	2270	2277	2278	rBV4	788	883	0.04%	0.006%
46	8.410	2290	2292	2296	rBV3	411	296	0.01%	0.002%
47	8.513	2320	2324	2326	rBV3	376	334	0.02%	0.002%
48	8.593	2345	2349	2352	rBV4	343	318	0.02%	0.002%
49	8.686	2376	2378	2383	rVB2	376	259	0.01%	0.002%
50	8.719	2385	2388	2392	rVB3	305	245	0.01%	0.002%
51	8.783	2397	2408	2434	rBV	875539	1440147	71.40%	9.468%
52	9.037	2485	2487	2490	rVB3	580	310	0.02%	0.002%
53	9.056	2490	2493	2497	rVB2	451	267	0.01%	0.002%
54	9.082	2497	2501	2503	rBV4	694	561	0.03%	0.004%
55	9.159	2520	2525	2526	rBV2	420	357	0.02%	0.002%
56	9.246	2551	2552	2557	rBV3	352	323	0.02%	0.002%
57	9.345	2580	2583	2590	rVB2	374	354	0.02%	0.002%
58	9.493	2623	2629	2635	rBV3	778	1222	0.06%	0.008%
59	9.751	2707	2709	2714	rVB2	323	248	0.01%	0.002%
60	9.873	2737	2747	2754	rBV4	1075	1812	0.09%	0.012%
61	9.972	2776	2778	2784	rVB2	340	282	0.01%	0.002%
62	10.149	2818	2833	2866	rBV	656606	1055504	52.33%	6.940%
63	10.368	2898	2901	2905	rVB2	696	469	0.02%	0.003%
64	10.484	2930	2937	2945	rBV6	1308	2143	0.11%	0.014%
65	10.551	2954	2958	2960	rBV	540	379	0.02%	0.002%
66	10.799	3033	3035	3042	rVB4	575	509	0.03%	0.003%
67	10.870	3051	3057	3063	rVV2	1332	1719	0.09%	0.011%
68	10.979	3087	3091	3096	rBV	278	318	0.02%	0.002%
69	11.124	3129	3136	3138	rBV3	2149	2060	0.10%	0.014%
70	11.181	3144	3154	3182	rBV	814349	1284467	63.68%	8.445%
71	11.480	3244	3247	3249	rBV4	475	263	0.01%	0.002%
72	11.558	3259	3271	3300	rBV	875593	1393704	69.10%	9.163%
73	11.879	3369	3371	3377	rVB3	533	413	0.02%	0.003%
74	11.911	3377	3381	3387	rVB5	457	481	0.02%	0.003%
75	11.972	3396	3400	3402	rBV3	314	245	0.01%	0.002%
76	11.988	3402	3405	3410	rVV3	556	476	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035493.D
 Acq On : 01 May 2024 13:56
 Operator : SY/MD
 Sample : VV0501WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M

Title : VOC Analysis

77	12.233	3476	3481	3484	rBV3	311	301	0.01%	0.002%
78	12.316	3505	3507	3510	rVB2	355	249	0.01%	0.002%
79	12.374	3516	3525	3529	rBV4	1078	1425	0.07%	0.009%
80	12.394	3529	3531	3534	rBV2	472	269	0.01%	0.002%
81	12.509	3561	3567	3569	rBV3	400	404	0.02%	0.003%
82	12.590	3586	3592	3607	rVB8	3178	5600	0.28%	0.037%
83	12.644	3607	3609	3615	rBV3	385	385	0.02%	0.003%
84	12.705	3626	3628	3631	rBV	401	248	0.01%	0.002%
85	12.776	3645	3650	3653	rBV4	505	473	0.02%	0.003%
86	12.796	3653	3656	3660	rVB4	623	518	0.03%	0.003%
87	12.818	3660	3663	3666	rBV2	385	355	0.02%	0.002%
88	12.876	3676	3681	3685	rBV2	438	462	0.02%	0.003%
89	13.021	3721	3726	3727	rBV2	387	321	0.02%	0.002%
90	13.207	3775	3784	3793	rBV4	5432	9033	0.45%	0.059%
91	13.448	3851	3859	3870	rBV	10204	17589	0.87%	0.116%
92	13.583	3898	3901	3905	rBV4	419	298	0.01%	0.002%
93	13.631	3910	3916	3918	rBV3	480	489	0.02%	0.003%
94	13.686	3925	3933	3942	rBV5	5337	9075	0.45%	0.060%
95	14.152	4075	4078	4081	rVB2	669	428	0.02%	0.003%
96	14.326	4130	4132	4138	rBV5	588	515	0.03%	0.003%
97	14.355	4138	4141	4142	rBV2	568	338	0.02%	0.002%
98	14.586	4211	4213	4216	rBV	461	295	0.01%	0.002%
99	14.702	4246	4249	4251	rBV3	534	310	0.02%	0.002%
100	14.808	4279	4282	4285	rBV4	773	465	0.02%	0.003%


Sum of corrected areas: 15210040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035493.D
Acq On : 01 May 2024 13:56
Operator : SY/MD
Sample : VV0501WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

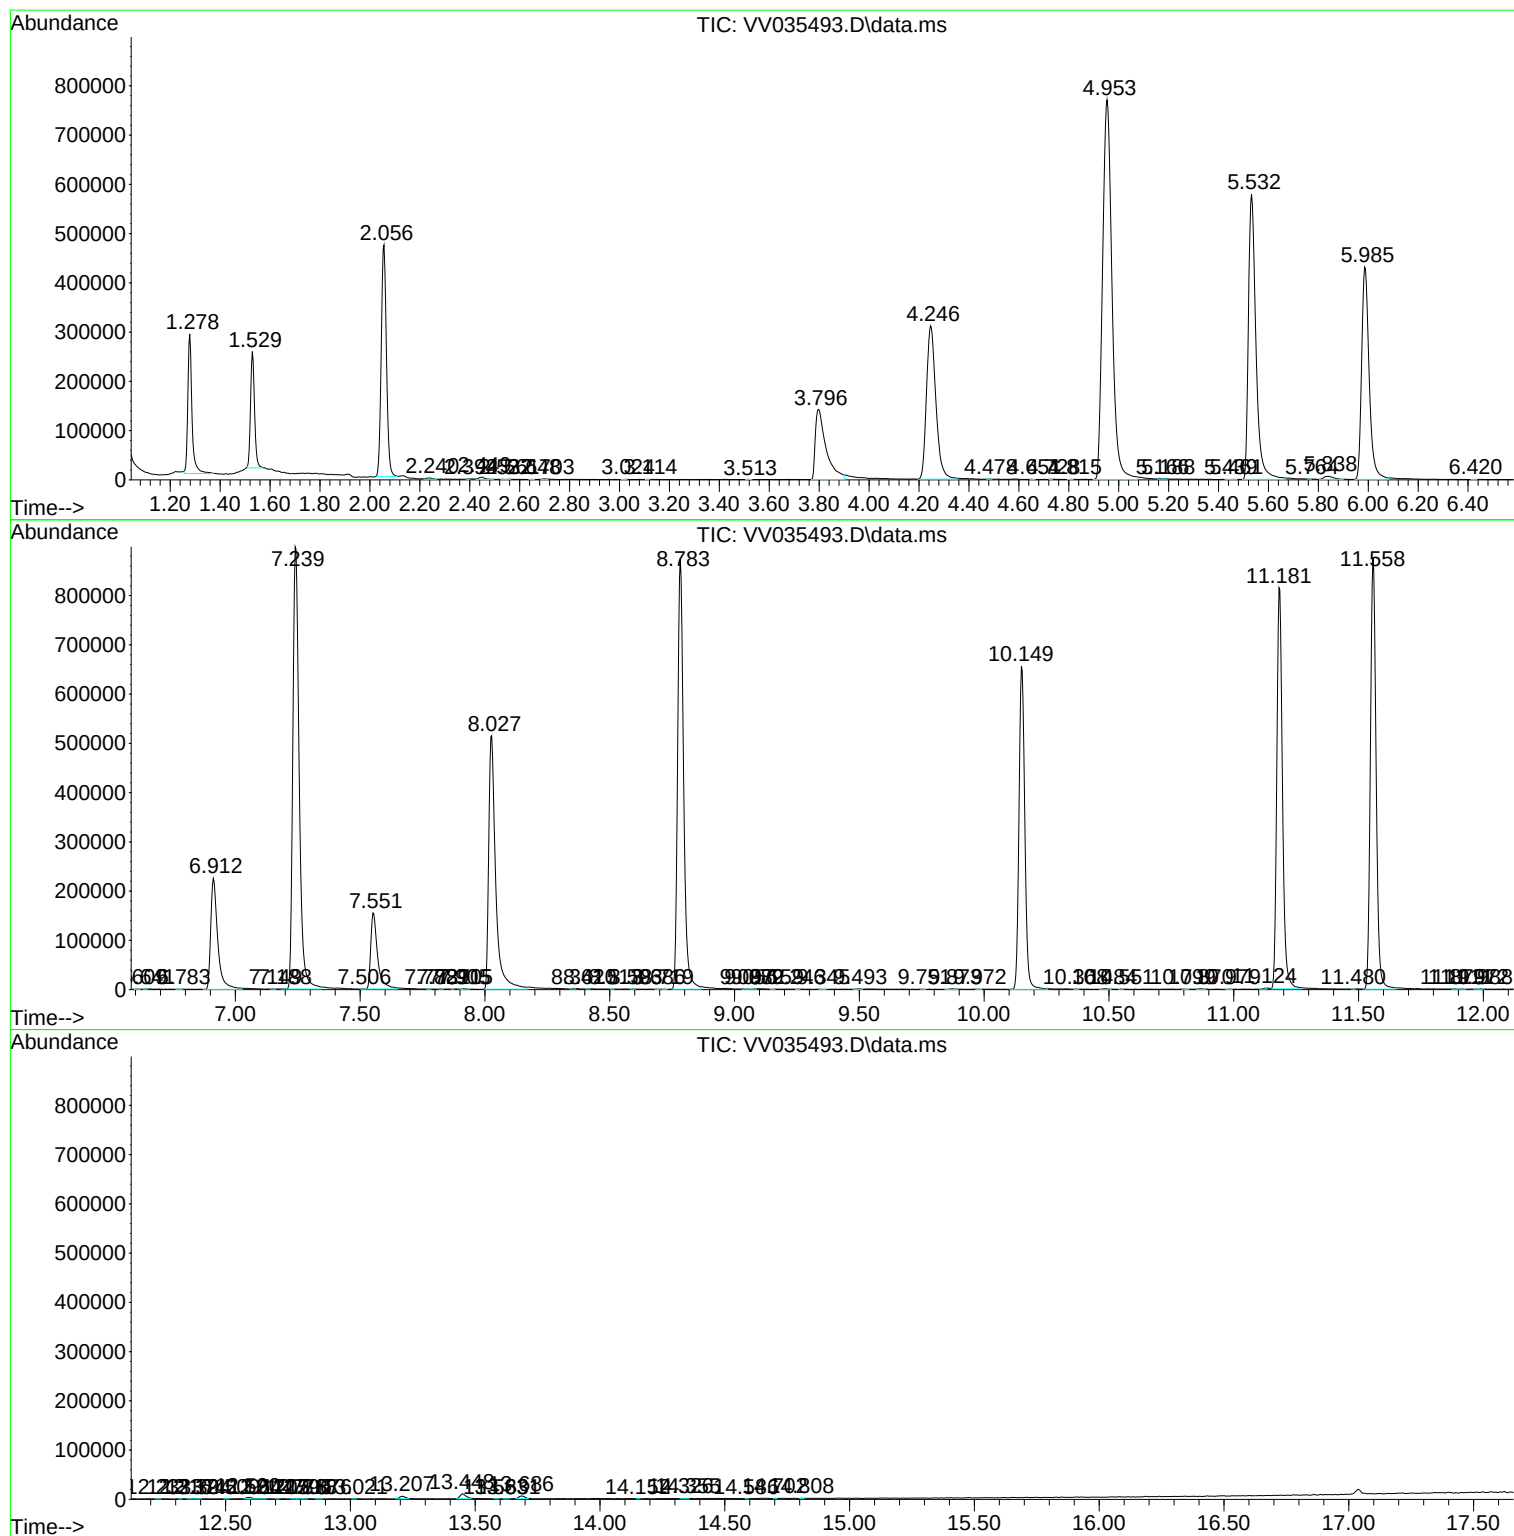

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035493.D
Acq On : 01 May 2024 13:56
Operator : SY/MD
Sample : VV0501WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035493.D
Acq On : 01 May 2024 13:56
Operator : SY/MD
Sample : VV0501WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc