

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035495.D
 Acq On : 01 May 2024 14:44
 Operator : SY/MD
 Sample : P2279-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M

Title : VOC Analysis

Signal : TIC: VV035495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	63	rBV2	26133	32007	1.69%	0.223%
2	1.275	67	73	91	rVB	266551	297561	15.71%	2.076%
3	1.526	145	151	165	rVB	210355	236481	12.49%	1.650%
4	2.053	305	315	333	rBV	448775	641492	33.87%	4.475%
5	2.320	396	398	403	rVB3	459	265	0.01%	0.002%
6	2.384	412	418	419	rBV3	879	713	0.04%	0.005%
7	2.442	430	436	448	rVB4	1741	2712	0.14%	0.019%
8	2.558	461	472	475	rBV3	3645	5764	0.30%	0.040%
9	2.706	509	518	527	rVB4	929	1674	0.09%	0.012%
10	2.767	533	537	542	rBV2	252	253	0.01%	0.002%
11	2.960	594	597	604	rVV4	405	383	0.02%	0.003%
12	3.085	633	636	641	rVB3	233	222	0.01%	0.002%
13	3.346	713	717	726	rVB2	275	286	0.02%	0.002%
14	3.629	802	805	812	rVB2	257	267	0.01%	0.002%
15	3.680	819	821	826	rBV2	331	314	0.02%	0.002%
16	3.796	848	857	902	rBV	134507	430529	22.73%	3.003%
17	4.111	953	955	957	rBV2	449	276	0.01%	0.002%
18	4.246	980	997	1030	rBV	293029	757735	40.01%	5.286%
19	4.571	1096	1098	1102	rBV	576	336	0.02%	0.002%
20	4.661	1124	1126	1129	rVB	396	208	0.01%	0.001%
21	4.725	1144	1146	1147	rBV2	527	287	0.02%	0.002%
22	4.950	1201	1216	1256	rBV2	722423	1893820	100.00%	13.211%
23	5.291	1320	1322	1324	rVB2	484	223	0.01%	0.002%
24	5.336	1331	1336	1338	rBV3	326	341	0.02%	0.002%
25	5.452	1369	1372	1377	rVB3	765	562	0.03%	0.004%
26	5.532	1385	1397	1431	rBV	546727	1145305	60.48%	7.990%
27	5.834	1482	1491	1503	rBV7	4560	10029	0.53%	0.070%
28	5.937	1520	1523	1526	rBV3	277	255	0.01%	0.002%
29	5.985	1526	1538	1577	rVV	405943	844957	44.62%	5.894%
30	6.236	1612	1616	1620	rVB4	476	360	0.02%	0.003%
31	6.259	1620	1623	1628	rVB4	651	404	0.02%	0.003%
32	6.365	1651	1656	1658	rBV2	277	253	0.01%	0.002%
33	6.535	1704	1709	1713	rBV3	277	276	0.01%	0.002%
34	6.622	1729	1736	1737	rBV2	469	428	0.02%	0.003%
35	6.635	1737	1740	1742	rVV2	506	339	0.02%	0.002%
36	6.664	1746	1749	1753	rVV3	408	364	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035495.D
 Acq On : 01 May 2024 14:44
 Operator : SY/MD
 Sample : P2279-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.738	1768	1772	1778	rVB4	542	500	0.03%	0.003%
38	6.911	1814	1826	1860	rBV	206947	402639	21.26%	2.809%
39	7.175	1906	1908	1911	rBV2	539	344	0.02%	0.002%
40	7.239	1917	1928	1956	rBV	825696	1465146	77.36%	10.221%
41	7.551	2016	2025	2058	rBV	143862	275485	14.55%	1.922%
42	7.873	2115	2125	2133	rVV4	4338	7404	0.39%	0.052%
43	8.027	2163	2173	2214	rBV	491221	926210	48.91%	6.461%
44	8.381	2281	2283	2291	rVB5	738	544	0.03%	0.004%
45	8.500	2316	2320	2321	rBV2	334	223	0.01%	0.002%
46	8.600	2348	2351	2354	rBV4	324	286	0.02%	0.002%
47	8.645	2361	2365	2369	rBV3	297	284	0.01%	0.002%
48	8.783	2393	2408	2440	rBV	836351	1388823	73.33%	9.688%
49	9.021	2479	2482	2487	rVB2	624	401	0.02%	0.003%
50	9.072	2495	2498	2501	rBV2	321	270	0.01%	0.002%
51	9.175	2527	2530	2533	rBV2	338	241	0.01%	0.002%
52	9.233	2546	2548	2555	rVB3	559	478	0.03%	0.003%
53	9.487	2625	2627	2630	rBV3	326	245	0.01%	0.002%
54	9.641	2670	2675	2680	rVB3	399	317	0.02%	0.002%
55	9.673	2680	2685	2687	rBV2	385	277	0.01%	0.002%
56	9.960	2771	2774	2776	rVV2	343	215	0.01%	0.001%
57	10.021	2790	2793	2798	rBV2	236	216	0.01%	0.002%
58	10.059	2801	2805	2810	rVB2	359	336	0.02%	0.002%
59	10.149	2821	2833	2855	rBV	632751	1004827	53.06%	7.010%
60	10.326	2879	2888	2898	rBV2	3940	6343	0.33%	0.044%
61	10.403	2910	2912	2915	rBV2	367	310	0.02%	0.002%
62	10.480	2932	2936	2937	rBV	473	325	0.02%	0.002%
63	10.558	2957	2960	2966	rVB3	298	296	0.02%	0.002%
64	10.622	2974	2980	2982	rBV2	249	278	0.01%	0.002%
65	10.741	3015	3017	3020	rBV	285	244	0.01%	0.002%
66	10.796	3030	3034	3040	rBV3	207	245	0.01%	0.002%
67	10.866	3051	3056	3062	rVB4	792	850	0.04%	0.006%
68	10.892	3062	3064	3068	rBV	518	284	0.01%	0.002%
69	11.082	3120	3123	3127	rVB3	605	409	0.02%	0.003%
70	11.127	3127	3137	3144	rBV4	6825	10935	0.58%	0.076%
71	11.185	3144	3155	3183	rVV	764631	1199409	63.33%	8.367%
72	11.333	3199	3201	3211	rVB3	834	756	0.04%	0.005%
73	11.406	3222	3224	3226	rBV	390	213	0.01%	0.001%
74	11.497	3244	3252	3253	rBV5	6139	6294	0.33%	0.044%
75	11.558	3260	3271	3302	rVB	809482	1287845	68.00%	8.984%
76	11.751	3329	3331	3337	rVV4	534	403	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035495.D
 Acq On : 01 May 2024 14:44
 Operator : SY/MD
 Sample : P2279-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.786	3340	3342	3346	rVB4	566	412	0.02%	0.003%
78	11.914	3381	3382	3386	rVV2	682	430	0.02%	0.003%
79	11.956	3392	3395	3401	rVB4	624	559	0.03%	0.004%
80	12.185	3460	3466	3467	rBV3	825	733	0.04%	0.005%
81	12.233	3478	3481	3484	rBV	316	224	0.01%	0.002%
82	12.278	3492	3495	3498	rBV2	311	229	0.01%	0.002%
83	12.304	3500	3503	3505	rVV2	476	384	0.02%	0.003%
84	12.361	3515	3521	3526	rVV5	437	464	0.02%	0.003%
85	12.522	3569	3571	3577	rBV2	383	289	0.02%	0.002%
86	12.551	3577	3580	3582	rBV	339	223	0.01%	0.002%
87	12.586	3586	3591	3603	rBV7	1836	3324	0.18%	0.023%
88	12.699	3623	3626	3629	rBV2	386	303	0.02%	0.002%
89	12.792	3648	3655	3657	rBV3	631	598	0.03%	0.004%
90	12.914	3691	3693	3696	rVB2	367	249	0.01%	0.002%
91	13.104	3749	3752	3755	rBV3	255	248	0.01%	0.002%
92	13.207	3776	3784	3794	rBV3	6534	10122	0.53%	0.071%
93	13.339	3822	3825	3829	rBV3	402	335	0.02%	0.002%
94	13.455	3852	3861	3868	rBV2	4488	6981	0.37%	0.049%
95	13.686	3922	3933	3947	rBV4	4338	8059	0.43%	0.056%
96	14.021	4034	4037	4039	rBV2	362	256	0.01%	0.002%
97	14.223	4098	4100	4103	rBV3	432	244	0.01%	0.002%
98	14.342	4134	4137	4140	rBV3	567	500	0.03%	0.003%
99	14.458	4171	4173	4174	rBV	588	296	0.02%	0.002%
100	15.091	4366	4370	4372	rBV2	778	749	0.04%	0.005%




Sum of corrected areas: 14335042

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035495.D
Acq On : 01 May 2024 14:44
Operator : SY/MD
Sample : P2279-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

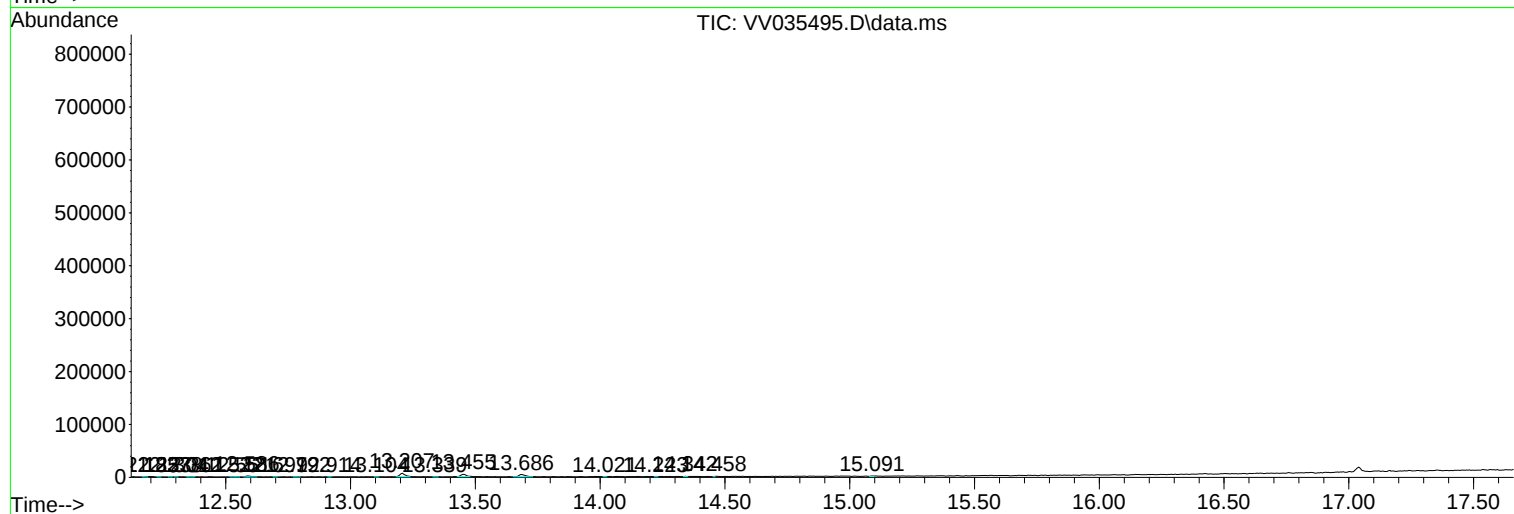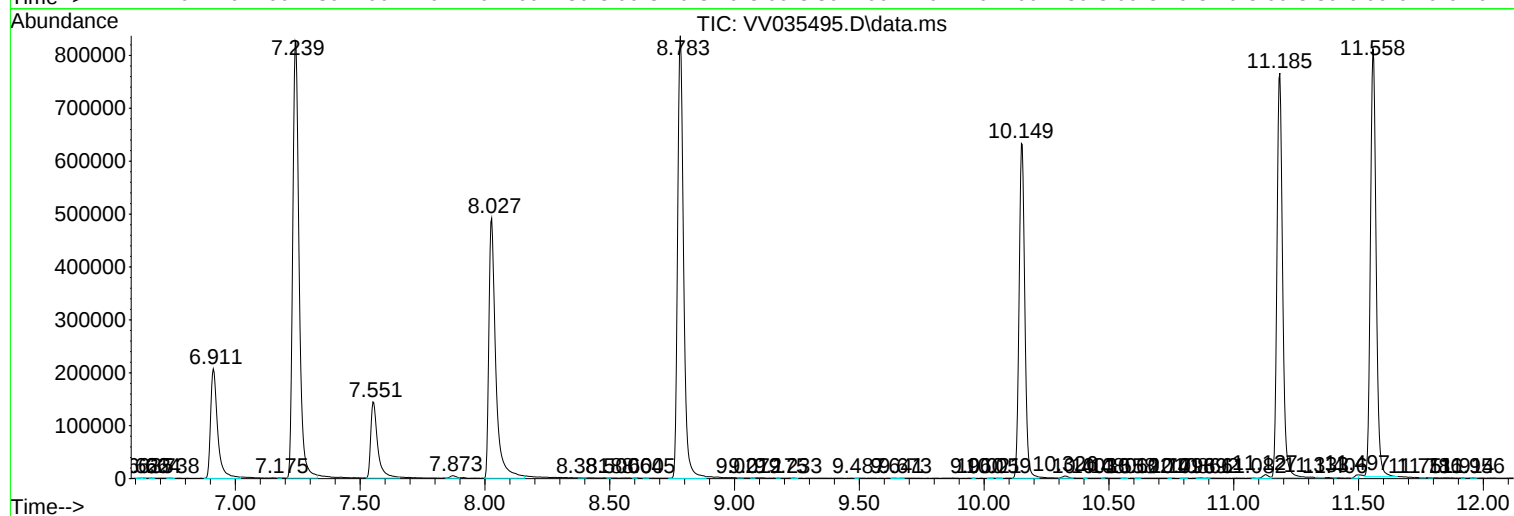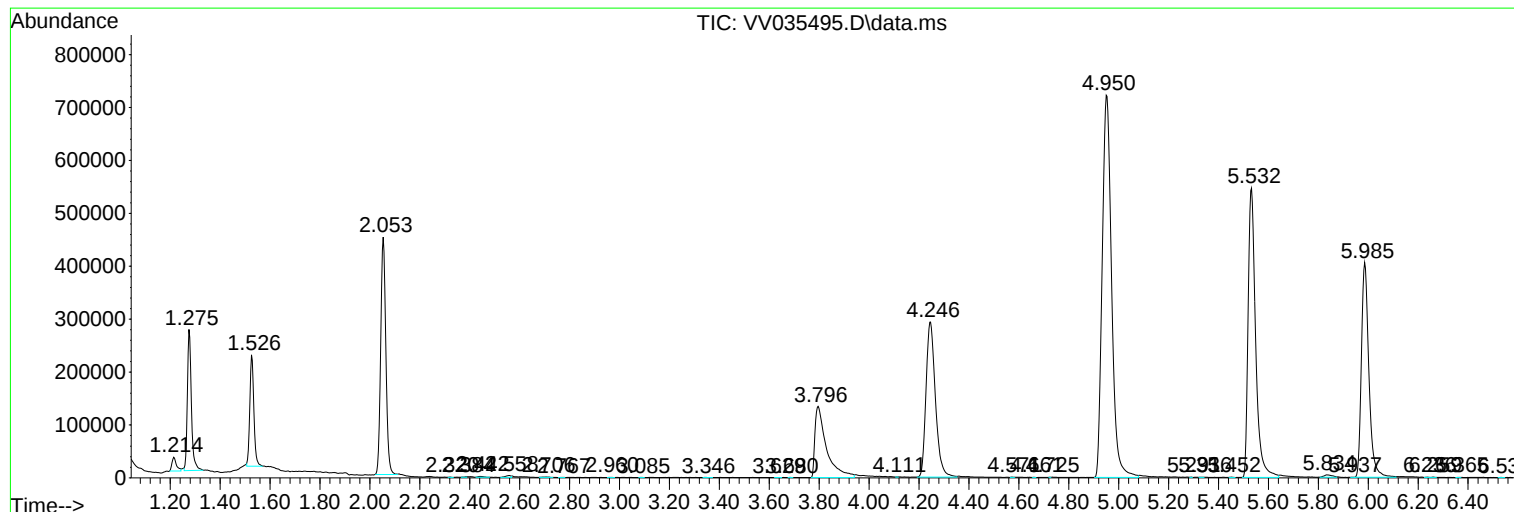

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035495.D
Acq On : 01 May 2024 14:44
Operator : SY/MD
Sample : P2279-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035495.D
Acq On : 01 May 2024 14:44
Operator : SY/MD
Sample : P2279-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
