

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035496.D
 Acq On : 01 May 2024 15:08
 Operator : SY/MD
 Sample : P2279-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	68	73	92	rVB	265968	288260	15.76%	2.024%
2	1.529	146	152	171	rVB	222510	263532	14.41%	1.850%
3	2.056	306	316	332	rBV	431394	624950	34.17%	4.387%
4	2.558	465	472	484	rVB2	6019	10560	0.58%	0.074%
5	2.671	505	507	509	rBV	253	116	0.01%	0.001%
6	2.748	528	531	534	rBV	170	140	0.01%	0.001%
7	2.780	537	541	543	rBV2	380	240	0.01%	0.002%
8	2.844	558	561	564	rBV3	133	93	0.01%	0.001%
9	3.037	619	621	626	rVB2	240	207	0.01%	0.001%
10	3.146	650	655	658	rBV2	263	212	0.01%	0.001%
11	3.182	663	666	671	rVB2	303	243	0.01%	0.002%
12	3.201	671	672	674	rBV2	126	70	0.00%	0.000%
13	3.211	674	675	679	rVB3	287	123	0.01%	0.001%
14	3.230	679	681	682	rBV	142	65	0.00%	0.000%
15	3.272	692	694	696	rBV	272	112	0.01%	0.001%
16	3.326	708	711	713	rBV	135	79	0.00%	0.001%
17	3.404	728	735	739	rVB3	466	532	0.03%	0.004%
18	3.429	739	743	745	rBV	202	156	0.01%	0.001%
19	3.494	761	763	765	rBV2	120	57	0.00%	0.000%
20	3.526	770	773	775	rBV	124	82	0.00%	0.001%
21	3.577	786	789	792	rVV2	227	131	0.01%	0.001%
22	3.606	796	798	801	rVB	115	62	0.00%	0.000%
23	3.674	816	819	820	rBV2	250	138	0.01%	0.001%
24	3.793	847	856	897	rBV	132936	432982	23.67%	3.039%
25	4.246	982	997	1033	rBV2	285988	733337	40.09%	5.148%
26	4.619	1110	1113	1116	rBV2	407	321	0.02%	0.002%
27	4.699	1134	1138	1140	rBV2	229	185	0.01%	0.001%
28	4.715	1140	1143	1144	rBV	197	95	0.01%	0.001%
29	4.789	1163	1166	1167	rBV2	180	93	0.01%	0.001%
30	4.799	1167	1169	1177	rVB2	378	372	0.02%	0.003%
31	4.834	1177	1180	1181	rBV	156	86	0.00%	0.001%
32	4.953	1201	1217	1252	rBV2	699582	1829191	100.00%	12.841%
33	5.217	1297	1299	1304	rVB3	730	356	0.02%	0.002%
34	5.272	1314	1316	1321	rBV3	509	358	0.02%	0.003%
35	5.365	1343	1345	1348	rVB2	232	89	0.00%	0.001%
36	5.429	1360	1365	1369	rBV3	423	459	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035496.D
 Acq On : 01 May 2024 15:08
 Operator : SY/MD
 Sample : P2279-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	5.484	1380	1382	1386	rVB2	471	255	0.01%	0.002%
38	5.532	1386	1397	1436	rBV	535587	1126376	61.58%	7.907%
39	5.940	1522	1524	1525	rBV	260	72	0.00%	0.001%
40	5.985	1525	1538	1571	rBV	393397	825394	45.12%	5.794%
41	6.378	1656	1660	1663	rBV2	496	424	0.02%	0.003%
42	6.420	1668	1673	1676	rBV2	418	403	0.02%	0.003%
43	6.481	1691	1692	1695	rVB	278	118	0.01%	0.001%
44	6.513	1695	1702	1706	rVB3	411	401	0.02%	0.003%
45	6.535	1706	1709	1711	rBV	131	79	0.00%	0.001%
46	6.551	1711	1714	1717	rVB	218	135	0.01%	0.001%
47	6.609	1726	1732	1734	rBV3	621	575	0.03%	0.004%
48	6.786	1782	1787	1788	rBV3	253	183	0.01%	0.001%
49	6.802	1790	1792	1794	rVB	212	62	0.00%	0.000%
50	6.815	1794	1796	1800	rVB2	260	141	0.01%	0.001%
51	6.834	1800	1802	1805	rVB	287	111	0.01%	0.001%
52	6.912	1814	1826	1857	rBV	201060	389432	21.29%	2.734%
53	7.239	1915	1928	1956	rBV	793704	1415628	77.39%	9.937%
54	7.551	2016	2025	2058	rBV	139442	264692	14.47%	1.858%
55	7.876	2116	2126	2141	rVB2	10716	19943	1.09%	0.140%
56	7.963	2147	2153	2155	rBV4	774	638	0.03%	0.004%
57	8.024	2163	2172	2213	rBV	466773	865622	47.32%	6.077%
58	8.571	2340	2342	2350	rVB3	593	435	0.02%	0.003%
59	8.783	2396	2408	2443	rBV	825363	1486437	81.26%	10.435%
60	9.082	2499	2501	2503	rBV	418	222	0.01%	0.002%
61	9.162	2522	2526	2531	rBV4	652	575	0.03%	0.004%
62	9.275	2559	2561	2564	rVB	268	124	0.01%	0.001%
63	9.323	2574	2576	2579	rVB	287	143	0.01%	0.001%
64	9.349	2580	2584	2587	rVB2	233	159	0.01%	0.001%
65	9.368	2587	2590	2596	rVB3	354	336	0.02%	0.002%
66	9.397	2596	2599	2601	rBV	153	107	0.01%	0.001%
67	9.413	2602	2604	2607	rVV2	231	174	0.01%	0.001%
68	9.448	2609	2615	2617	rBV2	279	293	0.02%	0.002%
69	9.497	2626	2630	2631	rBV2	377	286	0.02%	0.002%
70	9.535	2639	2642	2645	rBV2	271	172	0.01%	0.001%
71	9.558	2646	2649	2650	rBV3	401	182	0.01%	0.001%
72	9.670	2682	2684	2687	rBV	279	147	0.01%	0.001%
73	9.799	2717	2724	2729	rBV4	861	1288	0.07%	0.009%
74	9.860	2739	2743	2744	rBV2	458	274	0.01%	0.002%
75	9.992	2781	2784	2786	rBV2	162	102	0.01%	0.001%
76	10.069	2805	2808	2810	rBV2	292	161	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035496.D
 Acq On : 01 May 2024 15:08
 Operator : SY/MD
 Sample : P2279-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	10.149	2821	2833	2860	rBV	600532	950479	51.96%	6.672%
78	10.323	2880	2887	2900	rVB2	11862	19556	1.07%	0.137%
79	10.432	2916	2921	2925	rBV2	287	330	0.02%	0.002%
80	10.458	2927	2929	2933	rVB3	371	256	0.01%	0.002%
81	10.490	2934	2939	2942	rBV2	555	532	0.03%	0.004%
82	10.545	2953	2956	2959	rBV3	207	156	0.01%	0.001%
83	10.776	3025	3028	3029	rBV	315	175	0.01%	0.001%
84	10.870	3052	3057	3059	rBV2	505	428	0.02%	0.003%
85	10.940	3076	3079	3083	rVB	354	230	0.01%	0.002%
86	11.124	3127	3136	3144	rBV2	20252	32923	1.80%	0.231%
87	11.185	3145	3155	3190	rVB	765401	1324973	72.43%	9.301%
88	11.558	3260	3271	3302	rBV	784285	1302461	71.20%	9.143%
89	11.902	3376	3378	3380	rBV2	388	200	0.01%	0.001%
90	12.050	3422	3424	3429	rBV3	325	252	0.01%	0.002%
91	12.075	3429	3432	3436	rVV3	482	343	0.02%	0.002%
92	12.136	3449	3451	3456	rBV	503	372	0.02%	0.003%
93	12.307	3498	3504	3507	rBV6	1866	1912	0.10%	0.013%
94	12.413	3535	3537	3538	rBV6	329	123	0.01%	0.001%
95	12.587	3586	3591	3604	rVB5	2147	2985	0.16%	0.021%
96	12.725	3629	3634	3637	rBV3	647	572	0.03%	0.004%
97	13.207	3779	3784	3795	rVB5	3590	5359	0.29%	0.038%
98	13.451	3855	3860	3868	rBV3	3057	4329	0.24%	0.030%
99	13.689	3926	3934	3943	rBV5	2921	5026	0.27%	0.035%
100	13.847	3980	3983	3991	rBV5	714	958	0.05%	0.007%




Sum of corrected areas: 14245315

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035496.D
Acq On : 01 May 2024 15:08
Operator : SY/MD
Sample : P2279-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

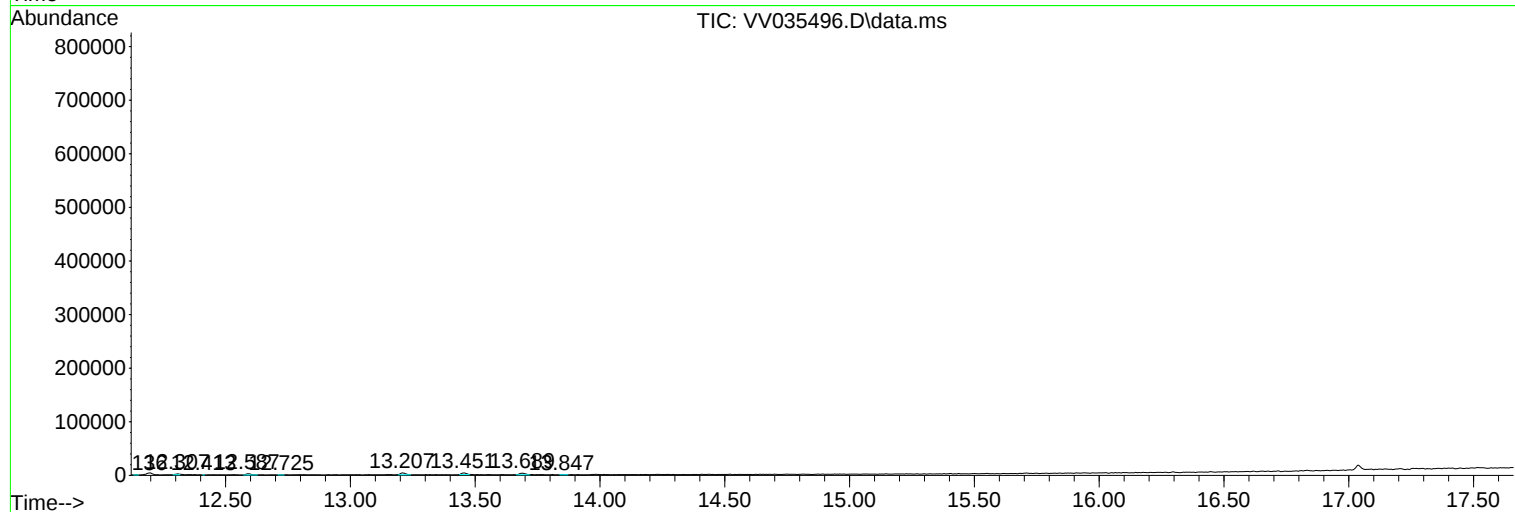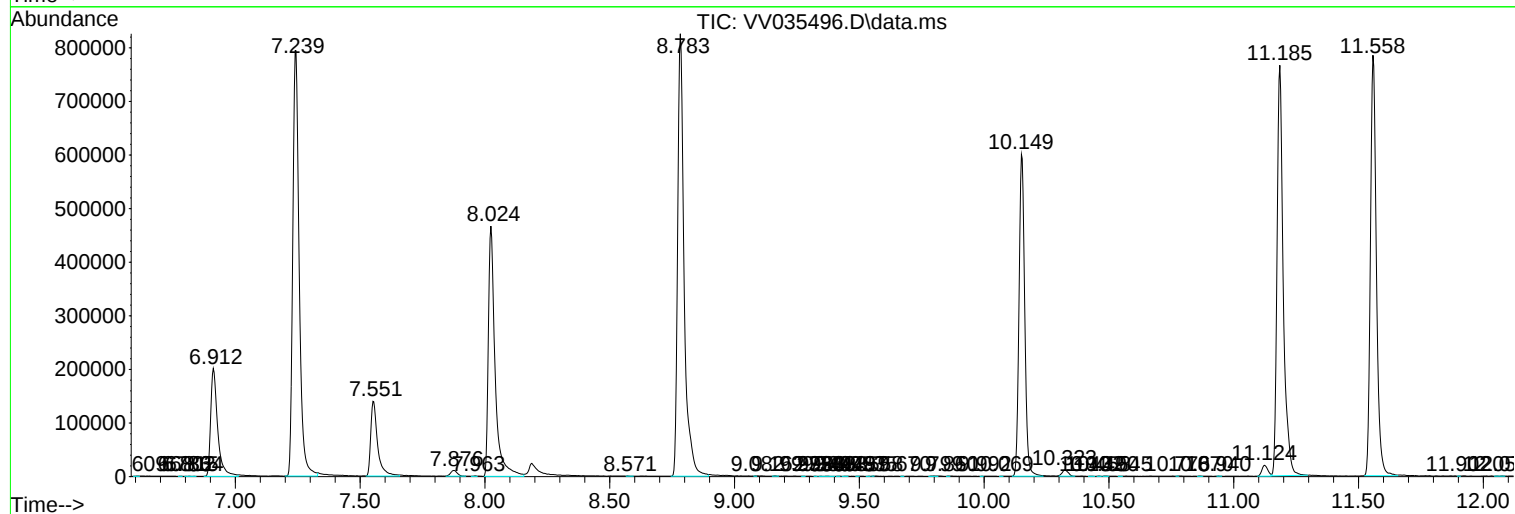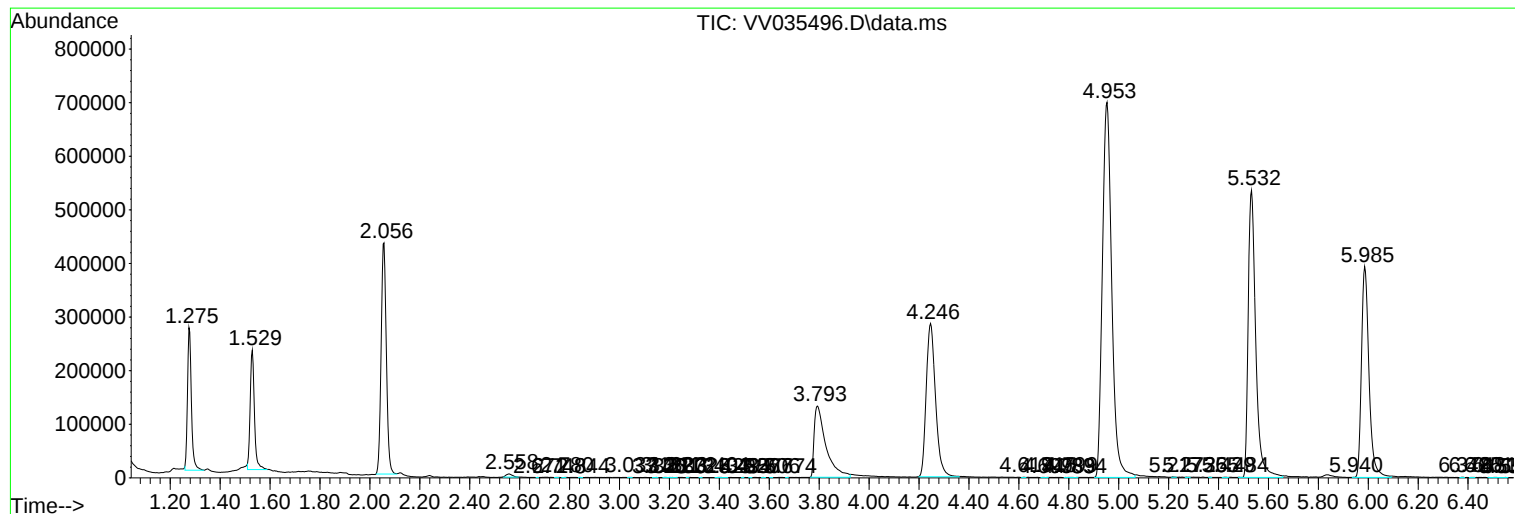

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035496.D
Acq On : 01 May 2024 15:08
Operator : SY/MD
Sample : P2279-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035496.D
Acq On : 01 May 2024 15:08
Operator : SY/MD
Sample : P2279-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc