

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035497.D
 Acq On : 01 May 2024 15:32
 Operator : SY/MD
 Sample : P2279-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M

Title : VOC Analysis

Signal : TIC: VV035497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	68	73	88	rVB	253822	276080	15.09%	1.991%
2	1.529	146	152	167	rVB	215459	249866	13.66%	1.802%
3	2.056	306	316	331	rBV	431364	623806	34.09%	4.500%
4	2.786	539	543	548	rBV2	263	347	0.02%	0.003%
5	2.809	548	550	553	rVV2	262	108	0.01%	0.001%
6	2.863	565	567	570	rBV2	260	142	0.01%	0.001%
7	2.883	570	573	575	rBV2	230	180	0.01%	0.001%
8	2.966	596	599	602	rBV	163	99	0.01%	0.001%
9	3.079	627	634	636	rBV2	358	364	0.02%	0.003%
10	3.146	650	655	657	rBV2	231	208	0.01%	0.002%
11	3.166	658	661	662	rVB	211	102	0.01%	0.001%
12	3.259	683	690	695	rBV3	361	401	0.02%	0.003%
13	3.294	699	701	704	rVB3	170	72	0.00%	0.001%
14	3.339	712	715	721	rBV2	224	203	0.01%	0.001%
15	3.410	735	737	741	rVB	147	72	0.00%	0.001%
16	3.445	745	748	750	rBV	97	74	0.00%	0.001%
17	3.519	767	771	774	rBV	219	201	0.01%	0.001%
18	3.561	780	784	787	rBV	299	272	0.01%	0.002%
19	3.629	803	805	808	rVB3	205	127	0.01%	0.001%
20	3.651	808	812	816	rVB2	106	98	0.01%	0.001%
21	3.677	816	820	824	rBV2	137	134	0.01%	0.001%
22	3.706	827	829	831	rVB2	202	84	0.00%	0.001%
23	3.760	843	846	847	rBV	121	75	0.00%	0.001%
24	3.793	847	856	903	rBV	135294	414235	22.64%	2.988%
25	4.246	983	997	1036	rVB	287288	740414	40.46%	5.341%
26	4.686	1130	1134	1135	rBV	363	207	0.01%	0.001%
27	4.748	1150	1153	1158	rVB4	460	368	0.02%	0.003%
28	4.770	1158	1160	1162	rBV2	209	83	0.00%	0.001%
29	4.831	1175	1179	1180	rBV	269	201	0.01%	0.001%
30	4.883	1191	1195	1197	rBV	257	186	0.01%	0.001%
31	4.899	1197	1200	1201	rBV	273	160	0.01%	0.001%
32	4.953	1201	1217	1247	rBV2	702622	1829835	100.00%	13.199%
33	5.394	1351	1354	1356	rBV	354	250	0.01%	0.002%
34	5.532	1386	1397	1448	rBV	547526	1150951	62.90%	8.302%
35	5.834	1481	1491	1515	rVB4	10673	27087	1.48%	0.195%
36	5.985	1525	1538	1574	rBV	399808	829219	45.32%	5.981%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035497.D
 Acq On : 01 May 2024 15:32
 Operator : SY/MD
 Sample : P2279-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.246	1617	1619	1626	rVB4	809	815	0.04%	0.006%
38	6.275	1626	1628	1632	rBV2	255	206	0.01%	0.001%
39	6.294	1632	1634	1638	rBV3	260	154	0.01%	0.001%
40	6.358	1650	1654	1658	rBV3	631	533	0.03%	0.004%
41	6.378	1658	1660	1663	rBV3	278	161	0.01%	0.001%
42	6.394	1663	1665	1667	rVV	149	95	0.01%	0.001%
43	6.416	1670	1672	1676	rVB2	230	163	0.01%	0.001%
44	6.481	1691	1692	1694	rBV	142	75	0.00%	0.001%
45	6.551	1711	1714	1716	rVB	370	184	0.01%	0.001%
46	6.571	1716	1720	1721	rBV	134	100	0.01%	0.001%
47	6.580	1721	1723	1725	rVV	167	76	0.00%	0.001%
48	6.641	1739	1742	1745	rVB2	293	194	0.01%	0.001%
49	6.709	1762	1763	1765	rVB	187	47	0.00%	0.000%
50	6.731	1765	1770	1773	rBV2	325	274	0.01%	0.002%
51	6.747	1773	1775	1776	rBV2	203	96	0.01%	0.001%
52	6.911	1816	1826	1859	rBV	198985	387535	21.18%	2.795%
53	7.243	1918	1929	1959	rBV	791095	1420646	77.64%	10.247%
54	7.551	2016	2025	2047	rBV	142631	262082	14.32%	1.890%
55	7.870	2118	2124	2125	rBV3	2713	2300	0.13%	0.017%
56	7.918	2137	2139	2144	rVB4	716	468	0.03%	0.003%
57	7.953	2148	2150	2153	rVB2	526	248	0.01%	0.002%
58	7.969	2153	2155	2156	rBV2	255	107	0.01%	0.001%
59	8.024	2163	2172	2212	rBV	475330	882156	48.21%	6.363%
60	8.599	2348	2351	2354	rBV2	372	308	0.02%	0.002%
61	8.783	2397	2408	2444	rBV	827439	1386452	75.77%	10.001%
62	9.095	2501	2505	2508	rBV4	477	510	0.03%	0.004%
63	9.152	2519	2523	2524	rBV3	690	376	0.02%	0.003%
64	9.188	2531	2534	2536	rBV3	516	289	0.02%	0.002%
65	9.214	2536	2542	2544	rBV3	392	434	0.02%	0.003%
66	9.297	2564	2568	2569	rBV	256	180	0.01%	0.001%
67	9.355	2583	2586	2589	rBV	229	205	0.01%	0.001%
68	9.480	2623	2625	2628	rBV	212	131	0.01%	0.001%
69	9.509	2628	2634	2638	rBV4	532	627	0.03%	0.005%
70	9.580	2652	2656	2657	rBV2	173	128	0.01%	0.001%
71	9.603	2661	2663	2667	rBV3	206	125	0.01%	0.001%
72	9.628	2667	2671	2674	rBV2	263	233	0.01%	0.002%
73	9.664	2679	2682	2687	rVB3	341	233	0.01%	0.002%
74	9.693	2687	2691	2692	rBV2	225	153	0.01%	0.001%
75	9.747	2706	2708	2709	rVB	226	70	0.00%	0.001%
76	9.760	2709	2712	2713	rBV2	140	77	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035497.D
 Acq On : 01 May 2024 15:32
 Operator : SY/MD
 Sample : P2279-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	9.789	2719	2721	2724	rBV	278	110	0.01%	0.001%
78	9.844	2737	2738	2741	rVB2	288	108	0.01%	0.001%
79	9.869	2742	2746	2748	rBV2	269	238	0.01%	0.002%
80	9.911	2756	2759	2762	rBV2	249	152	0.01%	0.001%
81	9.927	2762	2764	2766	rBV	268	116	0.01%	0.001%
82	10.050	2798	2802	2805	rBV2	233	208	0.01%	0.002%
83	10.149	2819	2833	2856	rBV	586594	936359	51.17%	6.754%
84	10.371	2900	2902	2904	rBV	204	93	0.01%	0.001%
85	10.519	2946	2948	2949	rBV	272	115	0.01%	0.001%
86	10.558	2958	2960	2961	rBV	308	118	0.01%	0.001%
87	10.641	2981	2986	2988	rBV	158	141	0.01%	0.001%
88	10.657	2989	2991	2993	rBV	209	98	0.01%	0.001%
89	10.744	3014	3018	3022	rBV2	377	276	0.02%	0.002%
90	10.763	3022	3024	3027	rVB	335	190	0.01%	0.001%
91	10.786	3027	3031	3036	rBV2	668	513	0.03%	0.004%
92	10.898	3064	3066	3069	rBV	356	156	0.01%	0.001%
93	10.985	3090	3093	3094	rBV	328	129	0.01%	0.001%
94	11.185	3144	3155	3182	rBV	751602	1187876	64.92%	8.568%
95	11.503	3246	3254	3255	rBV3	4609	4719	0.26%	0.034%
96	11.558	3261	3271	3298	rVB	775540	1232163	67.34%	8.888%
97	11.898	3374	3377	3380	rBV2	689	518	0.03%	0.004%
98	11.995	3404	3407	3410	rBV3	411	271	0.01%	0.002%
99	12.789	3649	3654	3657	rBV4	656	651	0.04%	0.005%
100	13.217	3780	3787	3796	rVB8	1673	2589	0.14%	0.019%




Sum of corrected areas: 13863464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035497.D
Acq On : 01 May 2024 15:32
Operator : SY/MD
Sample : P2279-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

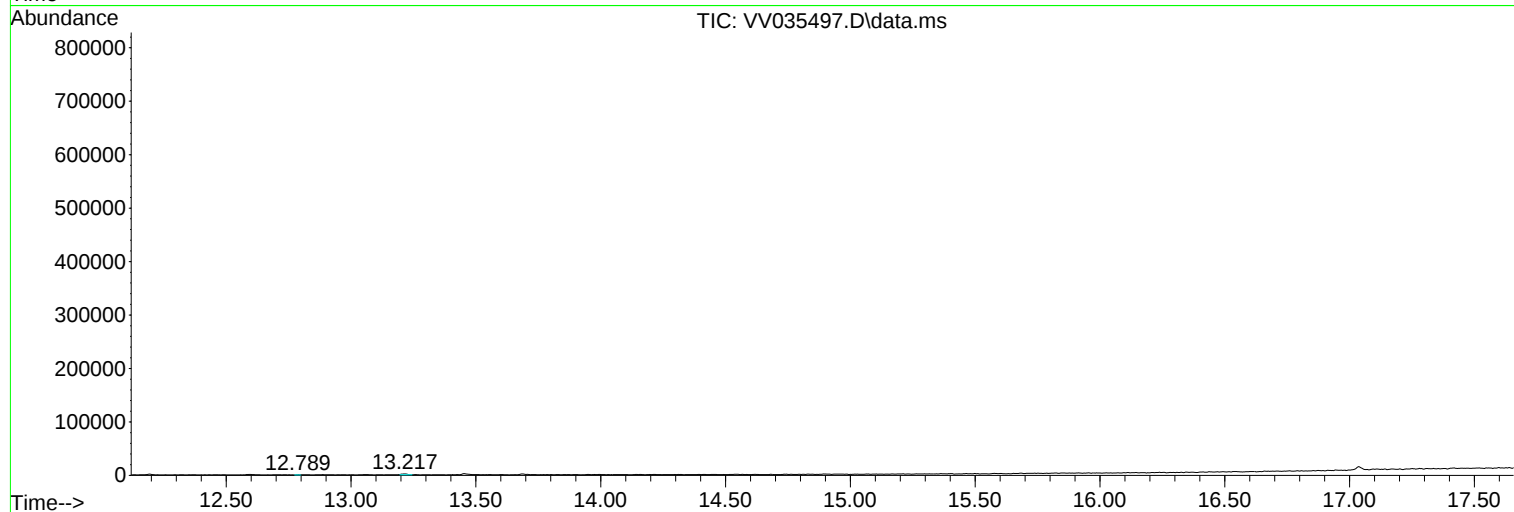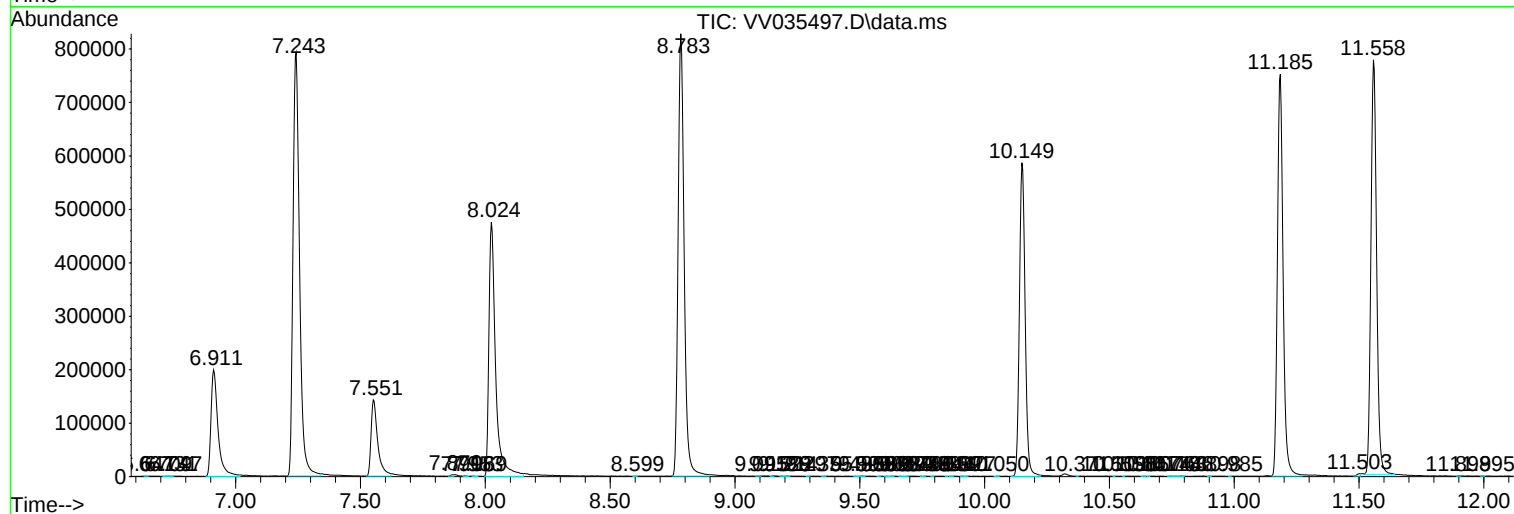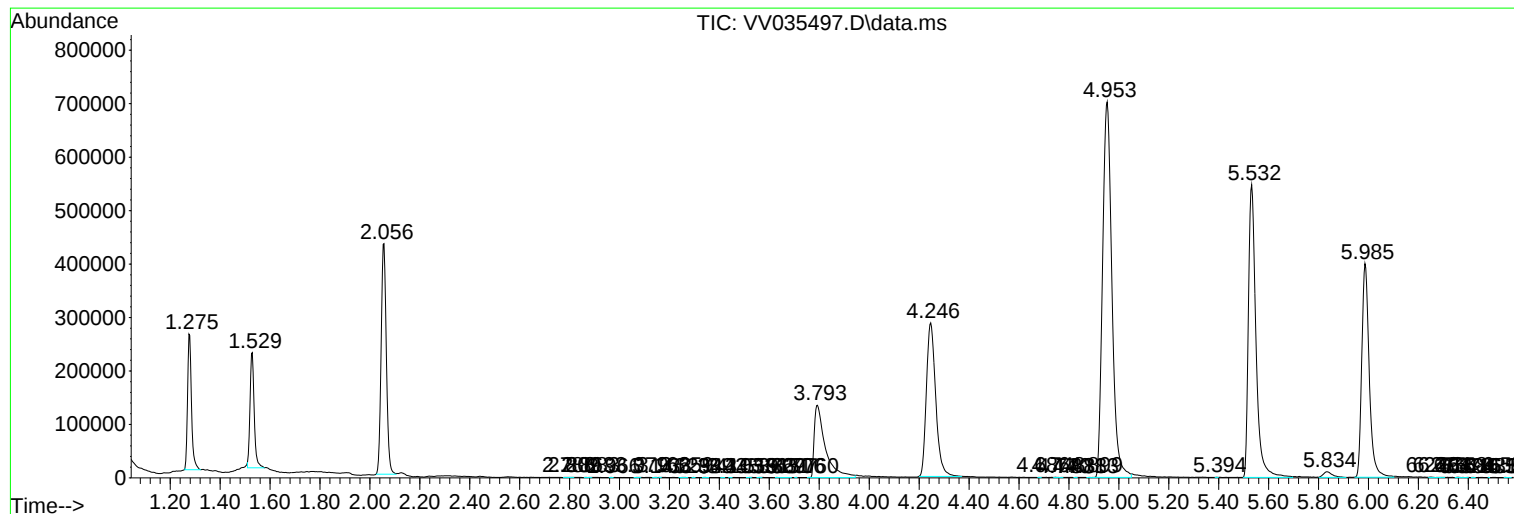

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035497.D
Acq On : 01 May 2024 15:32
Operator : SY/MD
Sample : P2279-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035497.D
Acq On : 01 May 2024 15:32
Operator : SY/MD
Sample : P2279-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc