

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035498.D
 Acq On : 01 May 2024 15:55
 Operator : SY/MD
 Sample : P2279-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	68	73	94	rVB	212243	236702	14.00%	1.903%
2	1.526	145	151	169	rVB	188894	232292	13.74%	1.868%
3	2.053	306	315	330	rVB	358709	517065	30.59%	4.158%
4	2.558	461	472	482	rBV2	3691	7519	0.44%	0.060%
5	2.879	570	572	575	rBV	289	180	0.01%	0.001%
6	2.953	593	595	599	rVB	419	200	0.01%	0.002%
7	3.034	618	620	625	rVB2	205	87	0.01%	0.001%
8	3.159	655	659	665	rBV3	352	305	0.02%	0.002%
9	3.201	671	672	673	rBV3	109	30	0.00%	0.000%
10	3.272	691	694	698	rBV2	312	229	0.01%	0.002%
11	3.320	705	709	711	rBV	126	101	0.01%	0.001%
12	3.336	711	714	716	rBV	173	122	0.01%	0.001%
13	3.375	724	726	729	rVB	260	119	0.01%	0.001%
14	3.394	729	732	736	rVB	171	116	0.01%	0.001%
15	3.416	736	739	740	rBV	66	39	0.00%	0.000%
16	3.439	744	746	749	rBV	133	84	0.00%	0.001%
17	3.577	787	789	791	rVB	207	88	0.01%	0.001%
18	3.593	791	794	797	rBV	303	165	0.01%	0.001%
19	3.641	803	809	815	rVB2	323	396	0.02%	0.003%
20	3.670	815	818	820	rBV	133	86	0.01%	0.001%
21	3.683	820	822	824	rBV	90	58	0.00%	0.000%
22	3.693	824	825	827	rBV	156	68	0.00%	0.001%
23	3.738	835	839	842	rBV	152	112	0.01%	0.001%
24	3.789	846	855	919	rBV	142327	445134	26.33%	3.579%
25	4.246	982	997	1033	rBV	258965	669970	39.63%	5.387%
26	4.629	1114	1116	1117	rBV	307	132	0.01%	0.001%
27	4.780	1160	1163	1165	rBV	287	201	0.01%	0.002%
28	4.812	1169	1173	1177	rVB3	391	385	0.02%	0.003%
29	4.831	1177	1179	1180	rBV	144	72	0.00%	0.001%
30	4.883	1192	1195	1198	rVB2	328	205	0.01%	0.002%
31	4.953	1201	1217	1262	rBV2	643063	1690367	100.00%	13.592%
32	5.439	1365	1368	1370	rBV2	368	165	0.01%	0.001%
33	5.487	1380	1383	1386	rBV	278	203	0.01%	0.002%
34	5.532	1386	1397	1432	rBV	449571	937063	55.44%	7.535%
35	5.838	1482	1492	1507	rBV6	5409	12558	0.74%	0.101%
36	5.985	1526	1538	1573	rBV	365301	764229	45.21%	6.145%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035498.D
 Acq On : 01 May 2024 15:55
 Operator : SY/MD
 Sample : P2279-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.249	1618	1620	1622	rBV2	558	323	0.02%	0.003%
38	6.297	1632	1635	1640	rVV3	298	265	0.02%	0.002%
39	6.323	1640	1643	1645	rVV3	271	181	0.01%	0.001%
40	6.349	1649	1651	1653	rVB	158	45	0.00%	0.000%
41	6.365	1653	1656	1658	rBV	167	107	0.01%	0.001%
42	6.420	1671	1673	1676	rVB	169	77	0.00%	0.001%
43	6.439	1676	1679	1681	rBV2	333	148	0.01%	0.001%
44	6.455	1682	1684	1685	rBV	302	95	0.01%	0.001%
45	6.490	1691	1695	1697	rBV2	138	116	0.01%	0.001%
46	6.503	1697	1699	1705	rVV	226	197	0.01%	0.002%
47	6.535	1706	1709	1712	rVV2	396	258	0.02%	0.002%
48	6.564	1716	1718	1720	rVB	272	107	0.01%	0.001%
49	6.580	1720	1723	1726	rBV2	197	135	0.01%	0.001%
50	6.622	1731	1736	1738	rBV2	398	327	0.02%	0.003%
51	6.702	1759	1761	1762	rBV	189	91	0.01%	0.001%
52	6.725	1765	1768	1770	rVV3	200	118	0.01%	0.001%
53	6.789	1784	1788	1791	rBV2	324	317	0.02%	0.003%
54	6.825	1795	1799	1802	rBV2	157	143	0.01%	0.001%
55	6.860	1808	1810	1812	rBV	102	57	0.00%	0.000%
56	6.911	1816	1826	1853	rBV	183905	358491	21.21%	2.883%
57	7.243	1917	1929	1965	rBV	685170	1243497	73.56%	9.999%
58	7.555	2017	2026	2053	rBV	129632	247540	14.64%	1.990%
59	7.873	2116	2125	2133	rBV6	1772	3005	0.18%	0.024%
60	7.989	2156	2161	2163	rBV2	423	401	0.02%	0.003%
61	8.024	2163	2172	2220	rBV	479214	886609	52.45%	7.129%
62	8.628	2357	2360	2364	rBV3	401	320	0.02%	0.003%
63	8.783	2397	2408	2452	rBV	692326	1160760	68.67%	9.334%
64	9.226	2543	2546	2548	rBV3	266	216	0.01%	0.002%
65	9.297	2564	2568	2571	rBV2	447	314	0.02%	0.003%
66	9.323	2574	2576	2577	rBV	132	55	0.00%	0.000%
67	9.461	2617	2619	2620	rBV	239	106	0.01%	0.001%
68	9.474	2620	2623	2624	rVV	179	107	0.01%	0.001%
69	9.529	2638	2640	2642	rBV	230	107	0.01%	0.001%
70	9.599	2660	2662	2666	rBV3	228	146	0.01%	0.001%
71	9.702	2690	2694	2697	rBV	171	120	0.01%	0.001%
72	9.731	2697	2703	2704	rBV3	274	255	0.02%	0.002%
73	9.773	2714	2716	2718	rVB2	168	56	0.00%	0.000%
74	9.796	2720	2723	2725	rBV3	340	238	0.01%	0.002%
75	9.879	2747	2749	2756	rVB4	449	423	0.03%	0.003%
76	10.008	2788	2789	2790	rBV4	124	39	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035498.D
 Acq On : 01 May 2024 15:55
 Operator : SY/MD
 Sample : P2279-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	10.098	2814	2817	2818	rBV	217	141	0.01%	0.001%
78	10.149	2822	2833	2869	rVV	587870	945511	55.94%	7.603%
79	10.464	2925	2931	2933	rBV2	422	322	0.02%	0.003%
80	10.484	2933	2937	2939	rBV4	430	344	0.02%	0.003%
81	10.632	2979	2983	2985	rBV	350	264	0.02%	0.002%
82	10.744	3013	3018	3024	rVB3	444	420	0.02%	0.003%
83	10.844	3047	3049	3051	rBV	207	85	0.01%	0.001%
84	10.940	3076	3079	3086	rBV	307	209	0.01%	0.002%
85	10.972	3087	3089	3091	rVV	332	166	0.01%	0.001%
86	10.985	3091	3093	3095	rVB2	323	113	0.01%	0.001%
87	11.078	3120	3122	3124	rBV	191	120	0.01%	0.001%
88	11.130	3132	3138	3141	rBV4	778	977	0.06%	0.008%
89	11.185	3144	3155	3180	rBV	608866	969759	57.37%	7.798%
90	11.558	3259	3271	3300	rBV	682757	1092667	64.64%	8.786%
91	12.069	3428	3430	3434	rBV	406	294	0.02%	0.002%
92	12.123	3445	3447	3450	rBV2	289	136	0.01%	0.001%
93	12.262	3486	3490	3493	rBV2	382	263	0.02%	0.002%
94	12.332	3508	3512	3518	rVB3	425	501	0.03%	0.004%
95	12.596	3589	3594	3600	rBV3	785	1183	0.07%	0.010%
96	12.676	3618	3619	3622	rBV	291	185	0.01%	0.001%




Sum of corrected areas: 12436419

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035498.D
Acq On : 01 May 2024 15:55
Operator : SY/MD
Sample : P2279-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

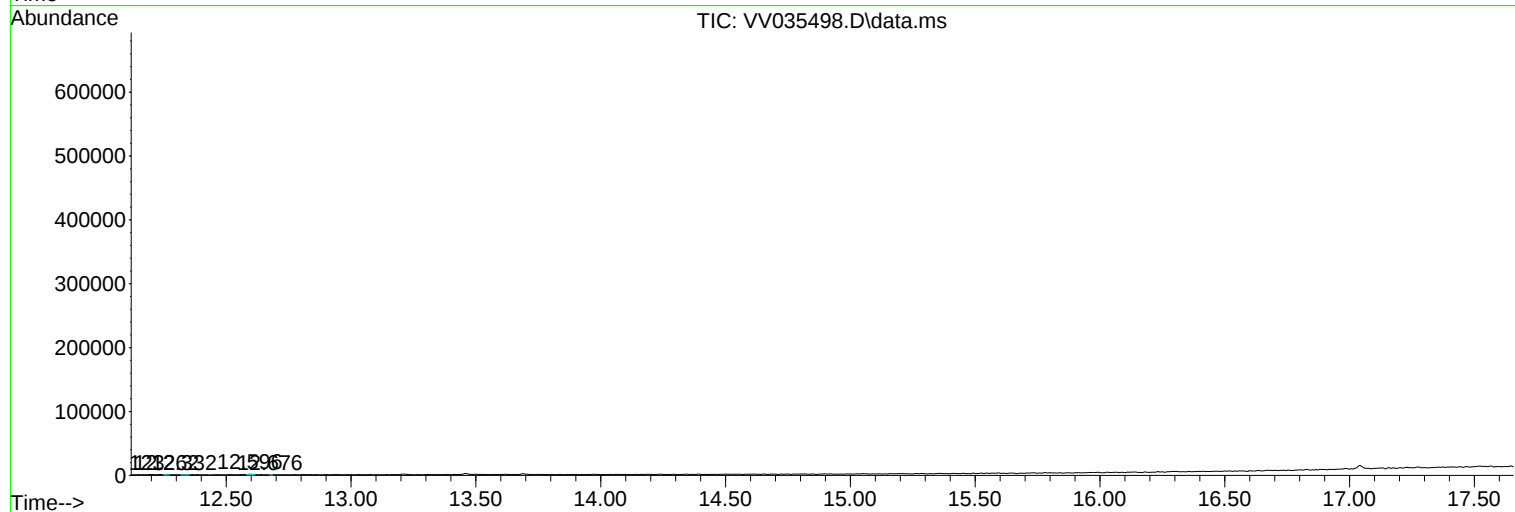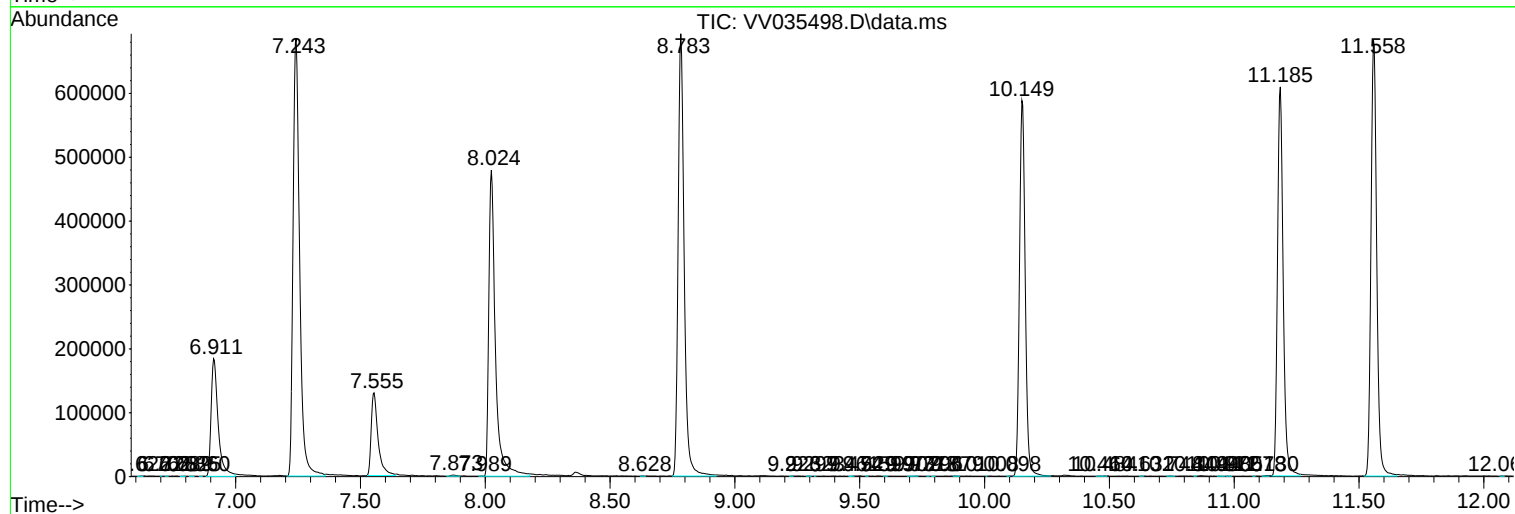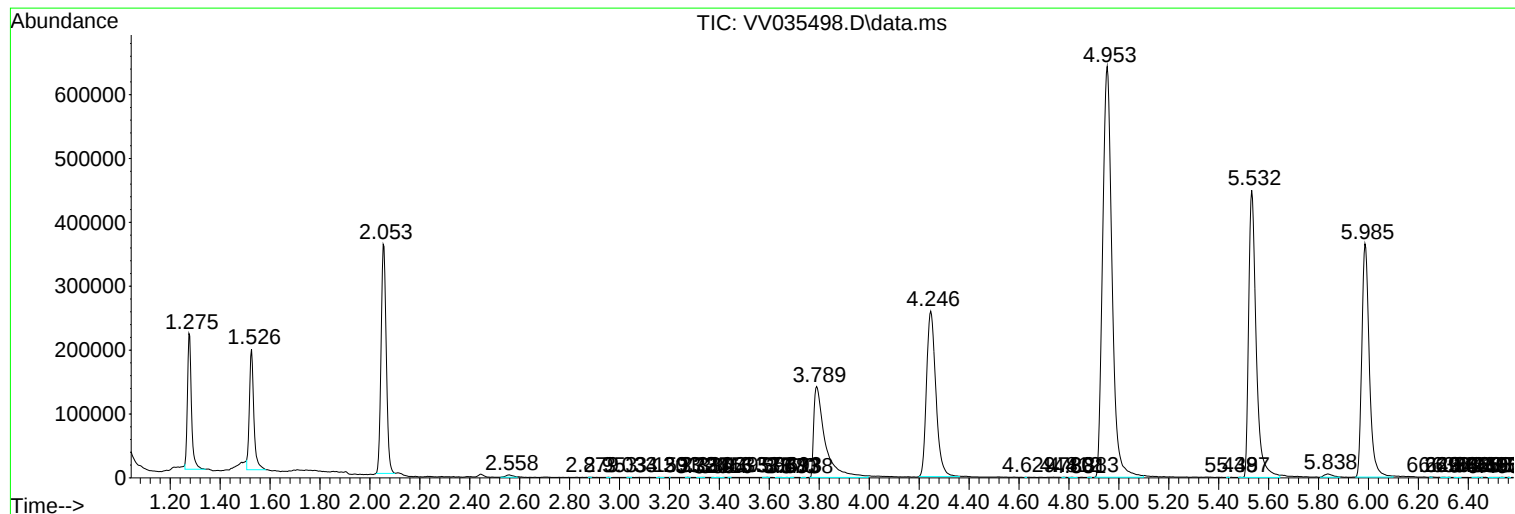

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035498.D
Acq On : 01 May 2024 15:55
Operator : SY/MD
Sample : P2279-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035498.D
Acq On : 01 May 2024 15:55
Operator : SY/MD
Sample : P2279-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc