

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035499.D
 Acq On : 01 May 2024 16:18
 Operator : SY/MD
 Sample : P2321-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M

Title : VOC Analysis

Signal : TIC: VV035499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	91	rVB	249864	271708	15.10%	2.061%
2	1.529	145	152	171	rVB	224959	268197	14.91%	2.035%
3	2.056	306	316	330	rBV	428954	612479	34.04%	4.647%
4	2.272	367	383	394	rBV4	5668	20047	1.11%	0.152%
5	2.381	409	417	431	rBV	17572	29857	1.66%	0.227%
6	2.571	474	476	480	rVB2	573	363	0.02%	0.003%
7	2.706	513	518	519	rBV3	718	454	0.03%	0.003%
8	2.870	564	569	577	rVB2	489	599	0.03%	0.005%
9	2.908	578	581	586	rBV2	217	228	0.01%	0.002%
10	2.937	586	590	593	rBV	297	268	0.01%	0.002%
11	3.124	645	648	650	rBV	302	214	0.01%	0.002%
12	3.465	743	754	757	rBV2	317	465	0.03%	0.004%
13	3.558	780	783	787	rBV2	275	225	0.01%	0.002%
14	3.648	808	811	817	rVB2	312	233	0.01%	0.002%
15	3.789	847	855	888	rBV	138924	404644	22.49%	3.070%
16	4.165	970	972	976	rVB3	519	260	0.01%	0.002%
17	4.246	981	997	1033	rVV	282469	733694	40.78%	5.566%
18	4.522	1079	1083	1086	rBV2	467	462	0.03%	0.004%
19	4.953	1199	1217	1252	rBV2	688986	1799169	100.00%	13.650%
20	5.249	1304	1309	1311	rBV3	656	528	0.03%	0.004%
21	5.307	1324	1327	1331	rBV4	450	407	0.02%	0.003%
22	5.436	1364	1367	1370	rVB2	366	235	0.01%	0.002%
23	5.532	1386	1397	1427	rBV	439830	923022	51.30%	7.003%
24	5.837	1481	1492	1512	rVB2	8872	21342	1.19%	0.162%
25	5.985	1525	1538	1573	rBV	390165	816540	45.38%	6.195%
26	6.275	1625	1628	1629	rBV	366	217	0.01%	0.002%
27	6.326	1641	1644	1649	rVB2	303	220	0.01%	0.002%
28	6.506	1698	1700	1703	rBV	331	224	0.01%	0.002%
29	6.587	1720	1725	1727	rBV2	468	368	0.02%	0.003%
30	6.632	1735	1739	1741	rBV3	448	242	0.01%	0.002%
31	6.792	1786	1789	1793	rVB2	306	232	0.01%	0.002%
32	6.911	1816	1826	1859	rBV	193351	379193	21.08%	2.877%
33	7.243	1917	1929	1958	rBV	782165	1396899	77.64%	10.598%
34	7.554	2016	2026	2061	rBV	138422	265363	14.75%	2.013%
35	7.850	2116	2118	2119	rBV	659	259	0.01%	0.002%
36	7.873	2120	2125	2136	rVB2	2990	4710	0.26%	0.036%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035499.D
 Acq On : 01 May 2024 16:18
 Operator : SY/MD
 Sample : P2321-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	7.989	2156	2161	2163	rBV4	315	328	0.02%	0.002%
38	8.024	2163	2172	2214	rBV	470572	869009	48.30%	6.593%
39	8.471	2308	2311	2314	rBV2	360	243	0.01%	0.002%
40	8.487	2314	2316	2318	rVB	562	248	0.01%	0.002%
41	8.706	2382	2384	2387	rVV2	426	232	0.01%	0.002%
42	8.783	2397	2408	2435	rBV	682608	1134945	63.08%	8.611%
43	9.146	2520	2521	2526	rVB3	458	275	0.02%	0.002%
44	9.236	2544	2549	2551	rBV4	404	355	0.02%	0.003%
45	9.278	2556	2562	2567	rVB3	490	374	0.02%	0.003%
46	9.403	2597	2601	2603	rBV2	429	271	0.02%	0.002%
47	9.419	2603	2606	2608	rVV2	285	214	0.01%	0.002%
48	9.445	2611	2614	2619	rVB2	331	273	0.02%	0.002%
49	9.471	2619	2622	2624	rBV2	434	271	0.02%	0.002%
50	9.596	2658	2661	2663	rVV	396	215	0.01%	0.002%
51	9.879	2742	2749	2751	rBV3	333	364	0.02%	0.003%
52	9.924	2760	2763	2767	rVB3	550	384	0.02%	0.003%
53	9.950	2767	2771	2775	rVB2	427	352	0.02%	0.003%
54	9.998	2782	2786	2791	rBV	324	281	0.02%	0.002%
55	10.152	2822	2834	2864	rVV	596479	942839	52.40%	7.153%
56	10.326	2880	2888	2898	rVB3	3773	6257	0.35%	0.047%
57	10.374	2901	2903	2909	rVB2	346	343	0.02%	0.003%
58	10.445	2920	2925	2927	rBV	364	291	0.02%	0.002%
59	10.468	2929	2932	2934	rBV3	362	257	0.01%	0.002%
60	10.532	2948	2952	2954	rBV	402	242	0.01%	0.002%
61	10.709	3004	3007	3011	rVV	373	300	0.02%	0.002%
62	10.789	3029	3032	3037	rVB2	462	356	0.02%	0.003%
63	10.914	3068	3071	3074	rVB2	392	213	0.01%	0.002%
64	10.947	3074	3081	3086	rBV2	415	499	0.03%	0.004%
65	11.037	3105	3109	3117	rVB4	506	477	0.03%	0.004%
66	11.094	3122	3127	3130	rBV2	443	301	0.02%	0.002%
67	11.123	3132	3136	3137	rBV2	610	479	0.03%	0.004%
68	11.185	3144	3155	3184	rBV	631884	1006236	55.93%	7.634%
69	11.387	3216	3218	3222	rVB3	562	360	0.02%	0.003%
70	11.461	3239	3241	3246	rVB2	782	414	0.02%	0.003%
71	11.512	3249	3257	3260	rBV5	3119	4377	0.24%	0.033%
72	11.557	3260	3271	3302	rVB	774471	1239497	68.89%	9.404%
73	11.734	3324	3326	3329	rVB3	680	335	0.02%	0.003%
74	11.853	3359	3363	3365	rBV2	569	344	0.02%	0.003%
75	11.934	3384	3388	3390	rBV4	927	651	0.04%	0.005%
76	11.998	3405	3408	3413	rBV3	468	455	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035499.D
 Acq On : 01 May 2024 16:18
 Operator : SY/MD
 Sample : P2321-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	12.085	3433	3435	3441	rVB3	443	378	0.02%	0.003%
78	12.120	3441	3446	3448	rBV2	298	269	0.01%	0.002%
79	12.197	3462	3470	3479	rVB2	997	1674	0.09%	0.013%
80	12.255	3486	3488	3492	rBV	315	251	0.01%	0.002%
81	12.307	3500	3504	3506	rBV	535	373	0.02%	0.003%
82	12.387	3526	3529	3531	rBV3	491	267	0.01%	0.002%
83	12.445	3543	3547	3550	rVB2	345	305	0.02%	0.002%
84	12.471	3550	3555	3556	rBV2	289	217	0.01%	0.002%
85	12.551	3576	3580	3584	rVB2	474	352	0.02%	0.003%
86	12.580	3587	3589	3592	rBV2	432	316	0.02%	0.002%
87	12.757	3642	3644	3647	rVB	373	215	0.01%	0.002%
88	12.847	3670	3672	3674	rBV	413	228	0.01%	0.002%
89	13.146	3762	3765	3767	rBV	465	288	0.02%	0.002%
90	13.210	3778	3785	3792	rVB5	1364	2086	0.12%	0.016%
91	13.246	3792	3796	3799	rBV2	475	338	0.02%	0.003%
92	13.458	3854	3862	3867	rBV5	1840	2209	0.12%	0.017%
93	13.573	3895	3898	3903	rVB2	362	274	0.02%	0.002%
94	13.686	3929	3933	3937	rBV4	1243	1367	0.08%	0.010%
95	14.088	4055	4058	4060	rVB	556	283	0.02%	0.002%
96	14.123	4066	4069	4071	rBV	497	324	0.02%	0.002%
97	14.175	4083	4085	4089	rVB2	472	223	0.01%	0.002%
98	14.397	4152	4154	4158	rBV3	414	326	0.02%	0.002%
99	14.522	4192	4193	4196	rBV2	437	235	0.01%	0.002%
100	15.020	4346	4348	4351	rBV3	620	306	0.02%	0.002%




Sum of corrected areas: 13180828

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035499.D
Acq On : 01 May 2024 16:18
Operator : SY/MD
Sample : P2321-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

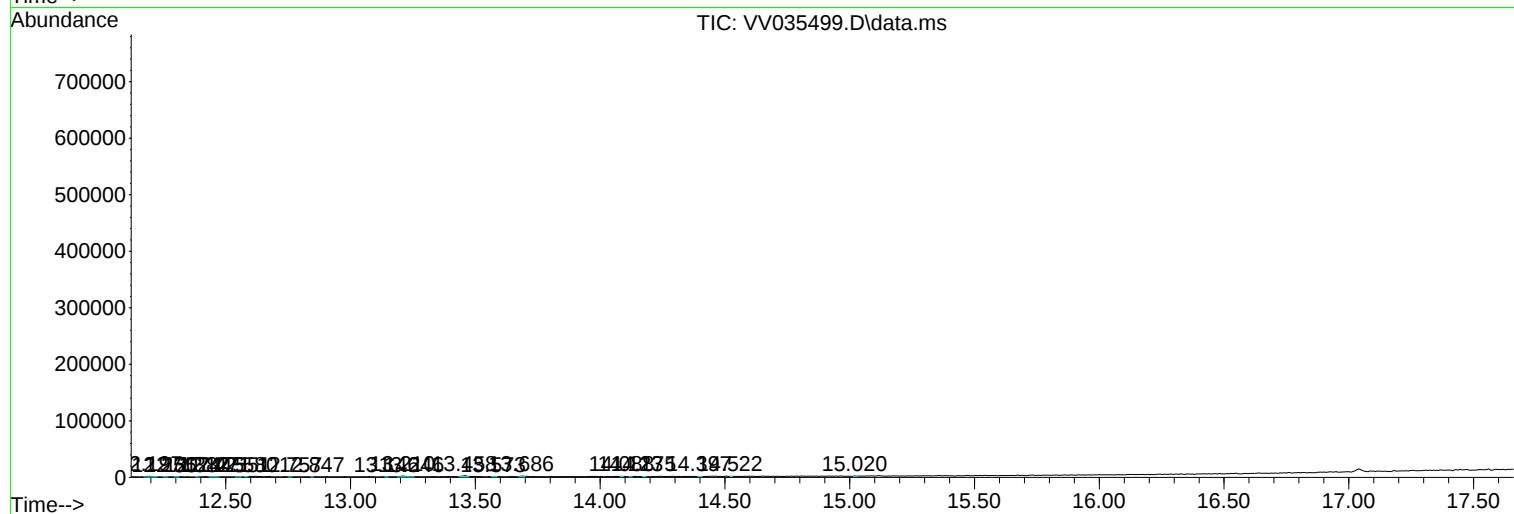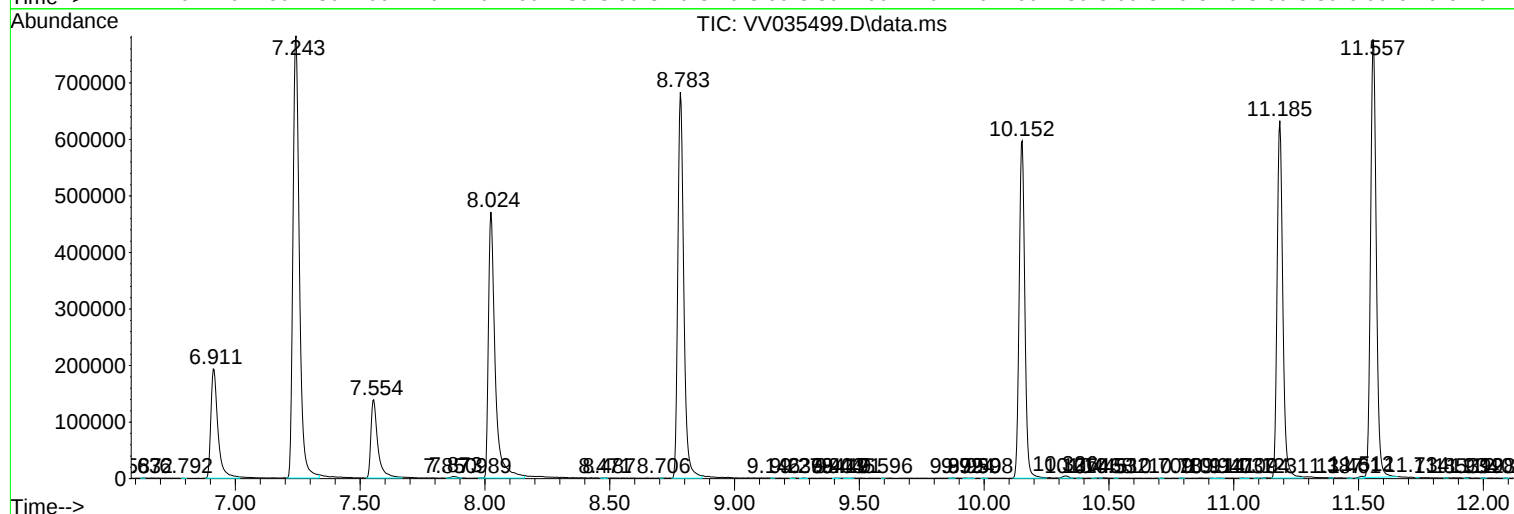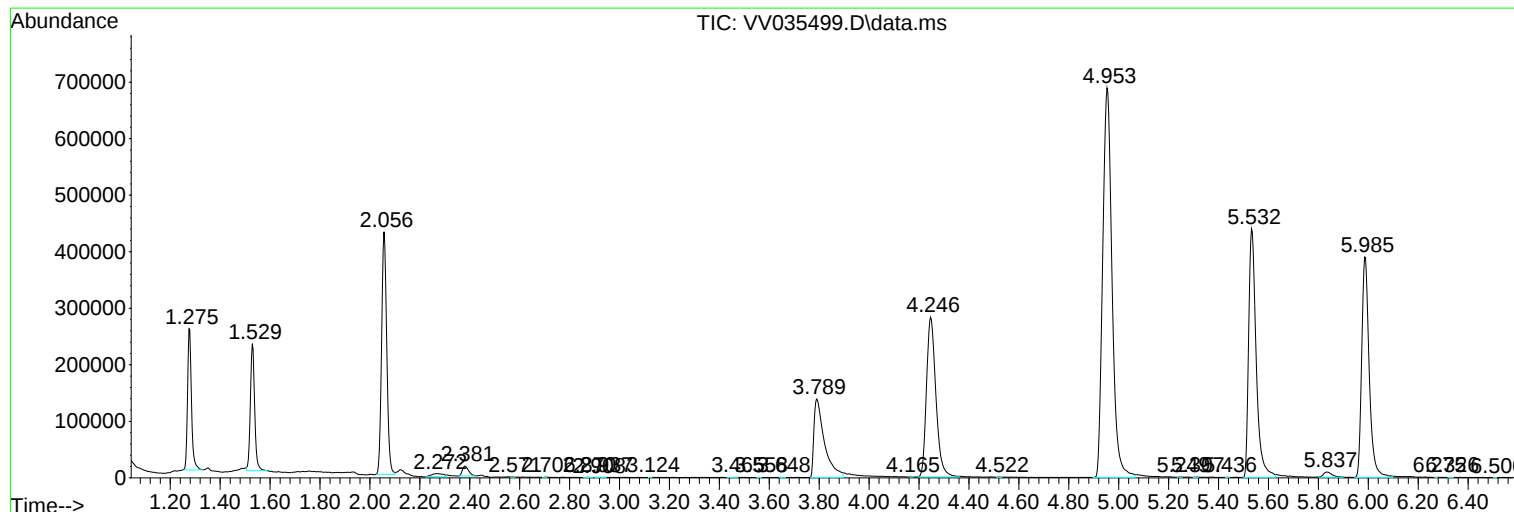

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035499.D
Acq On : 01 May 2024 16:18
Operator : SY/MD
Sample : P2321-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035499.D
Acq On : 01 May 2024 16:18
Operator : SY/MD
Sample : P2321-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc