

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035500.D
 Acq On : 01 May 2024 16:41
 Operator : SY/MD
 Sample : P2321-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	90	rVB	214167	235371	15.73%	2.048%
2	1.529	145	152	179	rVB	190090	237764	15.89%	2.069%
3	2.057	306	316	331	rBV	352946	506587	33.85%	4.409%
4	2.381	409	417	432	rBV	17974	33381	2.23%	0.291%
5	2.597	482	484	488	rBV2	376	300	0.02%	0.003%
6	2.696	510	515	516	rBV2	592	423	0.03%	0.004%
7	2.780	537	541	546	rVB2	271	351	0.02%	0.003%
8	2.806	546	549	553	rBV2	422	288	0.02%	0.003%
9	2.909	578	581	585	rVB3	477	339	0.02%	0.003%
10	3.121	638	647	649	rBV	296	287	0.02%	0.002%
11	3.204	670	673	678	rVB2	300	238	0.02%	0.002%
12	3.233	678	682	687	rBV3	259	325	0.02%	0.003%
13	3.455	747	751	755	rBV2	266	218	0.01%	0.002%
14	3.523	770	772	776	rBV2	287	196	0.01%	0.002%
15	3.597	789	795	801	rVB2	179	282	0.02%	0.002%
16	3.687	818	823	826	rBV	292	253	0.02%	0.002%
17	3.793	847	856	897	rBV2	111579	335341	22.40%	2.918%
18	4.246	981	997	1030	rBV	236514	613095	40.96%	5.336%
19	4.751	1152	1154	1160	rVV3	368	306	0.02%	0.003%
20	4.954	1201	1217	1255	rBV2	568959	1496750	100.00%	13.026%
21	5.175	1283	1286	1291	rBV3	400	435	0.03%	0.004%
22	5.217	1295	1299	1301	rBV2	479	352	0.02%	0.003%
23	5.256	1309	1311	1316	rVB2	479	290	0.02%	0.003%
24	5.282	1316	1319	1321	rBV2	413	320	0.02%	0.003%
25	5.433	1364	1366	1368	rBV2	405	239	0.02%	0.002%
26	5.532	1385	1397	1435	rBV	435667	925779	61.85%	8.057%
27	5.838	1480	1492	1510	rBV3	9232	21628	1.44%	0.188%
28	5.986	1526	1538	1570	rBV	319278	674772	45.08%	5.872%
29	6.339	1647	1648	1653	rBV2	297	216	0.01%	0.002%
30	6.468	1684	1688	1691	rBV	248	205	0.01%	0.002%
31	6.622	1729	1736	1738	rBV2	283	247	0.02%	0.002%
32	6.645	1738	1743	1751	rBV2	296	384	0.03%	0.003%
33	6.703	1758	1761	1765	rVB2	392	335	0.02%	0.003%
34	6.741	1770	1773	1777	rBV	380	272	0.02%	0.002%
35	6.838	1801	1803	1809	rBV	344	291	0.02%	0.003%
36	6.915	1816	1827	1865	rBV	157067	314564	21.02%	2.738%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035500.D
 Acq On : 01 May 2024 16:41
 Operator : SY/MD
 Sample : P2321-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	7.127	1890	1893	1898	rVB4	369	254	0.02%	0.002%
38	7.166	1898	1905	1911	rBV4	462	737	0.05%	0.006%
39	7.198	1911	1915	1917	rBV4	321	250	0.02%	0.002%
40	7.243	1917	1929	1956	rBV	635758	1138330	76.05%	9.906%
41	7.555	2016	2026	2057	rBV	111135	213522	14.27%	1.858%
42	7.873	2114	2125	2137	rBV2	3916	7560	0.51%	0.066%
43	8.024	2163	2172	2199	rBV	381175	704012	47.04%	6.127%
44	8.346	2268	2272	2274	rBV3	541	502	0.03%	0.004%
45	8.555	2335	2337	2342	rBV3	365	326	0.02%	0.003%
46	8.625	2355	2359	2361	rBV2	427	244	0.02%	0.002%
47	8.664	2367	2371	2372	rBV	324	229	0.02%	0.002%
48	8.783	2397	2408	2436	rBV	685149	1140178	76.18%	9.923%
49	9.056	2490	2493	2496	rVB4	458	249	0.02%	0.002%
50	9.101	2502	2507	2508	rBV2	553	422	0.03%	0.004%
51	9.233	2545	2548	2551	rBV2	578	419	0.03%	0.004%
52	9.346	2576	2583	2585	rBV2	368	344	0.02%	0.003%
53	9.375	2589	2592	2598	rVB3	276	223	0.01%	0.002%
54	9.439	2608	2612	2615	rBV2	389	288	0.02%	0.003%
55	9.494	2622	2629	2638	rBV4	587	1033	0.07%	0.009%
56	9.545	2643	2645	2650	rBV3	292	201	0.01%	0.002%
57	9.680	2683	2687	2692	rBV2	379	341	0.02%	0.003%
58	9.728	2697	2702	2704	rBV2	343	323	0.02%	0.003%
59	9.834	2730	2735	2740	rBV	267	357	0.02%	0.003%
60	9.883	2740	2750	2754	rBV4	518	731	0.05%	0.006%
61	9.966	2772	2776	2779	rVB2	281	256	0.02%	0.002%
62	9.982	2779	2781	2787	rBV	362	345	0.02%	0.003%
63	10.063	2802	2806	2811	rVB	360	214	0.01%	0.002%
64	10.098	2811	2817	2822	rVB3	267	351	0.02%	0.003%
65	10.149	2822	2833	2865	rBV	494559	784630	52.42%	6.828%
66	10.326	2880	2888	2900	rVB3	6230	9555	0.64%	0.083%
67	10.465	2926	2931	2932	rBV	606	436	0.03%	0.004%
68	10.535	2950	2953	2958	rBV3	263	240	0.02%	0.002%
69	10.661	2986	2992	2994	rBV	288	255	0.02%	0.002%
70	10.786	3028	3031	3036	rVB2	312	272	0.02%	0.002%
71	11.008	3097	3100	3105	rBV2	310	286	0.02%	0.002%
72	11.130	3132	3138	3141	rBV4	869	802	0.05%	0.007%
73	11.185	3144	3155	3183	rBV	635083	998565	66.72%	8.690%
74	11.465	3237	3242	3243	rBV2	613	506	0.03%	0.004%
75	11.493	3244	3251	3259	rVV2	11699	21857	1.46%	0.190%
76	11.558	3261	3271	3298	rVB	662048	1047717	70.00%	9.118%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035500.D
 Acq On : 01 May 2024 16:41
 Operator : SY/MD
 Sample : P2321-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.812	3346	3350	3354	rVB4	526	399	0.03%	0.003%
78	11.838	3354	3358	3359	rBV4	358	220	0.01%	0.002%
79	11.873	3367	3369	3371	rVB2	563	232	0.02%	0.002%
80	11.899	3374	3377	3381	rVB3	468	354	0.02%	0.003%
81	11.928	3383	3386	3388	rBV	659	440	0.03%	0.004%
82	11.976	3398	3401	3404	rVB3	580	452	0.03%	0.004%
83	12.034	3415	3419	3422	rVB	545	371	0.02%	0.003%
84	12.191	3462	3468	3476	rVB4	1458	2156	0.14%	0.019%
85	12.317	3505	3507	3511	rVV	438	333	0.02%	0.003%
86	12.513	3565	3568	3569	rBV	362	205	0.01%	0.002%
87	12.603	3588	3596	3597	rBV3	825	897	0.06%	0.008%
88	12.619	3598	3601	3602	rBV3	603	336	0.02%	0.003%
89	12.693	3620	3624	3626	rBV4	294	234	0.02%	0.002%
90	12.805	3658	3659	3662	rBV2	393	274	0.02%	0.002%
91	12.847	3669	3672	3676	rVB2	498	398	0.03%	0.003%
92	13.114	3752	3755	3757	rBV2	328	196	0.01%	0.002%
93	13.204	3780	3783	3785	rBV2	663	467	0.03%	0.004%
94	13.313	3814	3817	3818	rBV	415	225	0.02%	0.002%
95	13.452	3853	3860	3861	rBV3	1661	1350	0.09%	0.012%
96	13.680	3929	3931	3933	rBV2	562	215	0.01%	0.002%
97	13.821	3972	3975	3976	rVV2	592	329	0.02%	0.003%
98	14.098	4057	4061	4063	rBV	486	433	0.03%	0.004%
99	14.294	4119	4122	4123	rBV3	395	238	0.02%	0.002%
100	14.532	4193	4196	4197	rBV2	487	270	0.02%	0.002%




Sum of corrected areas: 11490810

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035500.D
Acq On : 01 May 2024 16:41
Operator : SY/MD
Sample : P2321-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

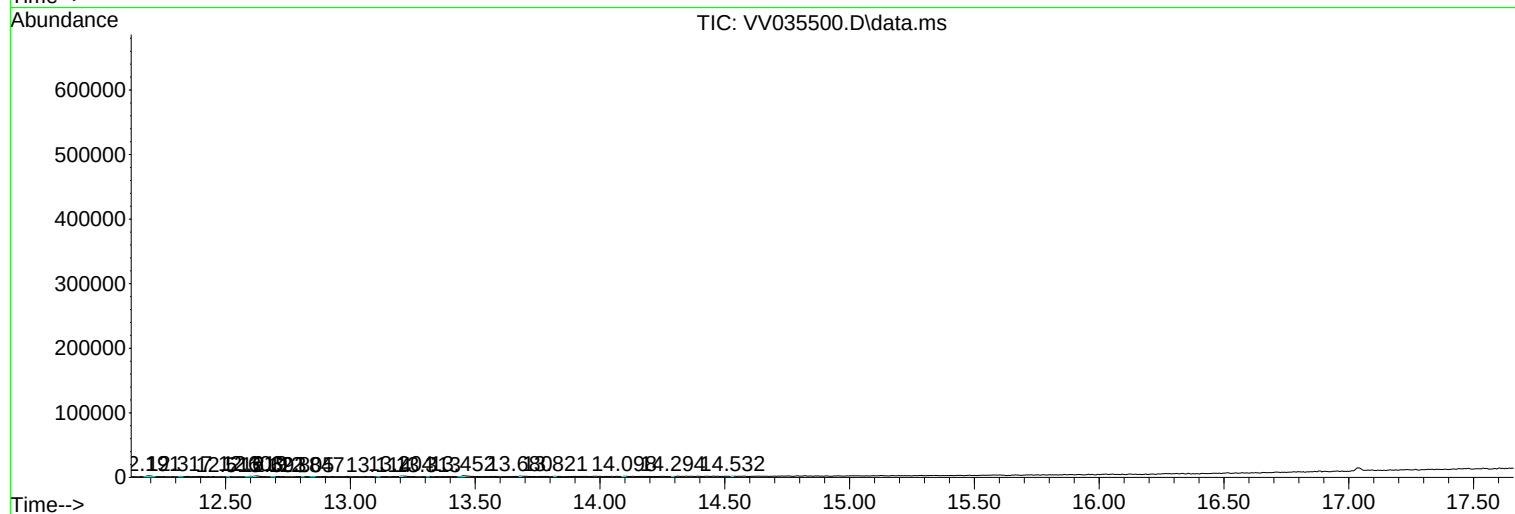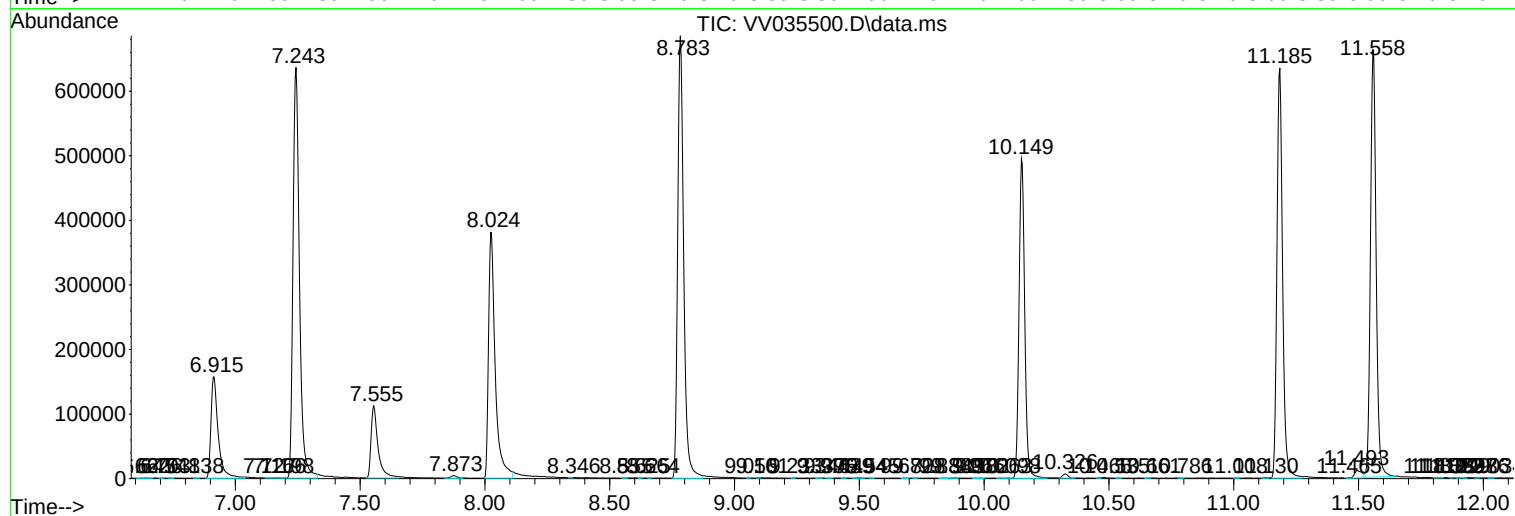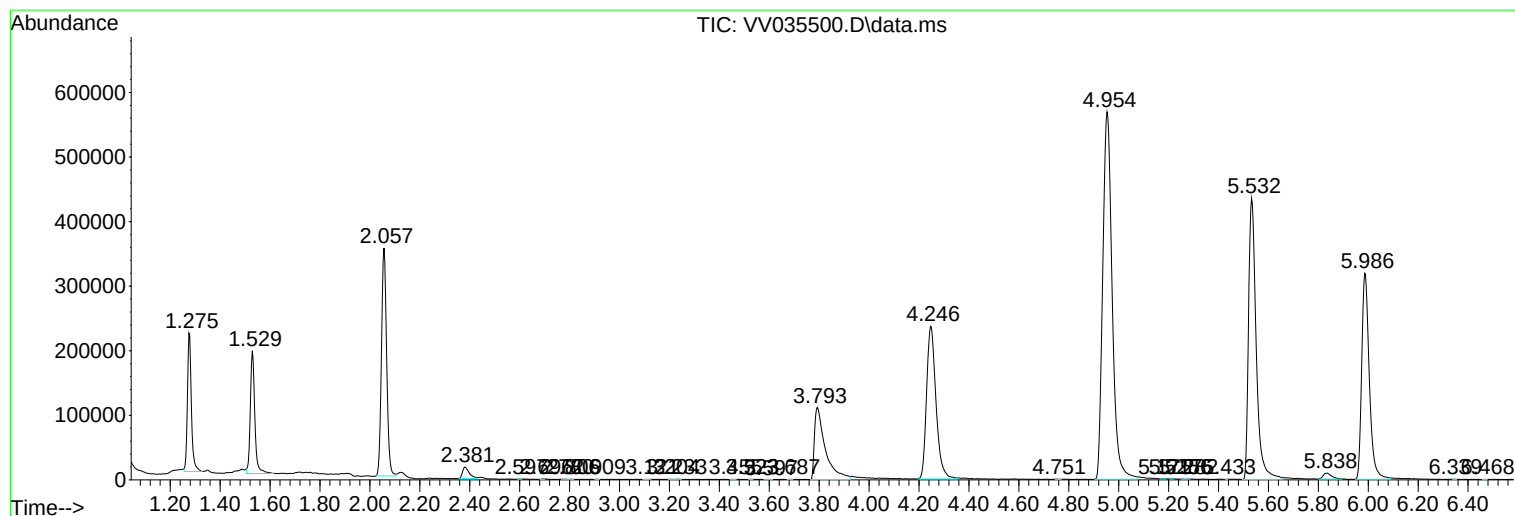

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035500.D
Acq On : 01 May 2024 16:41
Operator : SY/MD
Sample : P2321-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035500.D
Acq On : 01 May 2024 16:41
Operator : SY/MD
Sample : P2321-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------