

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035505.D
 Acq On : 01 May 2024 18:37
 Operator : SY/MD
 Sample : P2280-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M

Title : VOC Analysis

Signal : TIC: VV035505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	51	rBV	18347	16152	0.91%	0.118%
2	1.275	67	73	87	rVB	250832	271762	15.31%	1.984%
3	1.529	145	152	182	rVB	227565	279383	15.74%	2.040%
4	2.056	306	316	330	rBV	424213	608519	34.28%	4.443%
5	2.449	432	438	447	rVB4	1541	2653	0.15%	0.019%
6	2.490	447	451	457	rVB4	518	577	0.03%	0.004%
7	2.526	459	462	464	rBV	498	249	0.01%	0.002%
8	2.552	468	470	475	rBV2	331	244	0.01%	0.002%
9	2.597	478	484	488	rBV2	878	1137	0.06%	0.008%
10	2.696	511	515	521	rBV5	451	427	0.02%	0.003%
11	2.748	529	531	538	rVB	263	255	0.01%	0.002%
12	2.844	559	561	567	rVB2	338	252	0.01%	0.002%
13	2.892	567	576	587	rBV5	712	1561	0.09%	0.011%
14	3.256	685	689	694	rBV2	381	278	0.02%	0.002%
15	3.288	694	699	705	rBV2	283	253	0.01%	0.002%
16	3.584	782	791	792	rBV3	384	514	0.03%	0.004%
17	3.793	847	856	891	rBV	129975	385461	21.71%	2.815%
18	4.182	974	977	980	rBV2	432	301	0.02%	0.002%
19	4.246	980	997	1033	rVV2	293419	841009	47.37%	6.141%
20	4.474	1065	1068	1072	rVB3	442	275	0.02%	0.002%
21	4.516	1078	1081	1083	rBV3	548	339	0.02%	0.002%
22	4.642	1118	1120	1128	rVB2	540	402	0.02%	0.003%
23	4.680	1128	1132	1135	rVB2	384	271	0.02%	0.002%
24	4.703	1135	1139	1142	rBV	352	305	0.02%	0.002%
25	4.754	1151	1155	1161	rBV3	337	428	0.02%	0.003%
26	4.953	1201	1217	1250	rBV2	682243	1775316	100.00%	12.964%
27	5.532	1386	1397	1444	rBV	513656	1076141	60.62%	7.858%
28	5.838	1481	1492	1509	rVB4	6571	14349	0.81%	0.105%
29	5.986	1525	1538	1572	rBV	383892	800642	45.10%	5.846%
30	6.320	1639	1642	1647	rVB2	381	284	0.02%	0.002%
31	6.355	1647	1653	1654	rBV3	393	342	0.02%	0.002%
32	6.442	1668	1680	1696	rBV	12831	27162	1.53%	0.198%
33	6.532	1706	1708	1712	rBV2	487	261	0.01%	0.002%
34	6.580	1720	1723	1724	rBV3	415	250	0.01%	0.002%
35	6.596	1725	1728	1733	rVV4	575	572	0.03%	0.004%
36	6.654	1743	1746	1749	rVB3	426	308	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035505.D
 Acq On : 01 May 2024 18:37
 Operator : SY/MD
 Sample : P2280-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.912	1813	1826	1857	rBV	194817	374318	21.08%	2.733%
38	7.146	1892	1899	1901	rBV6	1052	1157	0.07%	0.008%
39	7.243	1918	1929	1951	rBV	779683	1374366	77.42%	10.036%
40	7.551	2014	2025	2064	rBV	137757	265280	14.94%	1.937%
41	7.773	2091	2094	2096	rBV3	588	334	0.02%	0.002%
42	7.834	2110	2113	2116	rBV2	577	552	0.03%	0.004%
43	7.873	2116	2125	2127	rBV4	2834	3528	0.20%	0.026%
44	7.921	2138	2140	2145	rVB3	508	359	0.02%	0.003%
45	7.966	2150	2154	2158	rBV3	355	371	0.02%	0.003%
46	7.992	2160	2162	2163	rBV	564	238	0.01%	0.002%
47	8.024	2163	2172	2207	rBV	469632	860851	48.49%	6.286%
48	8.455	2304	2306	2312	rVB5	364	245	0.01%	0.002%
49	8.583	2338	2346	2349	rBV5	638	849	0.05%	0.006%
50	8.722	2385	2389	2393	rVB5	451	348	0.02%	0.003%
51	8.783	2397	2408	2442	rBV	795167	1319213	74.31%	9.633%
52	9.165	2524	2527	2531	rBV4	397	259	0.01%	0.002%
53	9.207	2538	2540	2543	rVB3	636	387	0.02%	0.003%
54	9.288	2563	2565	2571	rVB2	484	291	0.02%	0.002%
55	9.349	2580	2584	2585	rBV	371	228	0.01%	0.002%
56	9.400	2597	2600	2603	rBV2	339	223	0.01%	0.002%
57	9.532	2638	2641	2645	rVB3	361	284	0.02%	0.002%
58	9.603	2659	2663	2667	rBV3	359	368	0.02%	0.003%
59	9.680	2681	2687	2688	rBV	349	360	0.02%	0.003%
60	9.979	2775	2780	2782	rBV2	560	375	0.02%	0.003%
61	10.053	2800	2803	2806	rBV	352	229	0.01%	0.002%
62	10.149	2821	2833	2864	rBV	590886	943109	53.12%	6.887%
63	10.323	2879	2887	2897	rVB2	3327	5699	0.32%	0.042%
64	10.423	2914	2918	2921	rBV2	318	290	0.02%	0.002%
65	10.455	2925	2928	2932	rBV2	363	269	0.02%	0.002%
66	10.561	2959	2961	2966	rVB3	304	283	0.02%	0.002%
67	10.706	3002	3006	3008	rBV	479	280	0.02%	0.002%
68	10.792	3029	3033	3037	rBV3	382	314	0.02%	0.002%
69	10.850	3047	3051	3053	rBV2	404	226	0.01%	0.002%
70	10.866	3053	3056	3062	rVB2	486	445	0.03%	0.003%
71	10.915	3066	3071	3072	rBV2	633	457	0.03%	0.003%
72	11.085	3121	3124	3126	rBV2	437	241	0.01%	0.002%
73	11.127	3133	3137	3138	rBV3	579	356	0.02%	0.003%
74	11.185	3143	3155	3182	rBV	741307	1172388	66.04%	8.561%
75	11.413	3225	3226	3229	rVB2	667	242	0.01%	0.002%
76	11.435	3229	3233	3236	rVV2	526	410	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
 Data File : VV035505.D
 Acq On : 01 May 2024 18:37
 Operator : SY/MD
 Sample : P2280-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.452	3236	3238	3244	rVB5	631	532	0.03%	0.004%
78	11.558	3260	3271	3298	rBV	785522	1243896	70.07%	9.083%
79	11.895	3373	3376	3383	rVB4	1023	1068	0.06%	0.008%
80	11.931	3384	3387	3392	rBV2	526	465	0.03%	0.003%
81	12.152	3452	3456	3459	rBV3	431	361	0.02%	0.003%
82	12.194	3463	3469	3480	rVB6	1092	1998	0.11%	0.015%
83	12.307	3498	3504	3508	rBV4	981	1420	0.08%	0.010%
84	12.400	3530	3533	3537	rBV2	546	496	0.03%	0.004%
85	12.448	3546	3548	3550	rBV	409	270	0.02%	0.002%
86	12.570	3582	3586	3588	rVB2	286	225	0.01%	0.002%
87	12.593	3590	3593	3598	rVV3	740	571	0.03%	0.004%
88	12.615	3598	3600	3606	rVV3	298	222	0.01%	0.002%
89	12.789	3648	3654	3655	rBV2	323	293	0.02%	0.002%
90	12.988	3713	3716	3719	rBV2	517	389	0.02%	0.003%
91	13.082	3742	3745	3749	rBV2	323	254	0.01%	0.002%
92	13.214	3780	3786	3790	rVB4	785	779	0.04%	0.006%
93	13.455	3858	3861	3864	rBV3	521	432	0.02%	0.003%
94	13.554	3889	3892	3895	rBV	500	287	0.02%	0.002%
95	13.738	3946	3949	3951	rBV2	369	222	0.01%	0.002%
96	13.750	3951	3953	3957	rVV2	382	256	0.01%	0.002%
97	13.908	4000	4002	4008	rBV2	326	253	0.01%	0.002%
98	14.014	4033	4035	4037	rBV	333	242	0.01%	0.002%
99	14.828	4286	4288	4291	rBV	659	354	0.02%	0.003%
100	15.435	4474	4477	4480	rBV3	1194	697	0.04%	0.005%




Sum of corrected areas: 13694638

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035505.D
Acq On : 01 May 2024 18:37
Operator : SY/MD
Sample : P2280-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

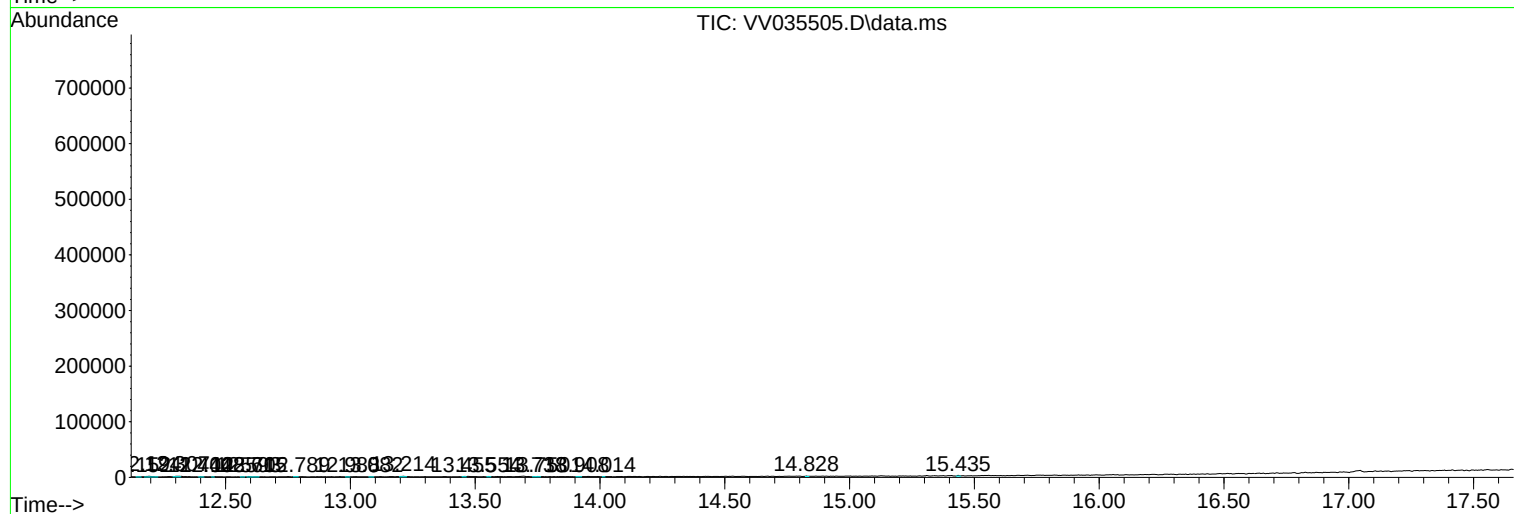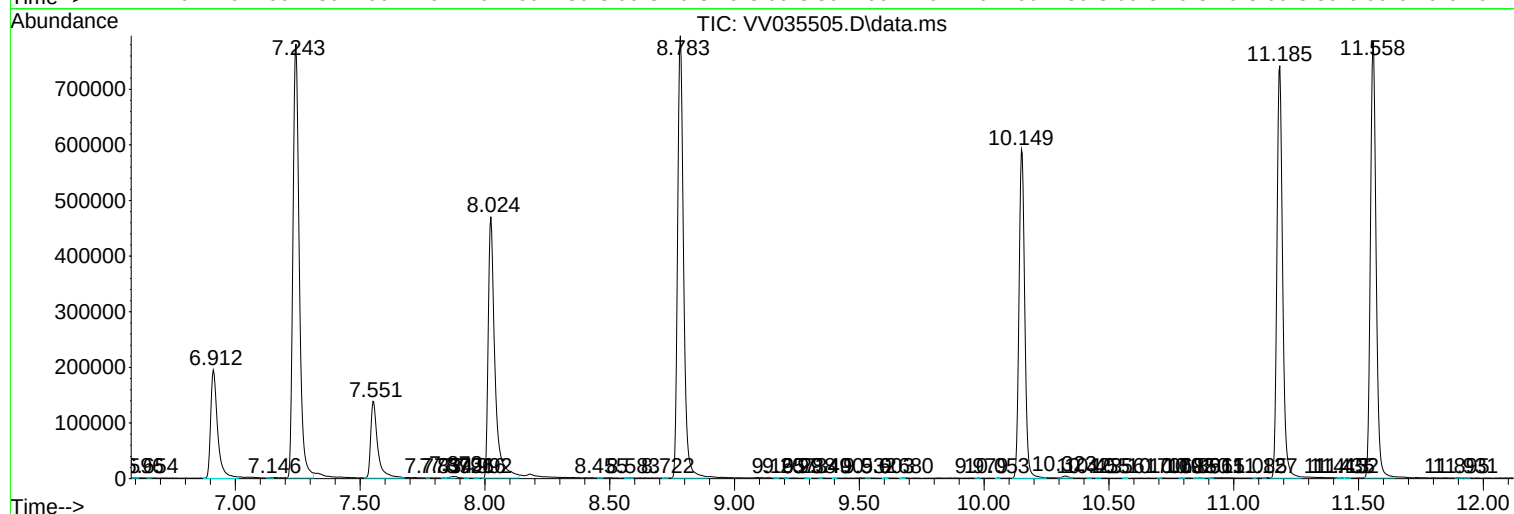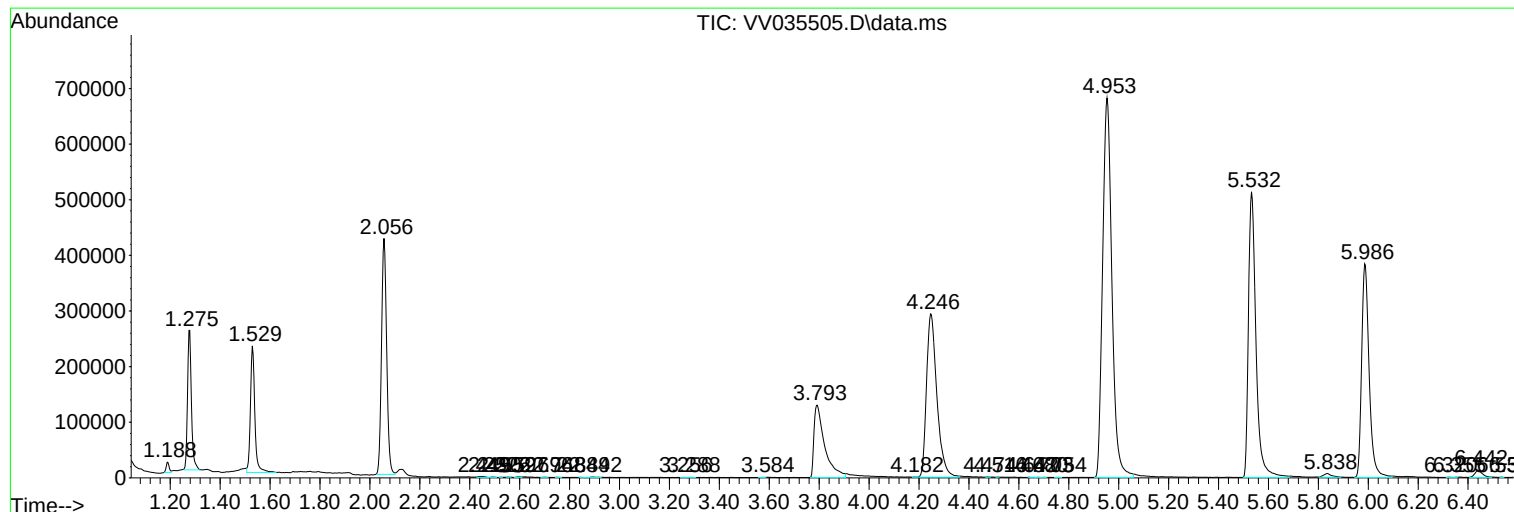

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035505.D
Acq On : 01 May 2024 18:37
Operator : SY/MD
Sample : P2280-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035505.D
Acq On : 01 May 2024 18:37
Operator : SY/MD
Sample : P2280-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
