
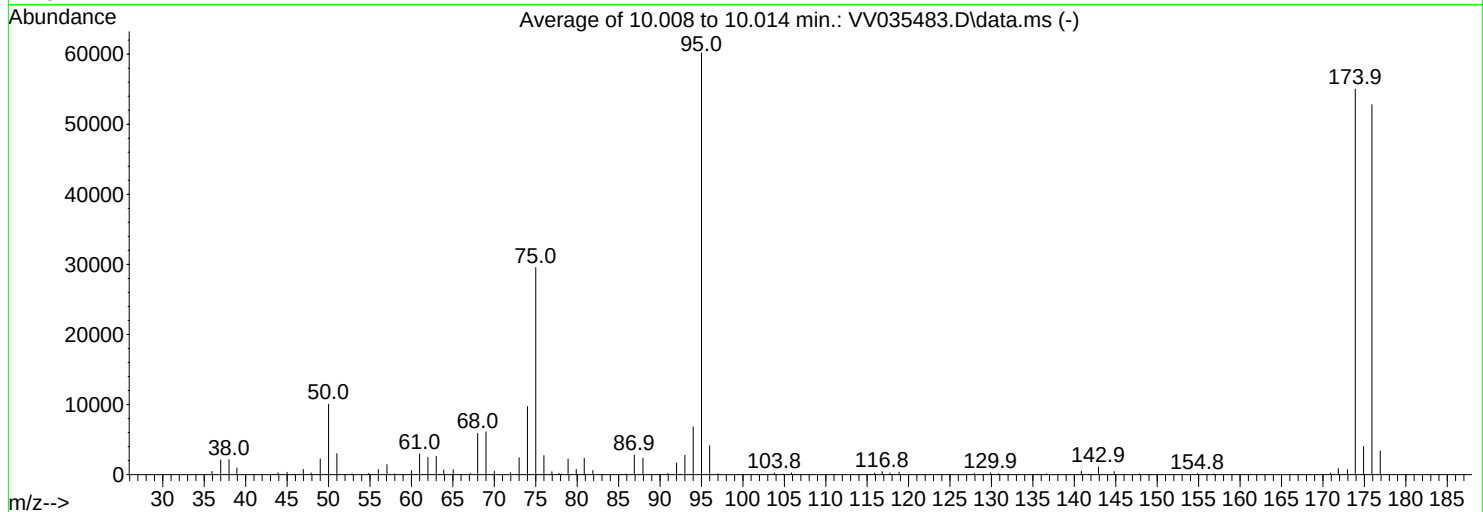


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050124\
Data File : VV035483.D
Acq On : 01 May 2024 08:58
Operator : SY/MD
Sample : BFB294
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB294

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Title : VOC Analysis
Last Update : Thu May 02 01:07:15 2024

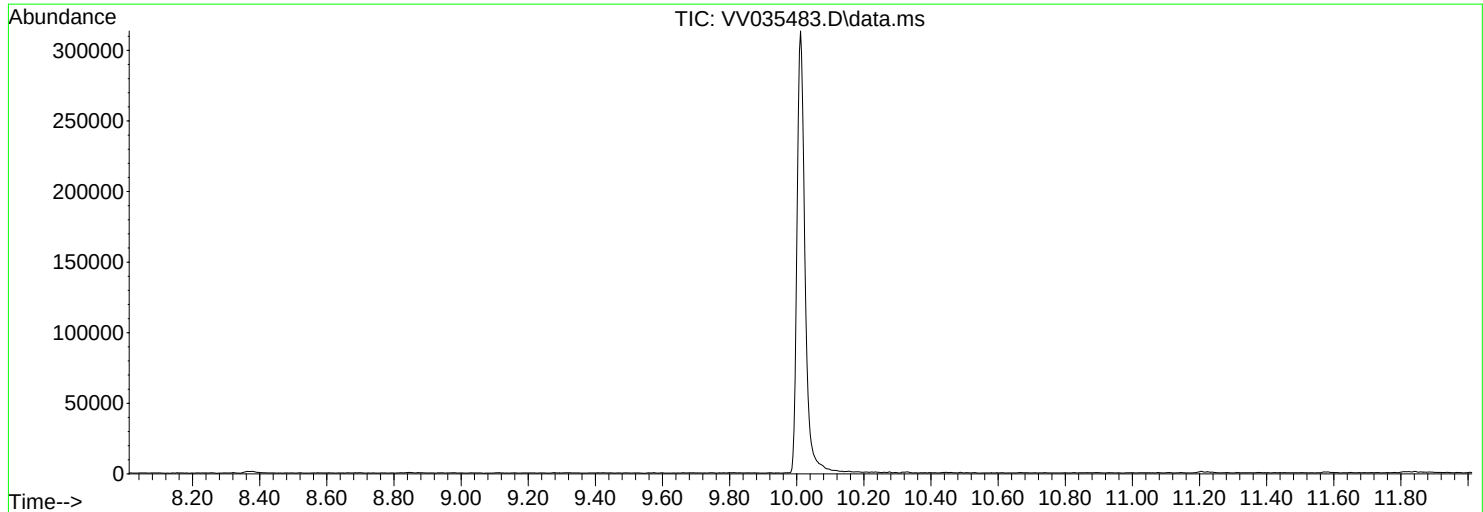

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	10047	PASS
75	95	30	80	49.1	29547	PASS
95	95	100	100	100.0	60187	PASS
96	95	5	9	6.9	4124	PASS
173	174	0.00	2	1.3	699	PASS
174	95	50	120	91.4	55024	PASS
175	174	5	9	7.3	4024	PASS
176	174	95	105	95.9	52781	PASS
177	176	5	10	6.5	3413	PASS

m/z	Abundance
39.90	262.0
43.90	535.0

Instrument :
MSVOA_V
ClientSampleId :
BFB294

m/z	Abundance
35.90	421.0
37.00	2230.0
38.00	2202.0
38.90	1001.0
39.90	283.0
43.90	832.0
45.00	275.0
47.00	679.0
47.90	265.0
49.00	2225.0
50.00	10112.0
51.00	2994.0
52.80	135.0
54.90	178.0
56.00	784.0
57.00	1495.0
58.00	120.0
60.00	630.0
61.00	3159.0
62.00	2548.0
63.00	2532.0
63.90	647.0
65.10	706.0
67.10	145.0
68.00	6163.0
69.00	6121.0
70.00	468.0
71.90	336.0
73.00	2391.0
74.00	9925.0
75.00	29496.0
76.00	2658.0
77.00	393.0
77.80	325.0
78.90	2176.0
79.90	711.0
80.90	2327.0
81.90	537.0
85.90	101.0
86.90	2928.0
88.00	2333.0
90.90	182.0
92.00	1648.0
93.00	2665.0
94.00	6719.0
95.00	59800.0
96.00	4205.0
97.00	147.0
103.80	274.0
105.80	227.0
115.90	249.0
116.80	438.0
117.70	243.0
118.90	300.0
127.90	247.0
129.90	238.0
130.80	144.0
136.60	114.0
140.80	461.0
142.90	1123.0
144.80	456.0
147.90	114.0
154.80	137.0
156.80	146.0
170.90	185.0
171.90	864.0
172.90	713.0
173.90	52872.0
174.90	3947.0
175.90	50856.0
176.90	3357.0

Instrument :
MSVOA_V
ClientSampleId :
BFB294

m/z	Abundance
36.00	468.0
37.00	2153.0
38.00	2255.0
39.00	974.0
39.90	261.0
43.90	827.0
45.00	347.0
45.90	113.0
47.00	800.0
47.90	269.0
49.00	2297.0
50.00	10416.0
51.00	3065.0
52.80	150.0
54.90	187.0
56.00	760.0
57.00	1484.0
58.00	114.0
60.00	594.0
61.00	3106.0
62.00	2530.0
63.00	2755.0
63.90	654.0
65.10	710.0
67.10	169.0
68.00	6070.0
69.00	6346.0
70.00	539.0
72.00	307.0
73.00	2451.0
74.00	10001.0
75.00	30512.0
76.00	2810.0
76.90	408.0
77.80	287.0
78.90	2325.0
79.90	789.0
80.80	2421.0
81.90	613.0
85.90	112.0
86.90	2978.0
87.90	2365.0
91.00	204.0
92.00	1746.0
93.00	2862.0
94.00	6981.0
95.00	62208.0
96.00	4229.0
97.00	123.0
103.80	270.0
104.90	146.0
105.90	247.0
115.90	242.0
116.80	431.0
117.70	266.0
118.90	337.0
127.90	223.0
129.90	261.0
130.90	160.0
136.60	123.0
140.80	518.0
141.70	114.0
142.90	1131.0
144.80	453.0
147.90	131.0
154.80	162.0
156.80	122.0
170.90	222.0
171.80	885.0
172.90	727.0
173.90	56960.0
174.90	4183.0
175.90	54624.0
176.90	3513.0
177.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB294

m/z	Abundance
36.00	468.0
37.00	1943.0
38.00	2007.0
39.00	898.0
40.00	239.0
43.90	760.0
45.00	437.0
45.90	101.0
46.90	814.0
47.90	249.0
49.00	2163.0
50.00	9612.0
51.00	2937.0
52.90	112.0
54.80	158.0
56.00	650.0
57.10	1361.0
57.90	104.0
60.00	505.0
61.00	2669.0
62.00	2348.0
63.00	2586.0
63.90	615.0
65.00	720.0
65.90	111.0
67.10	168.0
68.00	5470.0
69.00	5881.0
70.00	523.0
72.00	283.0
73.00	2391.0
74.00	9221.0
75.00	28632.0
76.00	2678.0
77.00	410.0
78.10	301.0
78.90	2239.0
79.90	768.0
80.80	2282.0
81.90	616.0
85.90	116.0
86.90	2518.0
87.90	2330.0
91.00	247.0
92.00	1639.0
93.00	2751.0
94.00	6787.0
95.00	58552.0
96.00	3938.0
97.00	121.0
103.80	225.0
104.80	139.0
105.90	259.0
115.90	228.0
116.80	417.0
117.80	269.0
118.80	365.0
127.90	181.0
129.90	266.0
130.90	142.0
136.60	119.0
140.90	518.0
141.70	111.0
142.90	1009.0
144.80	418.0
147.80	165.0
154.90	178.0
156.90	111.0
170.90	250.0
171.90	853.0
173.00	658.0
173.90	55240.0
174.90	3943.0
175.90	52864.0
176.90	3369.0
178.00	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB294