

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035512.D
 Acq On : 02 May 2024 11:00
 Operator : SY/MD
 Sample : VV0502WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK281

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	94	rVB	258208	279119	15.43%	2.029%
2	1.529	145	152	171	rVB	229652	272609	15.07%	1.982%
3	2.056	306	316	333	rBV	428148	619815	34.25%	4.506%
4	2.220	363	367	368	rBV	1094	668	0.04%	0.005%
5	2.230	368	370	372	rVV2	680	407	0.02%	0.003%
6	2.333	399	402	404	rBV2	451	308	0.02%	0.002%
7	2.449	431	438	451	rVB5	2437	3996	0.22%	0.029%
8	2.703	513	517	522	rVB2	950	871	0.05%	0.006%
9	2.854	562	564	568	rVV2	317	234	0.01%	0.002%
10	2.999	604	609	612	rBV3	346	277	0.02%	0.002%
11	3.153	652	657	660	rBV	315	283	0.02%	0.002%
12	3.256	685	689	691	rBV2	347	227	0.01%	0.002%
13	3.298	699	702	706	rBV	290	233	0.01%	0.002%
14	3.333	709	713	715	rVV	228	218	0.01%	0.002%
15	3.532	768	775	779	rBV2	259	276	0.02%	0.002%
16	3.626	799	804	807	rBV	306	332	0.02%	0.002%
17	3.790	846	855	906	rBV	131659	398111	22.00%	2.894%
18	4.246	980	997	1038	rVV	285202	743603	41.10%	5.406%
19	4.638	1117	1119	1122	rVB2	397	206	0.01%	0.001%
20	4.896	1197	1199	1201	rBV2	346	219	0.01%	0.002%
21	4.953	1201	1217	1255	rBV2	692161	1809418	100.00%	13.154%
22	5.320	1328	1331	1333	rBV3	706	356	0.02%	0.003%
23	5.461	1368	1375	1376	rBV3	428	440	0.02%	0.003%
24	5.532	1384	1397	1434	rBV	511755	1077527	59.55%	7.833%
25	5.838	1481	1492	1504	rBV5	6879	15557	0.86%	0.113%
26	5.986	1525	1538	1582	rVV	390116	819153	45.27%	5.955%
27	6.188	1599	1601	1608	rVB5	872	505	0.03%	0.004%
28	6.304	1633	1637	1639	rBV3	359	265	0.01%	0.002%
29	6.342	1646	1649	1654	rBV2	512	345	0.02%	0.003%
30	6.500	1696	1698	1707	rVB	370	320	0.02%	0.002%
31	6.629	1733	1738	1739	rBV2	444	283	0.02%	0.002%
32	6.680	1752	1754	1757	rVB	405	238	0.01%	0.002%
33	6.770	1779	1782	1787	rVB3	462	425	0.02%	0.003%
34	6.802	1787	1792	1798	rBV2	194	239	0.01%	0.002%
35	6.912	1815	1826	1853	rBV	191732	370221	20.46%	2.691%
36	7.159	1898	1903	1909	rVB4	699	787	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035512.D
 Acq On : 02 May 2024 11:00
 Operator : SY/MD
 Sample : VV0502WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK281

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	7.240	1916	1928	1973	rBV	777780	1395843	77.14%	10.147%
38	7.551	2016	2025	2057	rBV	138341	258357	14.28%	1.878%
39	7.876	2116	2126	2130	rBV4	1822	2609	0.14%	0.019%
40	7.912	2135	2137	2142	rVB5	501	419	0.02%	0.003%
41	8.024	2163	2172	2220	rBV	465681	877413	48.49%	6.379%
42	8.574	2341	2343	2347	rVB3	393	223	0.01%	0.002%
43	8.670	2370	2373	2376	rVB2	437	225	0.01%	0.002%
44	8.696	2378	2381	2383	rVB2	420	255	0.01%	0.002%
45	8.783	2393	2408	2443	rBV	802634	1342495	74.19%	9.760%
46	9.030	2481	2485	2492	rVB4	697	739	0.04%	0.005%
47	9.079	2496	2500	2503	rBV4	513	489	0.03%	0.004%
48	9.169	2525	2528	2529	rBV4	309	206	0.01%	0.001%
49	9.265	2553	2558	2559	rBV2	310	234	0.01%	0.002%
50	9.487	2623	2627	2629	rBV3	375	273	0.02%	0.002%
51	9.538	2641	2643	2648	rVB4	493	389	0.02%	0.003%
52	9.564	2648	2651	2653	rVV	356	205	0.01%	0.001%
53	9.664	2677	2682	2685	rVB2	261	224	0.01%	0.002%
54	9.690	2685	2690	2693	rBV2	400	376	0.02%	0.003%
55	9.873	2742	2747	2750	rBV	556	624	0.03%	0.005%
56	10.034	2795	2797	2800	rVV2	420	230	0.01%	0.002%
57	10.053	2800	2803	2806	rVB3	517	342	0.02%	0.002%
58	10.149	2820	2833	2864	rBV	606461	960689	53.09%	6.984%
59	10.323	2885	2887	2897	rVB2	2185	2493	0.14%	0.018%
60	10.416	2913	2916	2921	rVB3	396	363	0.02%	0.003%
61	10.487	2930	2938	2944	rBV3	792	1142	0.06%	0.008%
62	10.522	2946	2949	2952	rVB2	418	264	0.01%	0.002%
63	10.542	2952	2955	2958	rBV3	286	207	0.01%	0.002%
64	10.863	3048	3055	3061	rBV2	670	1063	0.06%	0.008%
65	11.001	3094	3098	3100	rBV	317	247	0.01%	0.002%
66	11.053	3111	3114	3120	rBV3	329	301	0.02%	0.002%
67	11.130	3132	3138	3143	rBV6	1680	2404	0.13%	0.017%
68	11.185	3143	3155	3188	rVV	747978	1183959	65.43%	8.607%
69	11.558	3256	3271	3298	rBV	787613	1259711	69.62%	9.158%
70	11.792	3341	3344	3349	rBV3	457	440	0.02%	0.003%
71	11.924	3382	3385	3388	rBV2	263	226	0.01%	0.002%
72	12.014	3409	3413	3415	rBV2	495	319	0.02%	0.002%
73	12.185	3462	3466	3467	rBV2	451	329	0.02%	0.002%
74	12.265	3488	3491	3495	rBV3	406	292	0.02%	0.002%
75	12.284	3495	3497	3500	rVB2	452	224	0.01%	0.002%
76	12.317	3504	3507	3510	rBV3	377	318	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035512.D
 Acq On : 02 May 2024 11:00
 Operator : SY/MD
 Sample : VV0502WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK281

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	12.365	3517	3522	3524	rBV4	409	431	0.02%	0.003%
78	12.429	3539	3542	3545	rVV2	511	399	0.02%	0.003%
79	12.448	3545	3548	3551	rVB2	431	302	0.02%	0.002%
80	12.590	3586	3592	3604	rVB4	2415	3682	0.20%	0.027%
81	12.757	3641	3644	3646	rVB	392	229	0.01%	0.002%
82	12.870	3674	3679	3682	rBV	420	316	0.02%	0.002%
83	12.972	3707	3711	3714	rBV2	438	333	0.02%	0.002%
84	13.008	3719	3722	3725	rBV2	371	328	0.02%	0.002%
85	13.075	3739	3743	3745	rBV2	243	211	0.01%	0.002%
86	13.114	3752	3755	3759	rBV2	234	213	0.01%	0.002%
87	13.207	3776	3784	3796	rVB5	4529	8153	0.45%	0.059%
88	13.262	3799	3801	3804	rBV	383	264	0.01%	0.002%
89	13.368	3831	3834	3838	rBV3	345	327	0.02%	0.002%
90	13.448	3850	3859	3875	rBV	7702	13902	0.77%	0.101%
91	13.641	3916	3919	3922	rVB	432	268	0.01%	0.002%
92	13.686	3925	3933	3944	rVB7	4614	7974	0.44%	0.058%
93	13.947	4012	4014	4017	rVV2	349	206	0.01%	0.001%
94	14.059	4047	4049	4054	rBV3	363	235	0.01%	0.002%
95	14.271	4112	4115	4119	rVB3	821	613	0.03%	0.004%
96	14.304	4120	4125	4126	rBV3	472	448	0.02%	0.003%
97	14.368	4142	4145	4146	rBV2	416	233	0.01%	0.002%
98	14.992	4337	4339	4342	rBV4	494	346	0.02%	0.003%
99	15.056	4356	4359	4362	rBV3	756	545	0.03%	0.004%
100	15.095	4368	4371	4372	rBV3	743	473	0.03%	0.003%

Sum of corrected areas: 13755683




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035512.D
Acq On : 02 May 2024 11:00
Operator : SY/MD
Sample : VV0502WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

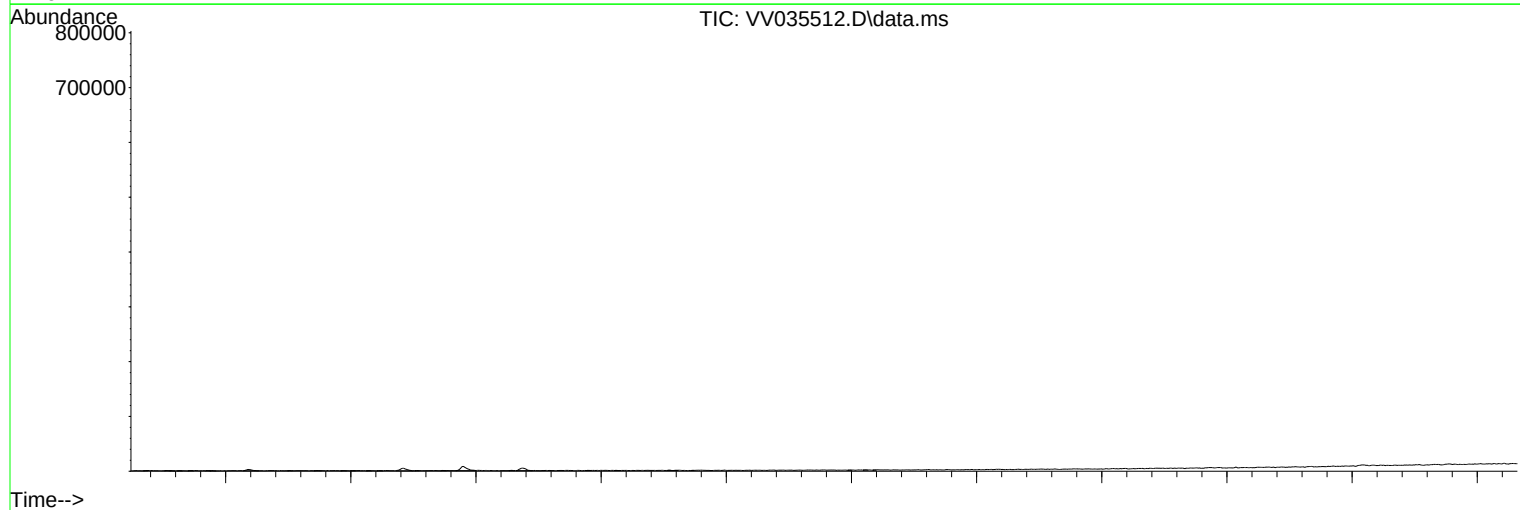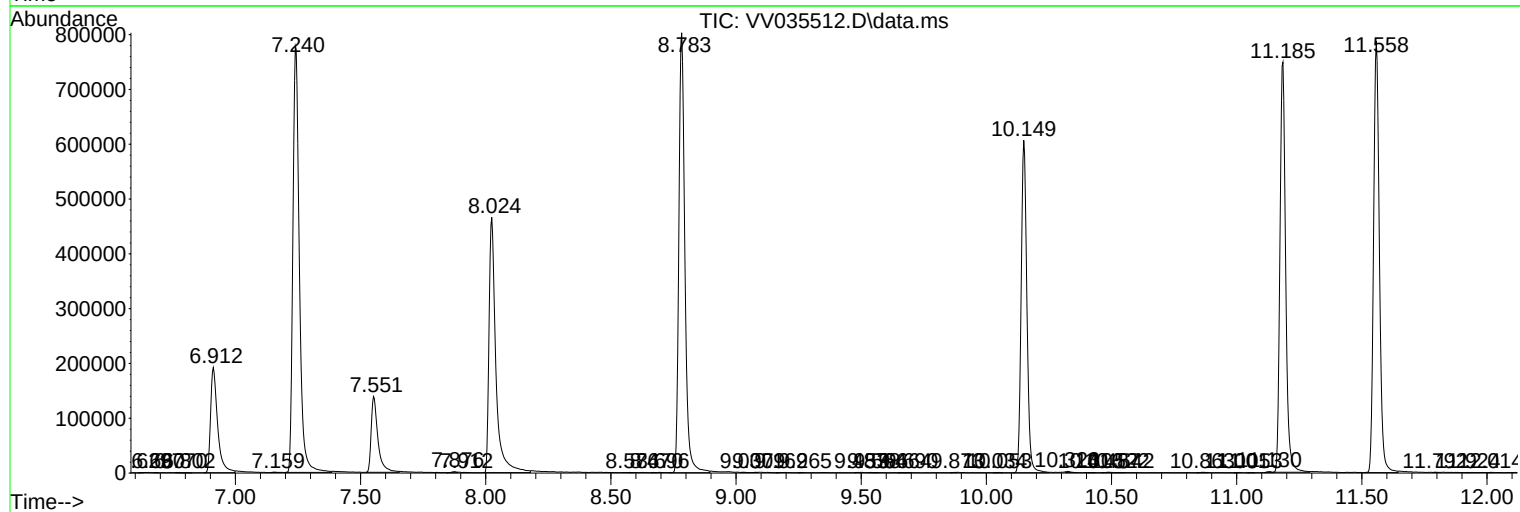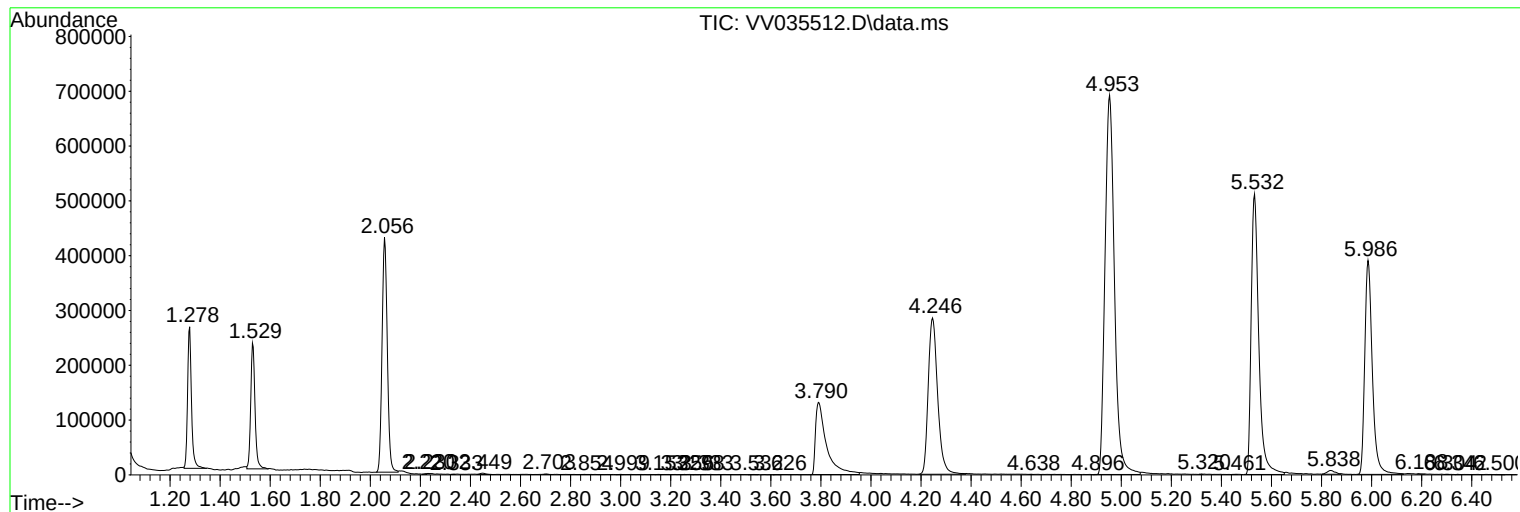

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035512.D
Acq On : 02 May 2024 11:00
Operator : SY/MD
Sample : VV0502WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035512.D
Acq On : 02 May 2024 11:00
Operator : SY/MD
Sample : VV0502WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------