

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035513.D
 Acq On : 02 May 2024 11:22
 Operator : SY/MD
 Sample : P2220-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	253806	264848	15.05%	1.976%
2	1.529	145	152	168	rVB	221218	263020	14.95%	1.962%
3	2.056	306	316	333	rBV	413883	606353	34.46%	4.523%
4	2.320	396	398	401	rVB2	385	217	0.01%	0.002%
5	2.384	415	418	421	rVB3	437	262	0.01%	0.002%
6	2.449	430	438	447	rVB7	2077	3613	0.21%	0.027%
7	2.484	447	449	456	rVB3	431	300	0.02%	0.002%
8	2.513	456	458	462	rVB2	352	275	0.02%	0.002%
9	2.545	464	468	470	rBV2	324	246	0.01%	0.002%
10	2.703	512	517	521	rBV4	480	484	0.03%	0.004%
11	2.764	532	536	538	rBV2	325	292	0.02%	0.002%
12	2.883	567	573	575	rBV	299	262	0.01%	0.002%
13	3.249	681	687	688	rBV2	249	247	0.01%	0.002%
14	3.362	719	722	727	rVB2	272	229	0.01%	0.002%
15	3.667	813	817	823	rBV3	238	228	0.01%	0.002%
16	3.744	838	841	846	rVB2	285	251	0.01%	0.002%
17	3.789	846	855	891	rBV	131122	383146	21.77%	2.858%
18	4.246	981	997	1035	rBV	278284	719158	40.87%	5.365%
19	4.603	1105	1108	1112	rVB3	426	259	0.01%	0.002%
20	4.664	1123	1127	1135	rVB	485	578	0.03%	0.004%
21	4.738	1146	1150	1151	rBV	414	304	0.02%	0.002%
22	4.770	1157	1160	1165	rBV2	337	253	0.01%	0.002%
23	4.834	1176	1180	1182	rBV	385	315	0.02%	0.002%
24	4.953	1201	1217	1250	rBV2	671055	1759701	100.00%	13.127%
25	5.339	1333	1337	1343	rBV2	316	307	0.02%	0.002%
26	5.532	1386	1397	1432	rBV	496673	1044507	59.36%	7.792%
27	5.834	1481	1491	1507	rBV3	6986	15760	0.90%	0.118%
28	5.928	1515	1520	1523	rBV4	472	385	0.02%	0.003%
29	5.985	1525	1538	1567	rBV	378580	794582	45.15%	5.928%
30	6.243	1613	1618	1621	rBV3	514	456	0.03%	0.003%
31	6.416	1669	1672	1674	rBV3	397	250	0.01%	0.002%
32	6.458	1680	1685	1690	rVB3	261	271	0.02%	0.002%
33	6.625	1733	1737	1741	rBV2	294	286	0.02%	0.002%
34	6.651	1741	1745	1747	rVV2	506	419	0.02%	0.003%
35	6.664	1747	1749	1752	rVB3	359	229	0.01%	0.002%
36	6.725	1765	1768	1772	rBV	489	366	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035513.D
 Acq On : 02 May 2024 11:22
 Operator : SY/MD
 Sample : P2220-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.911	1816	1826	1866	rBV	187297	366704	20.84%	2.736%
38	7.127	1891	1893	1896	rVB3	518	231	0.01%	0.002%
39	7.156	1896	1902	1904	rBV4	498	525	0.03%	0.004%
40	7.243	1918	1929	1965	rBV	755713	1354307	76.96%	10.103%
41	7.551	2016	2025	2064	rBV	133562	258392	14.68%	1.928%
42	7.802	2098	2103	2105	rVB3	615	443	0.03%	0.003%
43	7.847	2115	2117	2120	rBV2	276	214	0.01%	0.002%
44	7.876	2122	2126	2133	rVB4	748	816	0.05%	0.006%
45	7.915	2133	2138	2140	rBV3	414	261	0.01%	0.002%
46	7.989	2157	2161	2163	rBV2	339	244	0.01%	0.002%
47	8.024	2163	2172	2216	rBV	457577	856868	48.69%	6.392%
48	8.461	2305	2308	2311	rBV2	339	228	0.01%	0.002%
49	8.567	2338	2341	2344	rBV3	335	249	0.01%	0.002%
50	8.645	2364	2365	2372	rVB4	418	342	0.02%	0.003%
51	8.783	2394	2408	2439	rBV	796062	1315318	74.75%	9.812%
52	9.127	2513	2515	2518	rBV2	243	215	0.01%	0.002%
53	9.236	2545	2549	2553	rVB	521	336	0.02%	0.003%
54	9.288	2563	2565	2570	rVB3	401	268	0.02%	0.002%
55	9.487	2624	2627	2629	rBV3	449	316	0.02%	0.002%
56	9.616	2664	2667	2669	rBV2	293	239	0.01%	0.002%
57	9.651	2673	2678	2680	rVV2	354	314	0.02%	0.002%
58	9.767	2711	2714	2720	rVB3	349	313	0.02%	0.002%
59	9.931	2761	2765	2769	rBV2	272	211	0.01%	0.002%
60	10.149	2821	2833	2856	rBV	601924	948762	53.92%	7.078%
61	10.474	2931	2934	2935	rVV2	546	278	0.02%	0.002%
62	10.484	2935	2937	2944	rVB2	635	688	0.04%	0.005%
63	10.667	2990	2994	2998	rVB2	297	209	0.01%	0.002%
64	10.760	3020	3023	3026	rBV2	433	289	0.02%	0.002%
65	10.866	3052	3056	3057	rBV2	355	209	0.01%	0.002%
66	10.876	3057	3059	3062	rVV2	522	288	0.02%	0.002%
67	11.133	3132	3139	3143	rBV4	1536	2076	0.12%	0.015%
68	11.185	3144	3155	3185	rBV	740537	1169768	66.48%	8.726%
69	11.471	3240	3244	3247	rVB2	357	246	0.01%	0.002%
70	11.558	3256	3271	3299	rBV	772319	1242874	70.63%	9.272%
71	11.763	3333	3335	3341	rVB3	514	351	0.02%	0.003%
72	12.050	3421	3424	3428	rBV3	312	267	0.02%	0.002%
73	12.072	3428	3431	3434	rVV2	285	229	0.01%	0.002%
74	12.088	3434	3436	3444	rVB3	372	311	0.02%	0.002%
75	12.185	3462	3466	3467	rBV2	366	233	0.01%	0.002%
76	12.194	3467	3469	3473	rVV	414	275	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035513.D
 Acq On : 02 May 2024 11:22
 Operator : SY/MD
 Sample : P2220-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	12.220	3473	3477	3480	rVB3	502	371	0.02%	0.003%
78	12.265	3488	3491	3497	rBV3	480	414	0.02%	0.003%
79	12.387	3527	3529	3531	rBV3	390	222	0.01%	0.002%
80	12.567	3581	3585	3587	rBV	410	301	0.02%	0.002%
81	12.831	3663	3667	3672	rVB2	427	297	0.02%	0.002%
82	12.895	3684	3687	3689	rVV2	395	246	0.01%	0.002%
83	12.972	3708	3711	3715	rVB2	381	282	0.02%	0.002%
84	13.021	3719	3726	3727	rBV2	408	301	0.02%	0.002%
85	13.033	3728	3730	3735	rVB2	364	250	0.01%	0.002%
86	13.159	3767	3769	3775	rBV2	251	205	0.01%	0.002%
87	13.207	3778	3784	3785	rBV3	2302	1862	0.11%	0.014%
88	13.326	3816	3821	3822	rBV3	336	298	0.02%	0.002%
89	13.455	3854	3861	3873	rVV3	3008	5220	0.30%	0.039%
90	13.545	3886	3889	3892	rBV2	561	485	0.03%	0.004%
91	13.609	3907	3909	3918	rBV3	471	709	0.04%	0.005%
92	13.689	3927	3934	3941	rBV6	2287	3098	0.18%	0.023%
93	13.741	3947	3950	3953	rBV2	366	299	0.02%	0.002%
94	13.760	3954	3956	3959	rVB2	562	301	0.02%	0.002%
95	14.062	4048	4050	4053	rBV3	393	280	0.02%	0.002%
96	14.246	4104	4107	4110	rBV4	477	343	0.02%	0.003%
97	14.278	4115	4117	4122	rVV3	371	268	0.02%	0.002%
98	14.432	4162	4165	4170	rBV3	790	864	0.05%	0.006%
99	14.641	4228	4230	4232	rBV	498	232	0.01%	0.002%
100	14.718	4252	4254	4257	rBV3	570	438	0.02%	0.003%

Sum of corrected areas: 13404952




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035513.D
Acq On : 02 May 2024 11:22
Operator : SY/MD
Sample : P2220-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

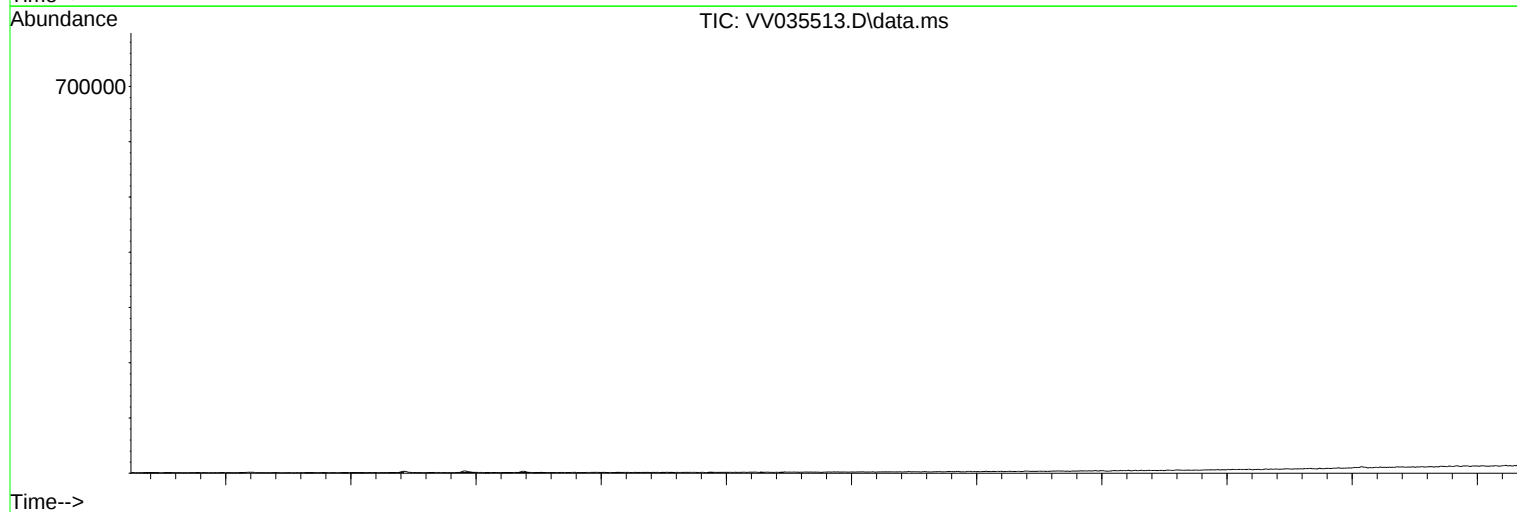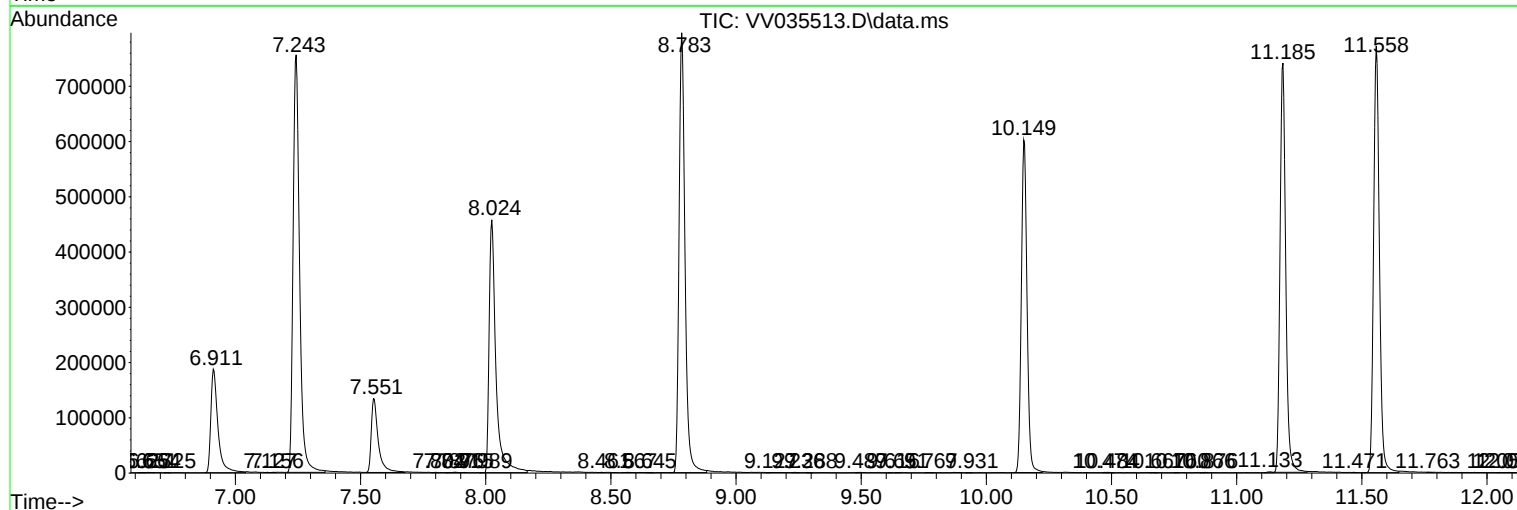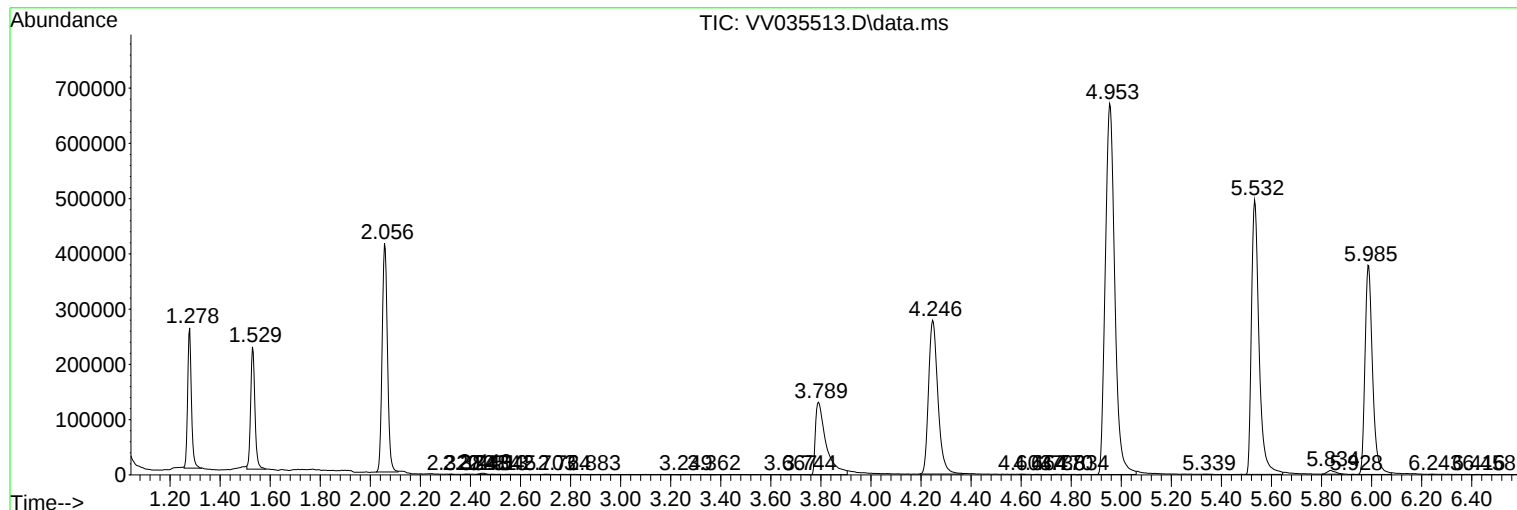

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035513.D
Acq On : 02 May 2024 11:22
Operator : SY/MD
Sample : P2220-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035513.D
Acq On : 02 May 2024 11:22
Operator : SY/MD
Sample : P2220-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------