

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035514.D
 Acq On : 02 May 2024 11:45
 Operator : SY/MD
 Sample : P2321-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	91	rVB	254945	274724	14.76%	1.904%
2	1.529	145	152	168	rVB	228707	266370	14.31%	1.846%
3	2.057	305	316	331	rBV	438918	639661	34.37%	4.433%
4	2.227	366	369	370	rBV2	558	327	0.02%	0.002%
5	2.381	410	417	432	rVB	14871	26657	1.43%	0.185%
6	2.622	490	492	496	rVB3	468	314	0.02%	0.002%
7	2.677	503	509	513	rBV2	226	284	0.02%	0.002%
8	2.700	513	516	517	rVV2	466	300	0.02%	0.002%
9	2.793	541	545	548	rBV	270	267	0.01%	0.002%
10	2.812	548	551	555	rVV3	411	347	0.02%	0.002%
11	2.909	576	581	584	rBV3	245	288	0.02%	0.002%
12	3.076	629	633	635	rBV2	322	242	0.01%	0.002%
13	3.298	696	702	707	rBV3	314	387	0.02%	0.003%
14	3.474	750	757	762	rVB2	223	308	0.02%	0.002%
15	3.507	762	767	769	rBV2	354	267	0.01%	0.002%
16	3.793	844	856	908	rBV	136989	437473	23.51%	3.032%
17	4.246	981	997	1035	rBV	293931	764678	41.09%	5.300%
18	4.825	1171	1177	1183	rBV3	465	514	0.03%	0.004%
19	4.854	1183	1186	1191	rBV3	371	239	0.01%	0.002%
20	4.886	1193	1196	1200	rBV3	306	306	0.02%	0.002%
21	4.954	1201	1217	1252	rBV2	706914	1860896	100.00%	12.898%
22	5.346	1335	1339	1341	rBV3	377	322	0.02%	0.002%
23	5.532	1386	1397	1430	rBV	551347	1155783	62.11%	8.011%
24	5.831	1479	1490	1507	rBV3	13275	30332	1.63%	0.210%
25	5.925	1516	1519	1524	rVB5	440	418	0.02%	0.003%
26	5.986	1524	1538	1574	rBV	400287	840281	45.15%	5.824%
27	6.285	1627	1631	1634	rVB2	368	326	0.02%	0.002%
28	6.330	1639	1645	1648	rBV2	298	335	0.02%	0.002%
29	6.371	1655	1658	1660	rVB	388	271	0.01%	0.002%
30	6.449	1679	1682	1686	rBV2	372	295	0.02%	0.002%
31	6.584	1719	1724	1728	rBV2	374	338	0.02%	0.002%
32	6.622	1732	1736	1738	rBV3	517	379	0.02%	0.003%
33	6.735	1766	1771	1774	rBV3	426	449	0.02%	0.003%
34	6.912	1816	1826	1864	rBV	202417	394467	21.20%	2.734%
35	7.111	1886	1888	1892	rVB3	656	305	0.02%	0.002%
36	7.153	1899	1901	1904	rBV3	543	367	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035514.D
 Acq On : 02 May 2024 11:45
 Operator : SY/MD
 Sample : P2321-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	7.243	1917	1929	1965	rBV	809844	1455660	78.22%	10.089%
38	7.500	2007	2009	2013	rVB4	403	254	0.01%	0.002%
39	7.551	2016	2025	2054	rBV	144700	270020	14.51%	1.871%
40	7.780	2092	2096	2101	rBV5	764	688	0.04%	0.005%
41	7.876	2114	2126	2133	rBV2	5134	9189	0.49%	0.064%
42	8.024	2162	2172	2209	rBV	481421	908367	48.81%	6.296%
43	8.330	2264	2267	2271	rBV3	579	410	0.02%	0.003%
44	8.584	2344	2346	2353	rVB3	363	290	0.02%	0.002%
45	8.664	2368	2371	2375	rVB3	384	324	0.02%	0.002%
46	8.783	2396	2408	2447	rBV	865276	1447483	77.78%	10.032%
47	9.053	2490	2492	2497	rVB3	668	446	0.02%	0.003%
48	9.088	2497	2503	2504	rBV2	722	657	0.04%	0.005%
49	9.162	2522	2526	2528	rBV2	348	272	0.01%	0.002%
50	9.201	2534	2538	2539	rBV2	412	258	0.01%	0.002%
51	9.420	2599	2606	2609	rBV3	499	440	0.02%	0.003%
52	9.445	2609	2614	2616	rBV3	350	372	0.02%	0.003%
53	9.580	2652	2656	2659	rVB2	337	251	0.01%	0.002%
54	9.703	2691	2694	2698	rBV2	261	273	0.01%	0.002%
55	9.883	2743	2750	2759	rVB3	643	918	0.05%	0.006%
56	10.149	2818	2833	2856	rBV	610665	971194	52.19%	6.731%
57	10.323	2876	2887	2903	rVB	6449	12244	0.66%	0.085%
58	10.487	2924	2938	2945	rBV7	1068	2299	0.12%	0.016%
59	10.667	2990	2994	3000	rBV	405	429	0.02%	0.003%
60	10.860	3051	3054	3057	rBV3	550	382	0.02%	0.003%
61	11.030	3103	3107	3111	rBV3	396	309	0.02%	0.002%
62	11.130	3132	3138	3143	rBV5	1273	1598	0.09%	0.011%
63	11.182	3143	3154	3181	rBV	817881	1282922	68.94%	8.892%
64	11.503	3247	3254	3255	rBV3	2938	2440	0.13%	0.017%
65	11.558	3260	3271	3301	rVB	852250	1330410	71.49%	9.221%
66	11.911	3378	3381	3384	rVB2	498	246	0.01%	0.002%
67	11.947	3390	3392	3394	rBV2	487	298	0.02%	0.002%
68	12.021	3409	3415	3419	rBV3	409	422	0.02%	0.003%
69	12.088	3431	3436	3439	rBV3	438	465	0.02%	0.003%
70	12.127	3445	3448	3452	rBV	334	278	0.01%	0.002%
71	12.194	3461	3469	3478	rVV4	1404	2278	0.12%	0.016%
72	12.317	3503	3507	3508	rVV2	530	299	0.02%	0.002%
73	12.358	3516	3520	3527	rVB4	519	540	0.03%	0.004%
74	12.391	3527	3530	3533	rVB2	344	239	0.01%	0.002%
75	12.413	3533	3537	3540	rBV	387	392	0.02%	0.003%
76	12.593	3585	3593	3598	rBV4	1867	2392	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035514.D
 Acq On : 02 May 2024 11:45
 Operator : SY/MD
 Sample : P2321-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	12.702	3624	3627	3633	rVB2	501	400	0.02%	0.003%
78	12.841	3668	3670	3673	rVB2	620	295	0.02%	0.002%
79	12.863	3673	3677	3680	rBV	408	331	0.02%	0.002%
80	12.908	3685	3691	3695	rBV2	371	384	0.02%	0.003%
81	12.979	3709	3713	3716	rBV2	387	368	0.02%	0.003%
82	13.210	3777	3785	3794	rVV4	2641	4174	0.22%	0.029%
83	13.268	3799	3803	3806	rBV	608	535	0.03%	0.004%
84	13.452	3851	3860	3862	rBV5	2987	3637	0.20%	0.025%
85	13.593	3898	3904	3906	rBV	509	606	0.03%	0.004%
86	13.651	3917	3922	3926	rBV2	386	448	0.02%	0.003%
87	13.686	3926	3933	3942	rVV6	2146	3061	0.16%	0.021%
88	13.879	3991	3993	3997	rBV3	374	306	0.02%	0.002%
89	14.088	4055	4058	4061	rBV3	380	266	0.01%	0.002%
90	14.226	4097	4101	4105	rBV2	407	462	0.02%	0.003%
91	14.249	4105	4108	4110	rBV3	415	269	0.01%	0.002%
92	14.368	4143	4145	4147	rVV3	483	247	0.01%	0.002%
93	14.403	4151	4156	4157	rBV3	548	449	0.02%	0.003%
94	14.570	4206	4208	4215	rBV5	635	703	0.04%	0.005%
95	14.815	4281	4284	4285	rBV2	444	261	0.01%	0.002%
96	14.937	4320	4322	4331	rVB4	898	936	0.05%	0.006%
97	14.995	4338	4340	4343	rVB2	580	272	0.01%	0.002%
98	15.107	4373	4375	4376	rBV	854	387	0.02%	0.003%
99	15.191	4399	4401	4402	rBV	832	352	0.02%	0.002%
100	15.423	4470	4473	4477	rBV4	883	868	0.05%	0.006%

Sum of corrected areas: 14428182




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035514.D
Acq On : 02 May 2024 11:45
Operator : SY/MD
Sample : P2321-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

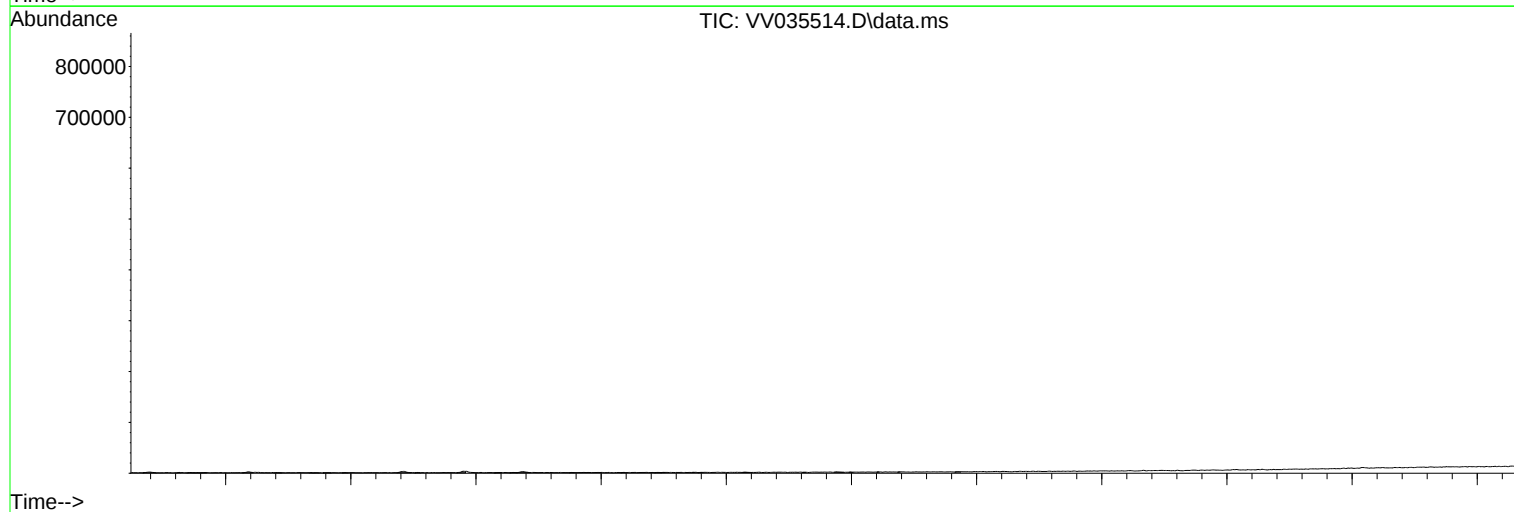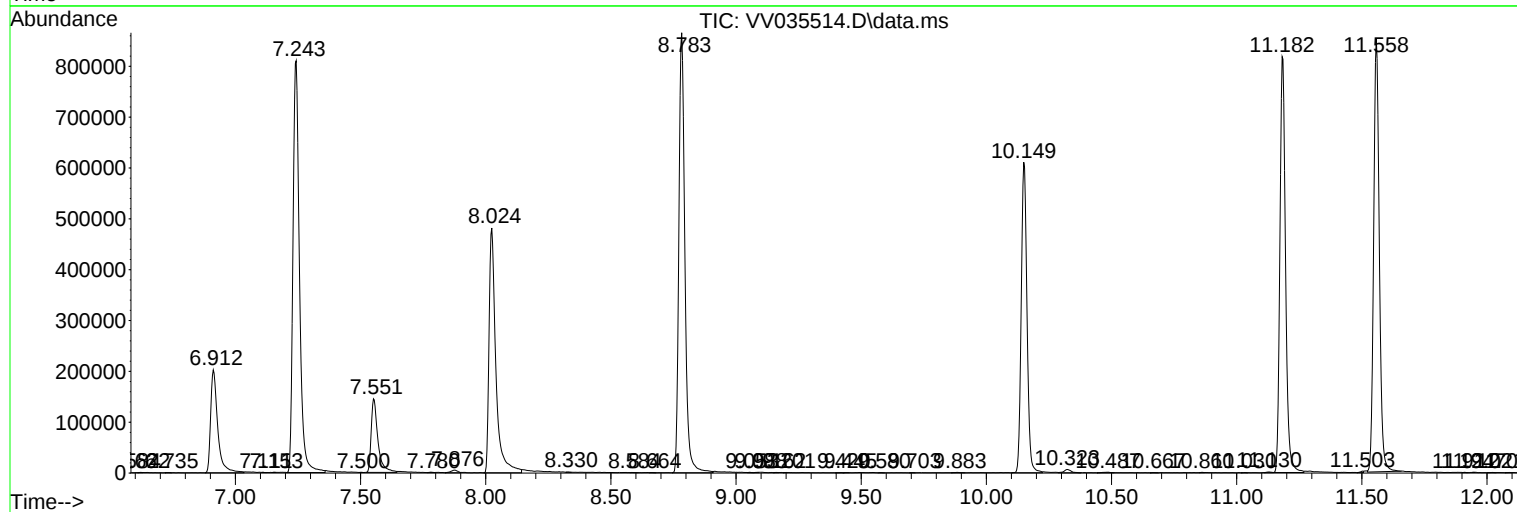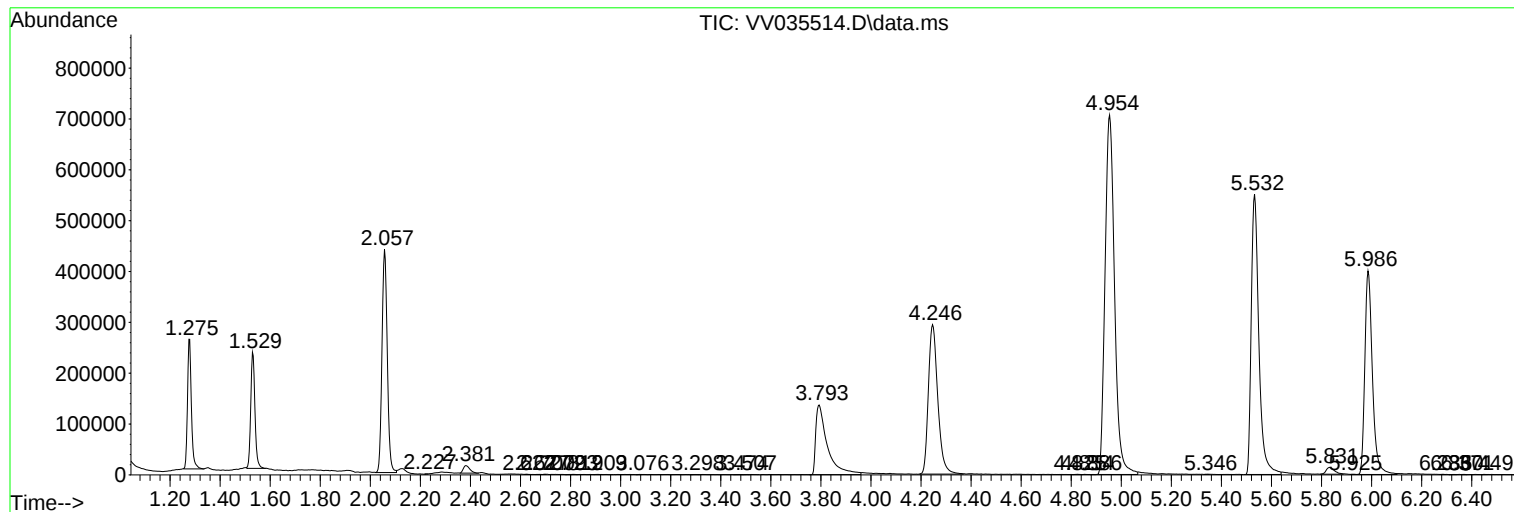

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035514.D
Acq On : 02 May 2024 11:45
Operator : SY/MD
Sample : P2321-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035514.D
Acq On : 02 May 2024 11:45
Operator : SY/MD
Sample : P2321-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------