

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035515.D
 Acq On : 02 May 2024 12:08
 Operator : SY/MD
 Sample : P2321-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	239467	259856	14.76%	1.908%
2	1.529	145	152	174	rVB	222092	268474	15.25%	1.971%
3	2.056	306	316	330	rBV	416712	598658	34.00%	4.395%
4	2.272	366	383	384	rBV3	5511	11639	0.66%	0.085%
5	2.381	409	417	430	rBV	14735	26228	1.49%	0.193%
6	2.548	464	469	470	rBV2	815	725	0.04%	0.005%
7	2.654	498	502	505	rBV2	423	255	0.01%	0.002%
8	2.706	512	518	526	rVB4	684	920	0.05%	0.007%
9	2.748	526	531	532	rBV	364	240	0.01%	0.002%
10	2.908	576	581	583	rVV3	401	348	0.02%	0.003%
11	3.387	726	730	735	rVB3	353	355	0.02%	0.003%
12	3.413	735	738	745	rBV	225	287	0.02%	0.002%
13	3.497	760	764	769	rVB2	262	252	0.01%	0.002%
14	3.690	820	824	829	rBV2	212	273	0.02%	0.002%
15	3.789	846	855	896	rBV	135405	416769	23.67%	3.060%
16	4.246	981	997	1030	rBV	279594	726759	41.27%	5.336%
17	4.577	1093	1100	1104	rVB5	385	411	0.02%	0.003%
18	4.699	1136	1138	1141	rVB3	416	261	0.01%	0.002%
19	4.744	1146	1152	1154	rBV2	396	350	0.02%	0.003%
20	4.895	1194	1199	1201	rBV	380	352	0.02%	0.003%
21	4.953	1201	1217	1252	rBV2	675438	1760958	100.00%	12.929%
22	5.227	1295	1302	1305	rBV5	573	608	0.03%	0.004%
23	5.259	1310	1312	1316	rVB3	507	325	0.02%	0.002%
24	5.532	1386	1397	1432	rBV	510275	1069612	60.74%	7.853%
25	5.831	1480	1490	1514	rBV3	18915	42967	2.44%	0.315%
26	5.985	1525	1538	1576	rVV	385536	801989	45.54%	5.888%
27	6.207	1605	1607	1613	rVB2	633	533	0.03%	0.004%
28	6.268	1624	1626	1632	rVB3	491	429	0.02%	0.003%
29	6.436	1673	1678	1680	rVV4	411	382	0.02%	0.003%
30	6.619	1730	1735	1737	rBV2	443	447	0.03%	0.003%
31	6.690	1755	1757	1762	rVB3	347	242	0.01%	0.002%
32	6.911	1816	1826	1858	rBV	188060	370007	21.01%	2.717%
33	7.156	1896	1902	1907	rBV4	1017	1219	0.07%	0.009%
34	7.178	1907	1909	1914	rVB5	818	504	0.03%	0.004%
35	7.243	1914	1929	1965	rBV	762085	1369196	77.75%	10.053%
36	7.487	2002	2005	2009	rVB2	407	307	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035515.D
 Acq On : 02 May 2024 12:08
 Operator : SY/MD
 Sample : P2321-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	7.555	2016	2026	2053	rBV	134796	254642	14.46%	1.870%
38	7.696	2068	2070	2079	rVB6	960	1168	0.07%	0.009%
39	7.731	2079	2081	2088	rBV5	458	401	0.02%	0.003%
40	7.799	2100	2102	2106	rVB2	543	368	0.02%	0.003%
41	7.873	2108	2125	2135	rBV2	5267	10209	0.58%	0.075%
42	7.982	2157	2159	2163	rVB2	340	263	0.01%	0.002%
43	8.024	2163	2172	2213	rBV	452536	861901	48.95%	6.328%
44	8.336	2267	2269	2274	rBV4	474	387	0.02%	0.003%
45	8.657	2366	2369	2377	rVB3	403	579	0.03%	0.004%
46	8.699	2377	2382	2384	rBV3	385	302	0.02%	0.002%
47	8.715	2384	2387	2390	rVB2	440	295	0.02%	0.002%
48	8.741	2390	2395	2397	rBV3	457	408	0.02%	0.003%
49	8.783	2397	2408	2438	rBV	812083	1335057	75.81%	9.802%
50	8.995	2471	2474	2477	rVB3	566	364	0.02%	0.003%
51	9.085	2500	2502	2506	rVV3	426	277	0.02%	0.002%
52	9.181	2529	2532	2533	rBV	445	280	0.02%	0.002%
53	9.223	2542	2545	2549	rVV2	398	246	0.01%	0.002%
54	9.307	2568	2571	2575	rBV3	415	341	0.02%	0.003%
55	9.490	2626	2628	2633	rVV4	437	336	0.02%	0.002%
56	9.590	2653	2659	2664	rVB4	407	503	0.03%	0.004%
57	9.670	2681	2684	2688	rBV2	366	308	0.02%	0.002%
58	9.882	2748	2750	2754	rVB	647	362	0.02%	0.003%
59	10.149	2821	2833	2867	rBV	575305	907051	51.51%	6.660%
60	10.326	2877	2888	2898	rVB	11533	18233	1.04%	0.134%
61	10.442	2922	2924	2926	rVV2	436	248	0.01%	0.002%
62	10.474	2926	2934	2941	rVB5	808	1524	0.09%	0.011%
63	10.545	2953	2956	2962	rVB3	432	376	0.02%	0.003%
64	10.812	3032	3039	3041	rBV2	240	278	0.02%	0.002%
65	10.857	3048	3053	3056	rBV3	860	836	0.05%	0.006%
66	10.873	3056	3058	3061	rVB3	578	324	0.02%	0.002%
67	10.915	3066	3071	3073	rBV	339	292	0.02%	0.002%
68	11.130	3133	3138	3143	rBV4	1003	1158	0.07%	0.009%
69	11.185	3143	3155	3178	rBV	758797	1193943	67.80%	8.766%
70	11.432	3230	3232	3235	rVB3	643	281	0.02%	0.002%
71	11.506	3247	3255	3259	rBV5	4918	7659	0.43%	0.056%
72	11.558	3260	3271	3302	rVB	795656	1262769	71.71%	9.271%
73	11.770	3334	3337	3340	rVB3	507	302	0.02%	0.002%
74	11.853	3360	3363	3365	rBV2	453	295	0.02%	0.002%
75	11.882	3370	3372	3378	rBV4	544	520	0.03%	0.004%
76	11.992	3404	3406	3410	rBV3	361	253	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035515.D
 Acq On : 02 May 2024 12:08
 Operator : SY/MD
 Sample : P2321-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	12.043	3418	3422	3424	rBV3	491	373	0.02%	0.003%
78	12.149	3453	3455	3461	rBV2	399	442	0.03%	0.003%
79	12.194	3462	3469	3477	rVB4	1997	2811	0.16%	0.021%
80	12.310	3501	3505	3507	rBV3	513	432	0.02%	0.003%
81	12.332	3510	3512	3517	rVB4	429	301	0.02%	0.002%
82	12.381	3522	3527	3529	rBV2	316	284	0.02%	0.002%
83	12.426	3539	3541	3545	rVB	523	396	0.02%	0.003%
84	12.590	3586	3592	3596	rBV4	1324	1569	0.09%	0.012%
85	12.898	3685	3688	3692	rVB3	316	264	0.01%	0.002%
86	12.927	3692	3697	3700	rBV2	515	509	0.03%	0.004%
87	12.972	3707	3711	3714	rBV2	571	398	0.02%	0.003%
88	13.140	3758	3763	3765	rBV2	396	332	0.02%	0.002%
89	13.210	3778	3785	3790	rBV6	1916	2787	0.16%	0.020%
90	13.303	3811	3814	3816	rBV2	471	286	0.02%	0.002%
91	13.387	3837	3840	3843	rBV3	403	270	0.02%	0.002%
92	13.451	3852	3860	3872	rBV3	2409	4450	0.25%	0.033%
93	13.693	3926	3935	3942	rBV6	1950	2598	0.15%	0.019%
94	13.834	3976	3979	3982	rBV2	512	364	0.02%	0.003%
95	13.914	4001	4004	4006	rBV4	474	293	0.02%	0.002%
96	13.956	4012	4017	4020	rBV4	627	753	0.04%	0.006%
97	14.152	4075	4078	4081	rVB2	586	349	0.02%	0.003%
98	14.606	4217	4219	4222	rBV2	476	236	0.01%	0.002%
99	15.178	4395	4397	4401	rBV2	797	666	0.04%	0.005%
100	15.197	4401	4403	4407	rVB3	759	461	0.03%	0.003%

Sum of corrected areas: 13620100




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035515.D
Acq On : 02 May 2024 12:08
Operator : SY/MD
Sample : P2321-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

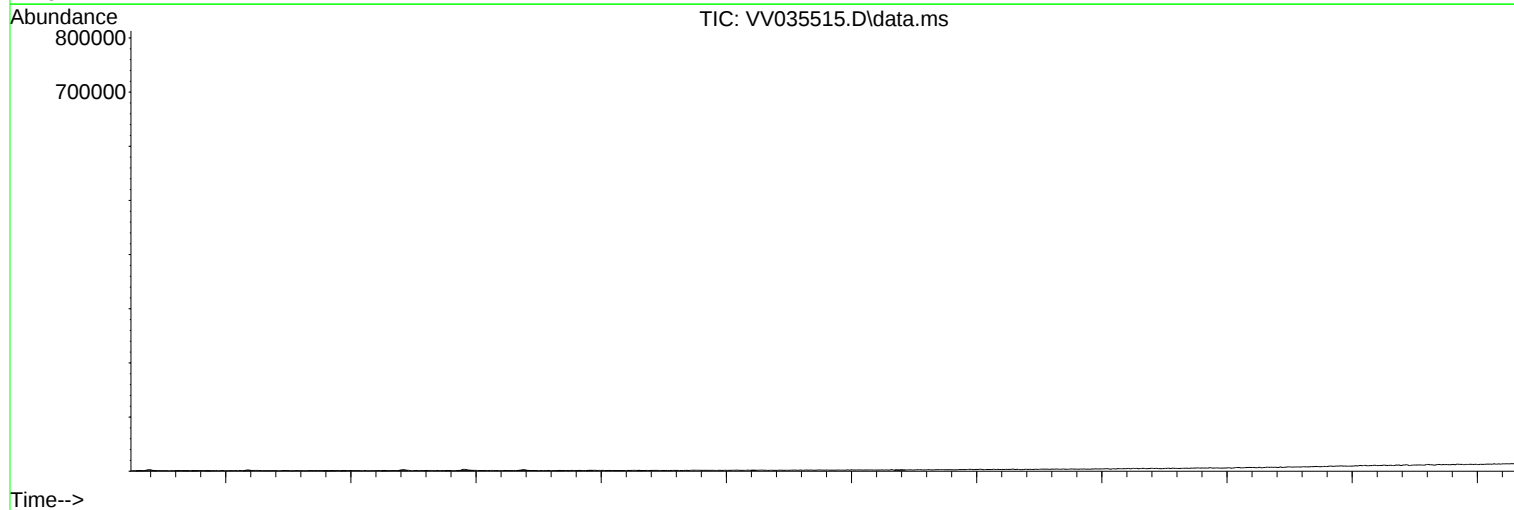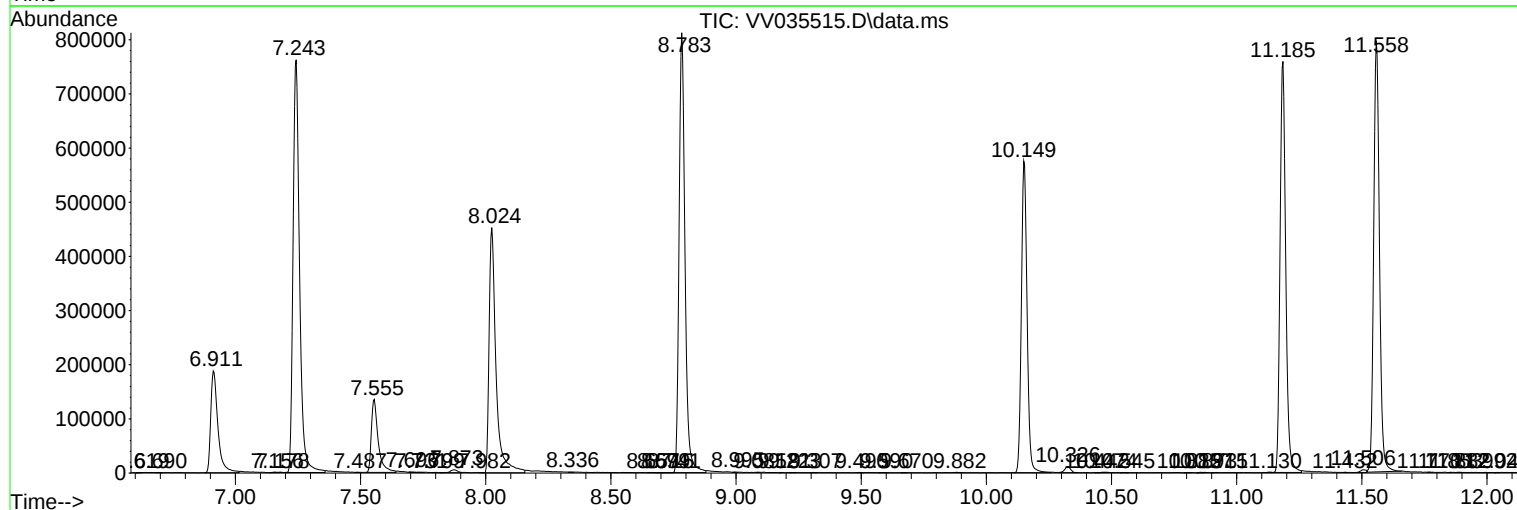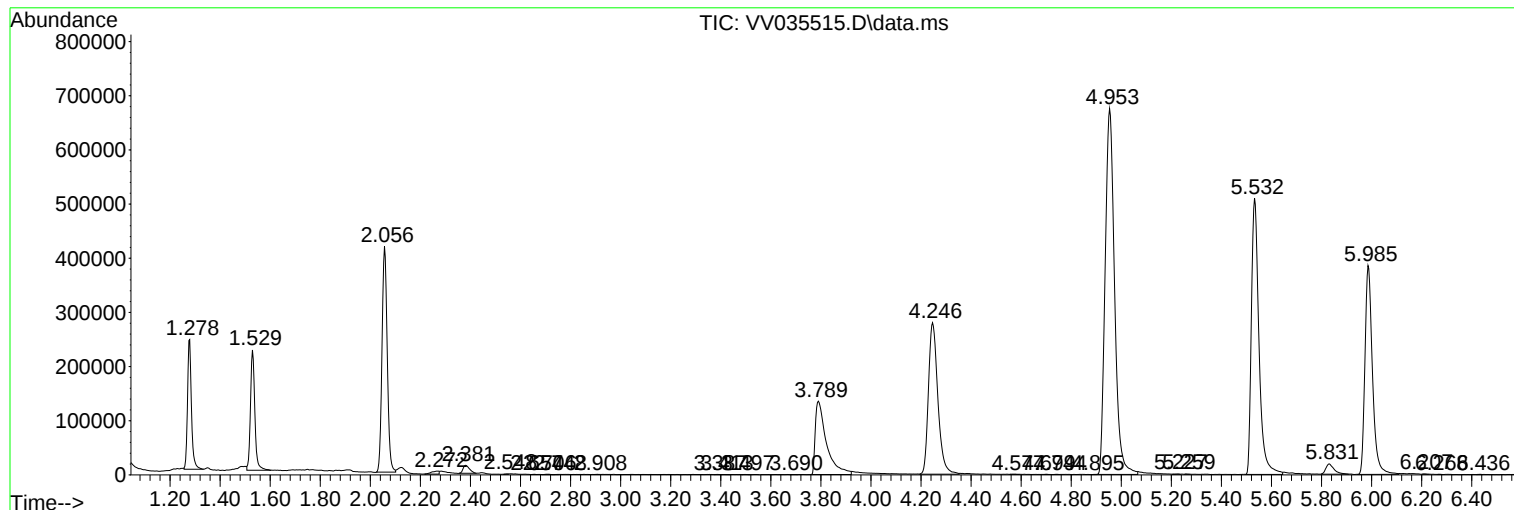

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035515.D
Acq On : 02 May 2024 12:08
Operator : SY/MD
Sample : P2321-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035515.D
Acq On : 02 May 2024 12:08
Operator : SY/MD
Sample : P2321-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------