

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035516.D
 Acq On : 02 May 2024 12:31
 Operator : SY/MD
 Sample : P2321-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	244749	267457	14.98%	1.933%
2	1.529	145	152	168	rVB	215875	251901	14.11%	1.820%
3	2.056	306	316	330	rBV	421511	605779	33.93%	4.377%
4	2.282	370	386	389	rBV3	6574	13313	0.75%	0.096%
5	2.381	411	417	432	rVB	15314	25958	1.45%	0.188%
6	2.558	463	472	482	rBV3	1539	3000	0.17%	0.022%
7	2.674	504	508	510	rBV2	326	232	0.01%	0.002%
8	2.706	511	518	522	rBV5	453	519	0.03%	0.004%
9	2.899	574	578	581	rVV2	452	343	0.02%	0.002%
10	2.986	599	605	610	rVB3	303	368	0.02%	0.003%
11	3.118	644	646	651	rVB	447	275	0.02%	0.002%
12	3.519	761	771	774	rBV	380	455	0.03%	0.003%
13	3.793	847	856	896	rBV	135036	426476	23.88%	3.082%
14	4.182	974	977	981	rBV3	489	519	0.03%	0.004%
15	4.246	981	997	1028	rVV	283180	737573	41.31%	5.330%
16	4.516	1078	1081	1084	rBV2	463	299	0.02%	0.002%
17	4.590	1102	1104	1109	rBV4	437	283	0.02%	0.002%
18	4.671	1124	1129	1131	rBV	336	316	0.02%	0.002%
19	4.716	1140	1143	1146	rBV3	458	266	0.01%	0.002%
20	4.886	1191	1196	1198	rBV2	305	275	0.02%	0.002%
21	4.953	1201	1217	1248	rBV2	685323	1785619	100.00%	12.903%
22	5.166	1280	1283	1285	rBV3	858	459	0.03%	0.003%
23	5.217	1297	1299	1303	rVB3	494	304	0.02%	0.002%
24	5.285	1318	1320	1324	rVB	529	352	0.02%	0.003%
25	5.307	1324	1327	1328	rBV3	468	260	0.01%	0.002%
26	5.339	1332	1337	1339	rBV3	330	257	0.01%	0.002%
27	5.416	1356	1361	1364	rBV5	339	295	0.02%	0.002%
28	5.449	1367	1371	1374	rVB4	527	441	0.02%	0.003%
29	5.532	1386	1397	1436	rBV	518339	1088606	60.97%	7.866%
30	5.828	1479	1489	1512	rBV3	19637	44559	2.50%	0.322%
31	5.986	1524	1538	1575	rBV	385139	810123	45.37%	5.854%
32	6.262	1621	1624	1628	rVB3	434	289	0.02%	0.002%
33	6.288	1628	1632	1637	rVB3	431	420	0.02%	0.003%
34	6.375	1655	1659	1661	rBV3	343	239	0.01%	0.002%
35	6.391	1661	1664	1667	rVB2	459	357	0.02%	0.003%
36	6.478	1687	1691	1695	rBV3	341	310	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035516.D
 Acq On : 02 May 2024 12:31
 Operator : SY/MD
 Sample : P2321-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.625	1734	1737	1739	rBV2	403	266	0.01%	0.002%
38	6.706	1759	1762	1764	rVB	499	271	0.02%	0.002%
39	6.738	1769	1772	1775	rBV2	319	217	0.01%	0.002%
40	6.912	1815	1826	1857	rBV	192499	372765	20.88%	2.694%
41	7.156	1898	1902	1903	rBV2	519	341	0.02%	0.002%
42	7.243	1914	1929	1956	rBV	776989	1391252	77.91%	10.053%
43	7.551	2016	2025	2059	rBV	136101	261196	14.63%	1.887%
44	7.783	2096	2097	2099	rBV	516	217	0.01%	0.002%
45	7.815	2104	2107	2111	rVV2	543	413	0.02%	0.003%
46	7.873	2117	2125	2135	rVB2	3516	6136	0.34%	0.044%
47	7.921	2135	2140	2142	rBV2	625	494	0.03%	0.004%
48	8.024	2163	2172	2212	rBV	463753	872745	48.88%	6.306%
49	8.481	2309	2314	2316	rBV2	425	379	0.02%	0.003%
50	8.500	2316	2320	2324	rVB2	420	363	0.02%	0.003%
51	8.542	2330	2333	2336	rBV4	364	231	0.01%	0.002%
52	8.744	2391	2396	2397	rBV	355	268	0.02%	0.002%
53	8.783	2397	2408	2439	rBV	834885	1366862	76.55%	9.877%
54	9.024	2480	2483	2487	rBV5	495	474	0.03%	0.003%
55	9.108	2505	2509	2513	rBV3	457	448	0.03%	0.003%
56	9.178	2527	2531	2533	rBV2	356	295	0.02%	0.002%
57	9.333	2576	2579	2583	rBV2	430	362	0.02%	0.003%
58	9.445	2611	2614	2620	rBV2	393	294	0.02%	0.002%
59	9.487	2623	2627	2630	rBV3	503	457	0.03%	0.003%
60	9.738	2701	2705	2712	rBV3	331	391	0.02%	0.003%
61	9.783	2712	2719	2723	rBV2	195	284	0.02%	0.002%
62	9.876	2743	2748	2750	rBV	456	399	0.02%	0.003%
63	10.149	2822	2833	2859	rVV	576058	914854	51.23%	6.611%
64	10.326	2878	2888	2900	rBV2	6394	11123	0.62%	0.080%
65	10.423	2912	2918	2920	rBV3	428	401	0.02%	0.003%
66	10.455	2926	2928	2930	rBV2	511	368	0.02%	0.003%
67	10.542	2951	2955	2959	rBV3	365	339	0.02%	0.002%
68	10.870	3049	3057	3060	rBV3	538	698	0.04%	0.005%
69	10.940	3077	3079	3082	rBV	324	234	0.01%	0.002%
70	10.960	3082	3085	3092	rVB3	389	310	0.02%	0.002%
71	11.005	3096	3099	3104	rVB	406	251	0.01%	0.002%
72	11.046	3107	3112	3116	rBV2	253	297	0.02%	0.002%
73	11.082	3120	3123	3126	rBV	288	218	0.01%	0.002%
74	11.133	3134	3139	3143	rVB4	1053	1122	0.06%	0.008%
75	11.185	3143	3155	3185	rBV	778774	1229900	68.88%	8.887%
76	11.497	3242	3252	3260	rBV2	12869	26962	1.51%	0.195%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035516.D
 Acq On : 02 May 2024 12:31
 Operator : SY/MD
 Sample : P2321-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.558	3261	3271	3297	rVB	814845	1293976	72.47%	9.350%
78	11.792	3341	3344	3349	rBV3	495	398	0.02%	0.003%
79	11.844	3358	3360	3364	rVB3	768	564	0.03%	0.004%
80	11.895	3373	3376	3379	rVB2	470	382	0.02%	0.003%
81	11.911	3379	3381	3384	rBV2	431	305	0.02%	0.002%
82	11.940	3387	3390	3391	rBV2	447	264	0.01%	0.002%
83	11.976	3397	3401	3402	rBV2	366	260	0.01%	0.002%
84	12.024	3414	3416	3421	rVB3	289	232	0.01%	0.002%
85	12.062	3423	3428	3433	rBV4	416	502	0.03%	0.004%
86	12.191	3463	3468	3469	rBV	800	603	0.03%	0.004%
87	12.313	3503	3506	3510	rBV2	492	414	0.02%	0.003%
88	12.432	3540	3543	3547	rBV3	525	424	0.02%	0.003%
89	12.526	3571	3572	3577	rBV2	358	242	0.01%	0.002%
90	12.583	3587	3590	3593	rBV3	1074	982	0.05%	0.007%
91	12.625	3599	3603	3614	rVB6	897	1162	0.07%	0.008%
92	12.853	3671	3674	3676	rBV2	497	289	0.02%	0.002%
93	13.204	3778	3783	3784	rBV4	1363	986	0.06%	0.007%
94	13.262	3799	3801	3806	rVB2	404	295	0.02%	0.002%
95	13.342	3824	3826	3831	rVB2	416	270	0.02%	0.002%
96	13.378	3831	3837	3841	rVB3	561	545	0.03%	0.004%
97	13.448	3853	3859	3860	rBV4	1819	1216	0.07%	0.009%
98	13.683	3928	3932	3933	rBV3	1089	807	0.05%	0.006%
99	14.133	4069	4072	4074	rBV2	565	360	0.02%	0.003%
100	14.506	4185	4188	4190	rBV2	621	369	0.02%	0.003%

Sum of corrected areas: 13839241




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035516.D
Acq On : 02 May 2024 12:31
Operator : SY/MD
Sample : P2321-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

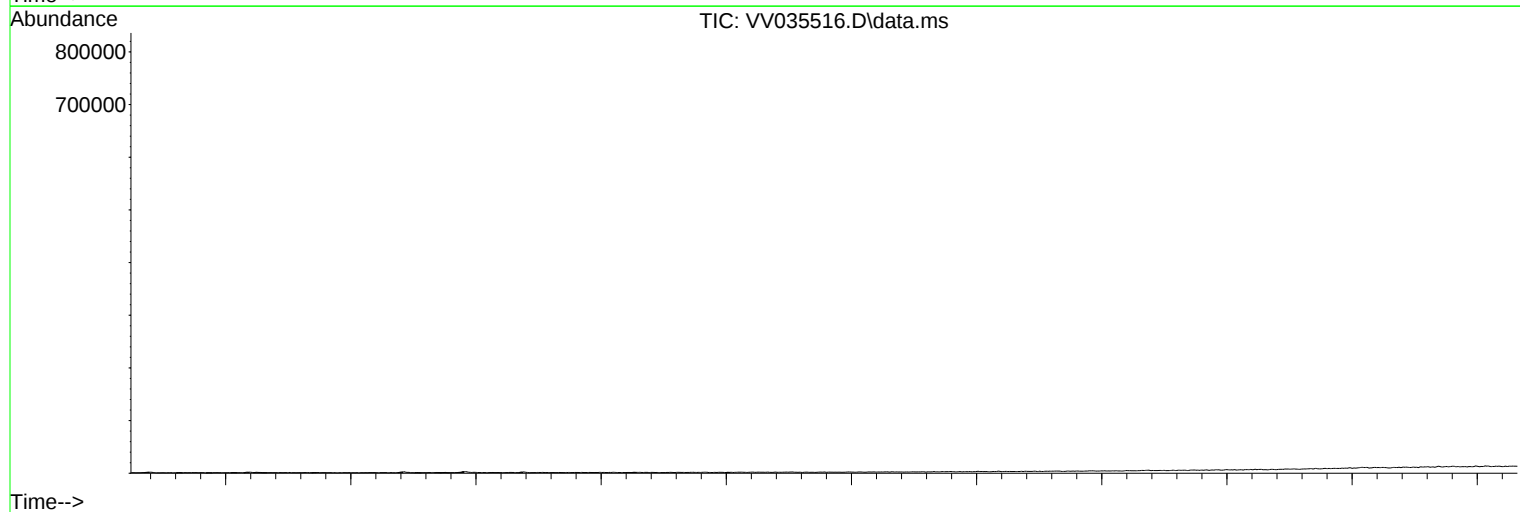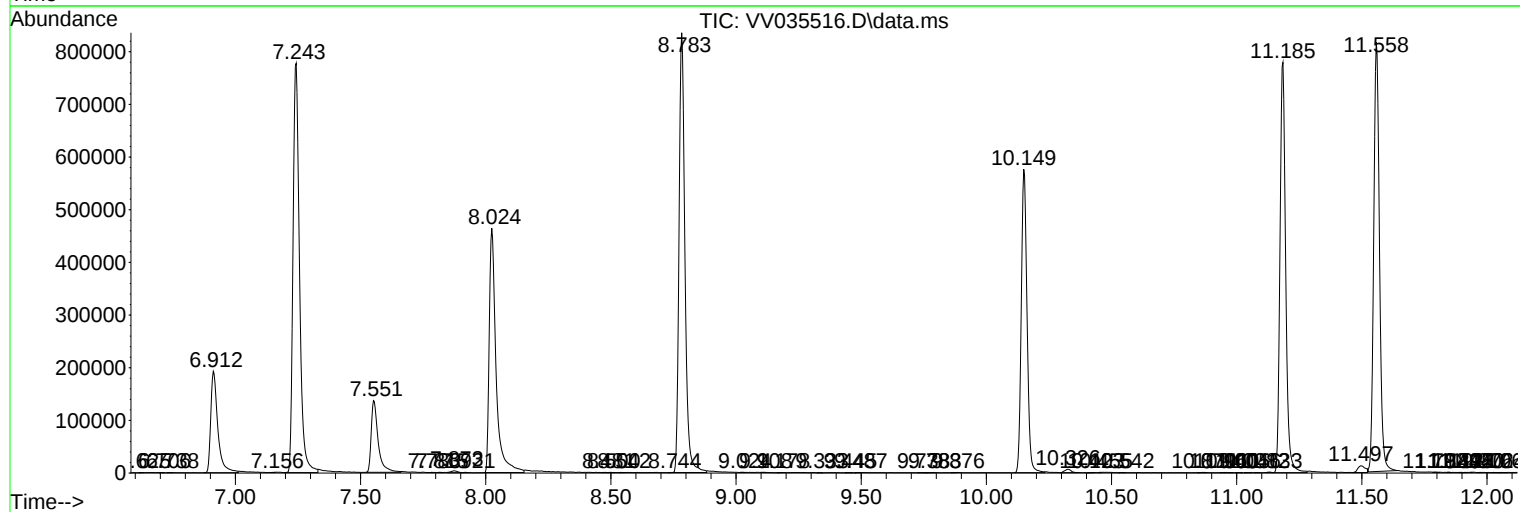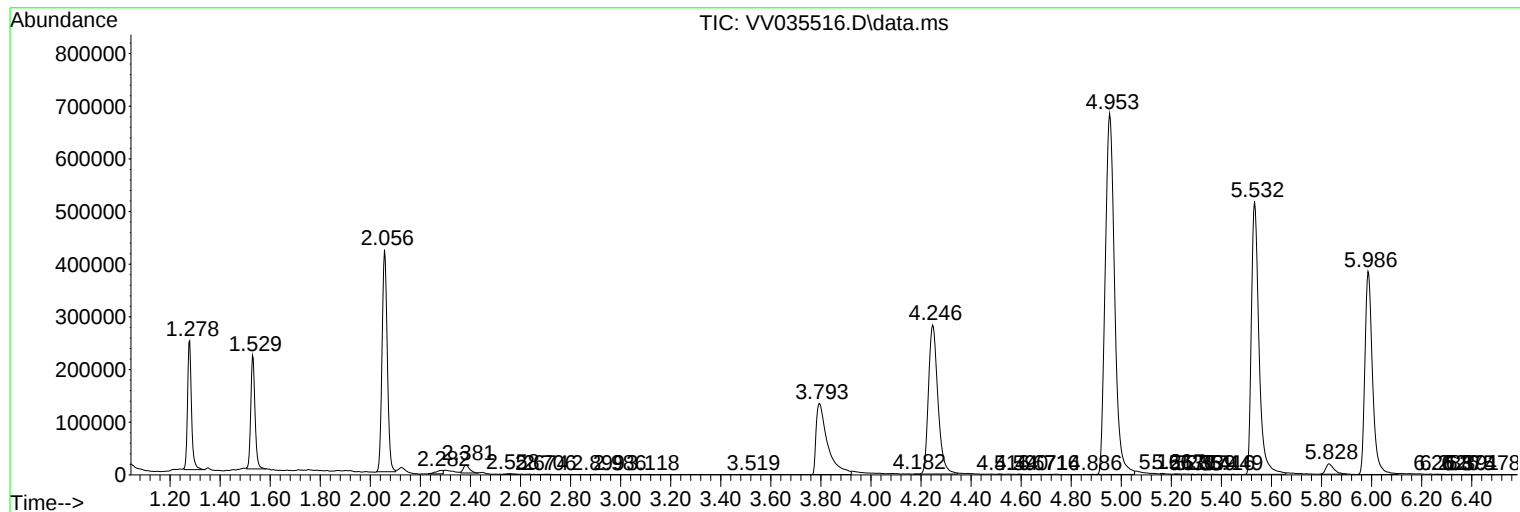

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035516.D
Acq On : 02 May 2024 12:31
Operator : SY/MD
Sample : P2321-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035516.D
Acq On : 02 May 2024 12:31
Operator : SY/MD
Sample : P2321-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------