

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035517.D
 Acq On : 02 May 2024 12:54
 Operator : SY/MD
 Sample : P2321-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	95	rVB	201077	224700	14.08%	1.867%
2	1.532	146	153	172	rVB	189134	223007	13.97%	1.853%
3	2.057	307	316	332	rVB	346638	497429	31.17%	4.134%
4	2.449	431	438	448	rVB4	2704	4207	0.26%	0.035%
5	2.629	492	494	495	rBV2	262	87	0.01%	0.001%
6	2.696	513	515	520	rVB2	313	232	0.01%	0.002%
7	2.719	520	522	526	rBV2	197	134	0.01%	0.001%
8	2.819	548	553	558	rBV2	336	407	0.03%	0.003%
9	2.934	587	589	590	rBV	133	35	0.00%	0.000%
10	2.966	595	599	602	rVV2	278	232	0.01%	0.002%
11	3.044	620	623	625	rBV3	285	169	0.01%	0.001%
12	3.073	629	632	634	rVB2	141	89	0.01%	0.001%
13	3.304	701	704	707	rBV2	127	86	0.01%	0.001%
14	3.410	734	737	738	rBV	198	89	0.01%	0.001%
15	3.442	745	747	751	rBV2	184	90	0.01%	0.001%
16	3.510	765	768	770	rBV	85	38	0.00%	0.000%
17	3.523	770	772	778	rVV2	168	145	0.01%	0.001%
18	3.545	778	779	780	rVV2	126	25	0.00%	0.000%
19	3.558	780	783	785	rVB2	172	87	0.01%	0.001%
20	3.577	786	789	792	rVB	340	196	0.01%	0.002%
21	3.613	796	800	803	rBV	148	154	0.01%	0.001%
22	3.632	803	806	809	rBV3	291	181	0.01%	0.002%
23	3.754	841	844	848	rBV	190	154	0.01%	0.001%
24	3.793	848	856	903	rBV2	127761	412644	25.85%	3.429%
25	4.246	981	997	1033	rBV2	251166	653625	40.95%	5.432%
26	4.706	1135	1140	1144	rBV3	415	452	0.03%	0.004%
27	4.764	1155	1158	1162	rVB	302	216	0.01%	0.002%
28	4.790	1162	1166	1170	rBV2	403	392	0.02%	0.003%
29	4.954	1202	1217	1253	rBV2	599518	1596009	100.00%	13.264%
30	5.371	1345	1347	1349	rBV	302	136	0.01%	0.001%
31	5.532	1386	1397	1440	rBV	427431	908846	56.94%	7.553%
32	5.834	1483	1491	1506	rBV5	6255	13155	0.82%	0.109%
33	5.986	1524	1538	1571	rBV	348720	734149	46.00%	6.101%
34	6.259	1619	1623	1626	rBV3	444	378	0.02%	0.003%
35	6.336	1644	1647	1650	rVB3	478	278	0.02%	0.002%
36	6.368	1652	1657	1659	rBV2	275	278	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035517.D
 Acq On : 02 May 2024 12:54
 Operator : SY/MD
 Sample : P2321-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.426	1672	1675	1678	rVB2	248	179	0.01%	0.001%
38	6.452	1678	1683	1685	rBV2	351	224	0.01%	0.002%
39	6.465	1685	1687	1689	rBV	324	121	0.01%	0.001%
40	6.551	1712	1714	1715	rVB	147	36	0.00%	0.000%
41	6.564	1715	1718	1719	rBV	102	51	0.00%	0.000%
42	6.574	1719	1721	1727	rVB2	202	95	0.01%	0.001%
43	6.603	1727	1730	1731	rBV	173	97	0.01%	0.001%
44	6.699	1755	1760	1761	rBV2	254	234	0.01%	0.002%
45	6.761	1772	1779	1781	rBV3	315	354	0.02%	0.003%
46	6.812	1790	1795	1798	rBV2	153	148	0.01%	0.001%
47	6.834	1801	1802	1806	rVV2	173	77	0.00%	0.001%
48	6.912	1815	1826	1851	rBV	168557	327570	20.52%	2.722%
49	7.243	1918	1929	1956	rBV	658031	1167656	73.16%	9.704%
50	7.555	2016	2026	2056	rBV	122295	236329	14.81%	1.964%
51	7.966	2151	2154	2155	rBV	334	162	0.01%	0.001%
52	7.982	2157	2159	2163	rVB3	379	212	0.01%	0.002%
53	8.024	2163	2172	2210	rBV	452139	853572	53.48%	7.094%
54	8.545	2332	2334	2337	rBV2	230	113	0.01%	0.001%
55	8.577	2341	2344	2345	rBV	381	160	0.01%	0.001%
56	8.619	2353	2357	2358	rBV	223	160	0.01%	0.001%
57	8.741	2392	2395	2397	rBV	254	154	0.01%	0.001%
58	8.783	2397	2408	2445	rBV	697768	1156864	72.48%	9.614%
59	9.146	2519	2521	2522	rBV	264	116	0.01%	0.001%
60	9.194	2532	2536	2538	rBV2	346	277	0.02%	0.002%
61	9.265	2555	2558	2560	rBV	269	184	0.01%	0.002%
62	9.323	2574	2576	2578	rBV	258	138	0.01%	0.001%
63	9.358	2586	2587	2591	rBV	215	96	0.01%	0.001%
64	9.410	2600	2603	2607	rBV2	413	265	0.02%	0.002%
65	9.461	2617	2619	2623	rBV2	285	180	0.01%	0.001%
66	9.506	2628	2633	2637	rBV2	558	427	0.03%	0.004%
67	9.577	2652	2655	2656	rBV	62	33	0.00%	0.000%
68	9.593	2656	2660	2665	rVV3	300	306	0.02%	0.003%
69	9.712	2694	2697	2698	rBV	188	99	0.01%	0.001%
70	9.992	2781	2784	2787	rBV2	290	188	0.01%	0.002%
71	10.149	2821	2833	2864	rBV	584901	920768	57.69%	7.652%
72	10.387	2904	2907	2911	rBV3	404	372	0.02%	0.003%
73	10.474	2932	2934	2935	rBV	318	124	0.01%	0.001%
74	10.542	2953	2955	2957	rBV	165	48	0.00%	0.000%
75	10.641	2983	2986	2992	rBV2	412	262	0.02%	0.002%
76	10.792	3032	3033	3035	rBV2	225	91	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035517.D
Acq On : 02 May 2024 12:54
Operator : SY/MD
Sample : P2321-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Title : VOC Analysis

77	10.841	3046	3048	3049	rVB2	198	55	0.00%	0.000%
78	10.934	3074	3077	3081	rBV	282	187	0.01%	0.002%
79	11.079	3120	3122	3123	rBV	177	55	0.00%	0.000%
80	11.185	3143	3155	3181	rBV	626348	1002507	62.81%	8.331%
81	11.558	3259	3271	3297	rBV	693092	1089183	68.24%	9.052%

Sum of corrected areas: 12033060




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035517.D
Acq On : 02 May 2024 12:54
Operator : SY/MD
Sample : P2321-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

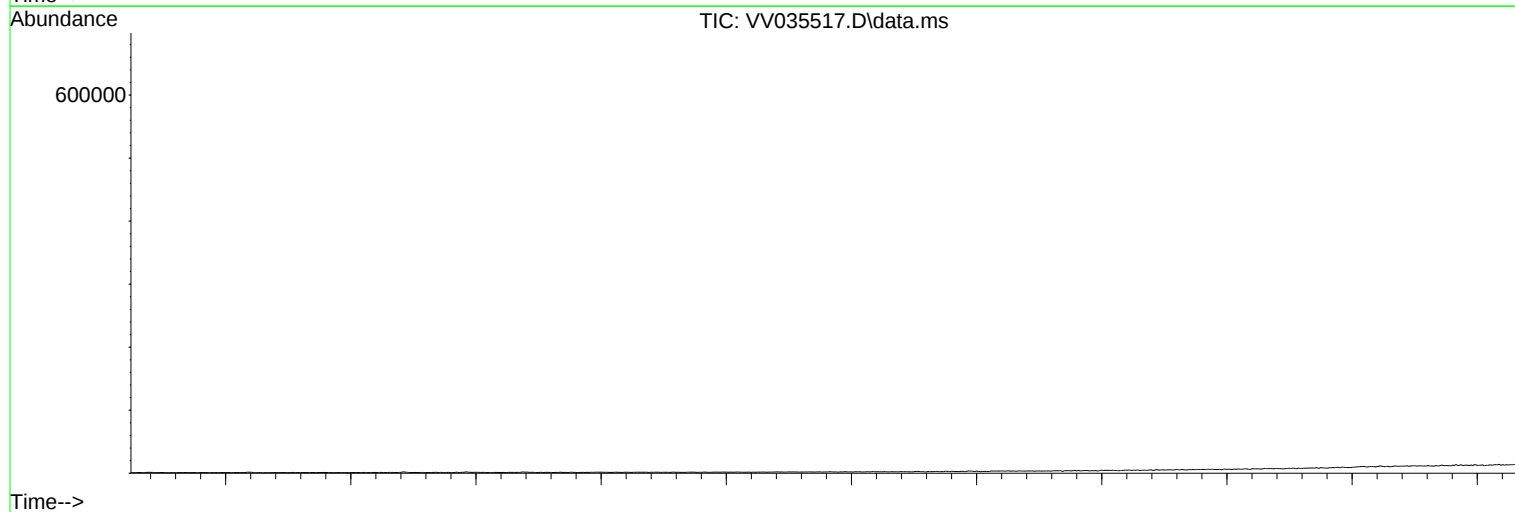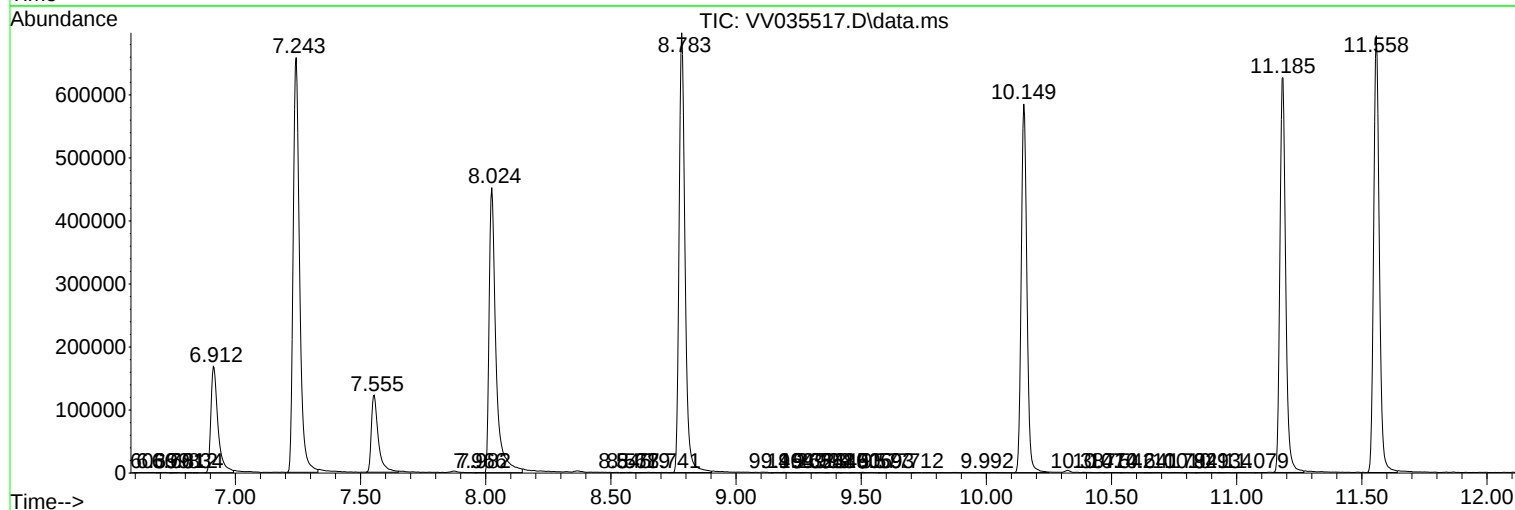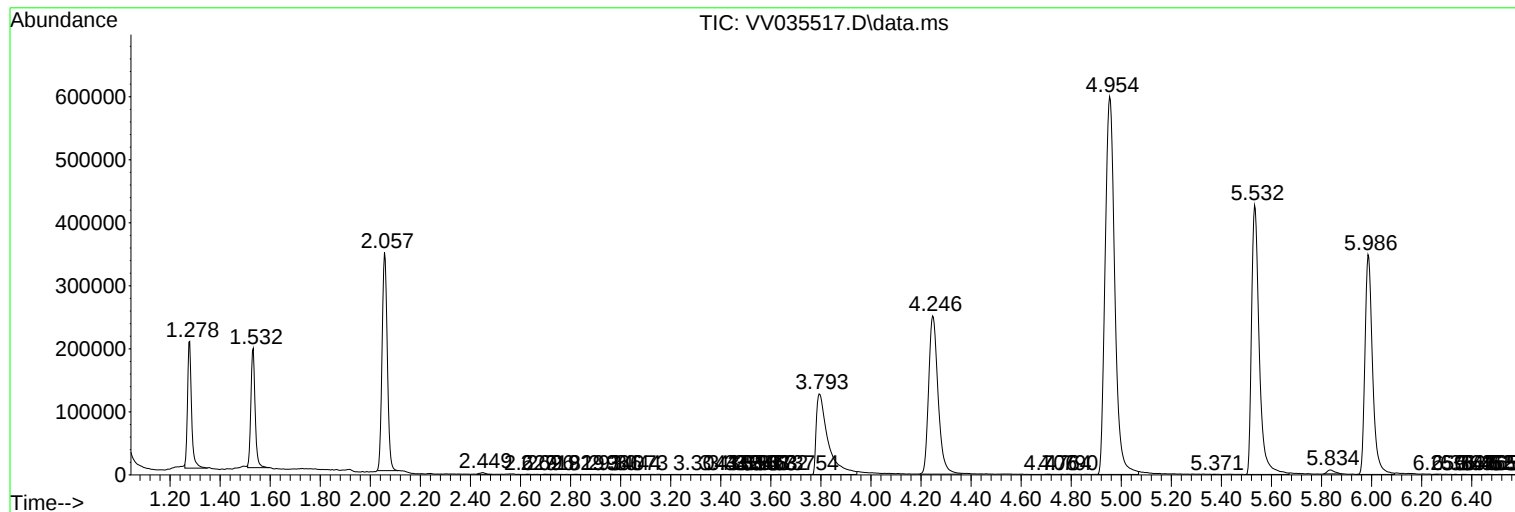

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035517.D
Acq On : 02 May 2024 12:54
Operator : SY/MD
Sample : P2321-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035517.D
Acq On : 02 May 2024 12:54
Operator : SY/MD
Sample : P2321-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------