

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035518.D
 Acq On : 02 May 2024 13:16
 Operator : SY/MD
 Sample : P2349-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	91	rVB	239338	263068	14.81%	1.923%
2	1.529	145	152	164	rVB	218480	249452	14.04%	1.824%
3	2.056	306	316	330	rBV	425380	613205	34.53%	4.483%
4	2.233	367	371	376	rBV6	809	857	0.05%	0.006%
5	2.339	402	404	407	rVB2	440	271	0.02%	0.002%
6	2.365	407	412	413	rBV3	556	462	0.03%	0.003%
7	2.445	432	437	439	rBV4	866	762	0.04%	0.006%
8	2.593	476	483	486	rBV2	898	1119	0.06%	0.008%
9	2.860	559	566	570	rBV2	374	425	0.02%	0.003%
10	2.886	570	574	576	rBV2	529	411	0.02%	0.003%
11	3.024	614	617	621	rVV3	425	300	0.02%	0.002%
12	3.088	632	637	641	rBV2	267	267	0.02%	0.002%
13	3.436	740	745	748	rBV2	245	297	0.02%	0.002%
14	3.455	748	751	759	rVB	262	307	0.02%	0.002%
15	3.590	789	793	796	rVV4	438	401	0.02%	0.003%
16	3.619	796	802	808	rVB3	587	706	0.04%	0.005%
17	3.789	847	855	889	rBV	131209	382330	21.53%	2.795%
18	4.249	980	998	1035	rBV2	292885	836332	47.09%	6.114%
19	4.638	1117	1119	1123	rVB3	314	265	0.01%	0.002%
20	4.731	1146	1148	1152	rVB	383	252	0.01%	0.002%
21	4.783	1157	1164	1167	rBV3	382	476	0.03%	0.003%
22	4.879	1192	1194	1200	rVB2	272	233	0.01%	0.002%
23	4.953	1200	1217	1256	rBV2	677608	1776109	100.00%	12.984%
24	5.249	1307	1309	1314	rVB2	406	245	0.01%	0.002%
25	5.313	1326	1329	1335	rVB3	570	578	0.03%	0.004%
26	5.349	1338	1340	1345	rVB3	373	299	0.02%	0.002%
27	5.391	1350	1353	1357	rVB2	401	233	0.01%	0.002%
28	5.439	1363	1368	1371	rVB4	506	468	0.03%	0.003%
29	5.532	1386	1397	1426	rBV	508223	1059218	59.64%	7.743%
30	5.831	1479	1490	1513	rBV	17009	38619	2.17%	0.282%
31	5.989	1526	1539	1569	rVV	384606	805397	45.35%	5.888%
32	6.368	1653	1657	1658	rBV	506	305	0.02%	0.002%
33	6.397	1661	1666	1670	rVB3	358	283	0.02%	0.002%
34	6.445	1670	1681	1698	rBV3	9343	20175	1.14%	0.147%
35	6.629	1736	1738	1743	rVV2	529	421	0.02%	0.003%
36	6.760	1776	1779	1783	rVB2	532	299	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035518.D
 Acq On : 02 May 2024 13:16
 Operator : SY/MD
 Sample : P2349-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.911	1816	1826	1856	rBV	186927	368127	20.73%	2.691%
38	7.149	1894	1900	1901	rBV2	581	557	0.03%	0.004%
39	7.243	1915	1929	1950	rBV	770572	1369398	77.10%	10.011%
40	7.555	2016	2026	2052	rBV	136234	257437	14.49%	1.882%
41	7.754	2084	2088	2091	rVB5	423	338	0.02%	0.002%
42	7.773	2091	2094	2098	rBV3	392	290	0.02%	0.002%
43	7.844	2114	2116	2118	rBV2	502	247	0.01%	0.002%
44	7.876	2118	2126	2134	rVB3	2283	4064	0.23%	0.030%
45	8.024	2163	2172	2215	rBV	453161	867156	48.82%	6.339%
46	8.445	2301	2303	2308	rVB4	586	388	0.02%	0.003%
47	8.484	2310	2315	2316	rBV2	335	293	0.02%	0.002%
48	8.561	2336	2339	2342	rBV3	362	300	0.02%	0.002%
49	8.606	2349	2353	2356	rBV3	474	359	0.02%	0.003%
50	8.783	2397	2408	2434	rBV	808912	1338419	75.36%	9.784%
51	9.021	2480	2482	2489	rVB4	566	593	0.03%	0.004%
52	9.062	2490	2495	2499	rBV5	439	486	0.03%	0.004%
53	9.085	2499	2502	2504	rBV2	673	460	0.03%	0.003%
54	9.162	2523	2526	2531	rVB3	466	363	0.02%	0.003%
55	9.194	2534	2536	2540	rVB	434	255	0.01%	0.002%
56	9.223	2540	2545	2549	rBV3	476	441	0.02%	0.003%
57	9.278	2558	2562	2565	rVB2	353	269	0.02%	0.002%
58	9.368	2586	2590	2595	rBV3	368	296	0.02%	0.002%
59	9.500	2627	2631	2638	rVB5	379	468	0.03%	0.003%
60	9.587	2654	2658	2659	rBV	427	252	0.01%	0.002%
61	9.876	2742	2748	2750	rBV3	426	379	0.02%	0.003%
62	9.947	2765	2770	2773	rBV3	235	287	0.02%	0.002%
63	9.972	2776	2778	2781	rVV2	339	234	0.01%	0.002%
64	10.149	2818	2833	2866	rBV	581419	921074	51.86%	6.733%
65	10.323	2879	2887	2898	rVB4	4396	7407	0.42%	0.054%
66	10.406	2907	2913	2915	rBV3	334	375	0.02%	0.003%
67	10.587	2965	2969	2972	rBV2	356	233	0.01%	0.002%
68	10.744	3016	3018	3022	rVB3	379	271	0.02%	0.002%
69	10.770	3022	3026	3032	rBV3	283	332	0.02%	0.002%
70	10.863	3051	3055	3059	rBV2	415	353	0.02%	0.003%
71	10.940	3076	3079	3081	rBV2	444	321	0.02%	0.002%
72	10.972	3085	3089	3091	rBV	405	247	0.01%	0.002%
73	11.062	3112	3117	3122	rVB2	402	420	0.02%	0.003%
74	11.088	3122	3125	3130	rBV	399	306	0.02%	0.002%
75	11.120	3133	3135	3137	rBV2	433	254	0.01%	0.002%
76	11.185	3144	3155	3180	rBV	764657	1200264	67.58%	8.774%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
 Data File : VV035518.D
 Acq On : 02 May 2024 13:16
 Operator : SY/MD
 Sample : P2349-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.400	3216	3222	3226	rBV4	653	814	0.05%	0.006%
78	11.468	3239	3243	3248	rVB5	484	423	0.02%	0.003%
79	11.558	3257	3271	3302	rBV	803294	1268131	71.40%	9.270%
80	11.783	3339	3341	3344	rVV3	603	295	0.02%	0.002%
81	11.889	3370	3374	3376	rBV2	414	321	0.02%	0.002%
82	12.156	3452	3457	3459	rBV	448	326	0.02%	0.002%
83	12.185	3463	3466	3469	rBV3	521	454	0.03%	0.003%
84	12.599	3588	3595	3599	rBV	706	714	0.04%	0.005%
85	12.699	3624	3626	3633	rVB3	534	434	0.02%	0.003%
86	12.738	3633	3638	3640	rBV2	390	377	0.02%	0.003%
87	12.979	3709	3713	3716	rBV2	365	300	0.02%	0.002%
88	13.056	3732	3737	3742	rVB3	380	384	0.02%	0.003%
89	13.210	3778	3785	3790	rBV9	1565	2227	0.13%	0.016%
90	13.297	3808	3812	3813	rBV2	359	249	0.01%	0.002%
91	13.400	3841	3844	3847	rVB2	467	278	0.02%	0.002%
92	13.451	3855	3860	3863	rBV3	747	899	0.05%	0.007%
93	13.686	3930	3933	3941	rVB4	1074	1172	0.07%	0.009%
94	13.792	3962	3966	3971	rBV4	581	596	0.03%	0.004%
95	13.873	3989	3991	3994	rBV3	429	267	0.02%	0.002%
96	14.078	4052	4055	4057	rBV3	452	281	0.02%	0.002%
97	14.358	4139	4142	4145	rBV2	513	326	0.02%	0.002%
98	14.406	4154	4157	4160	rVB2	540	308	0.02%	0.002%
99	14.789	4274	4276	4277	rBV2	640	246	0.01%	0.002%
100	14.831	4286	4289	4294	rBV4	792	627	0.04%	0.005%

Sum of corrected areas: 13679309




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035518.D
Acq On : 02 May 2024 13:16
Operator : SY/MD
Sample : P2349-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

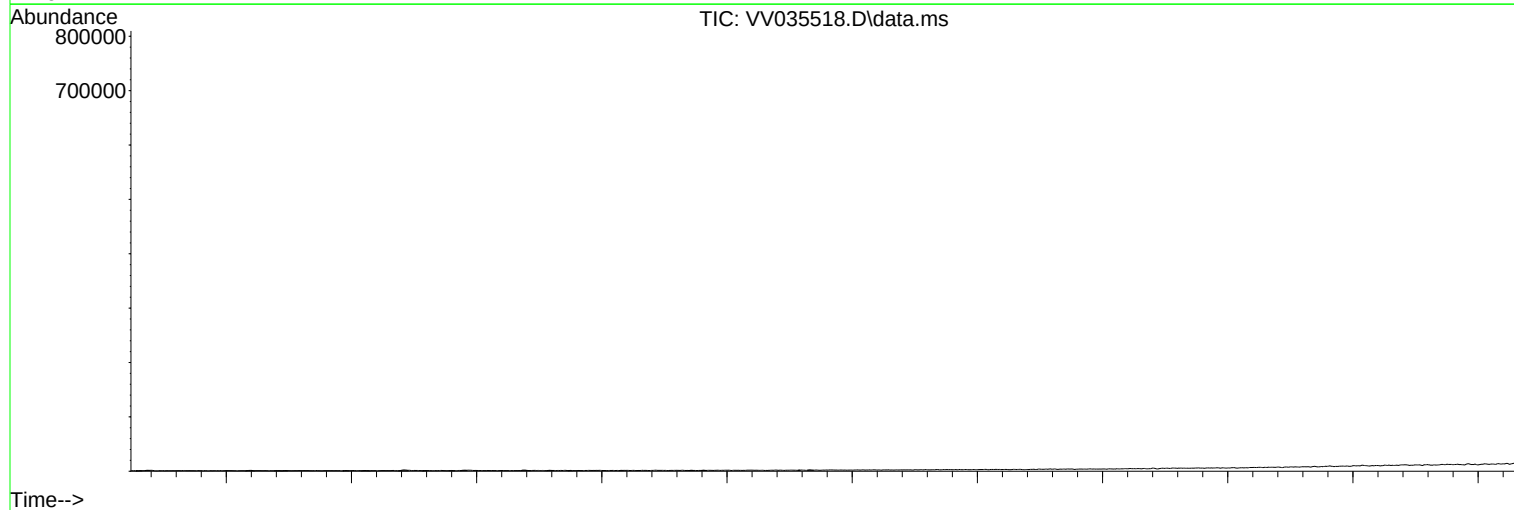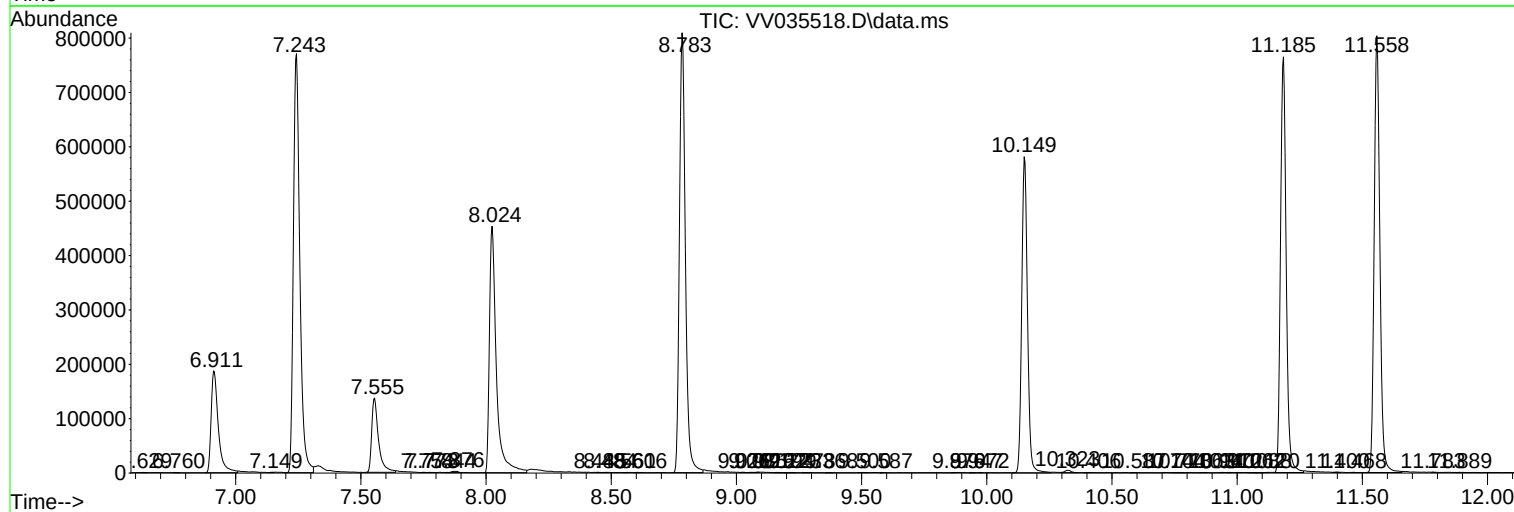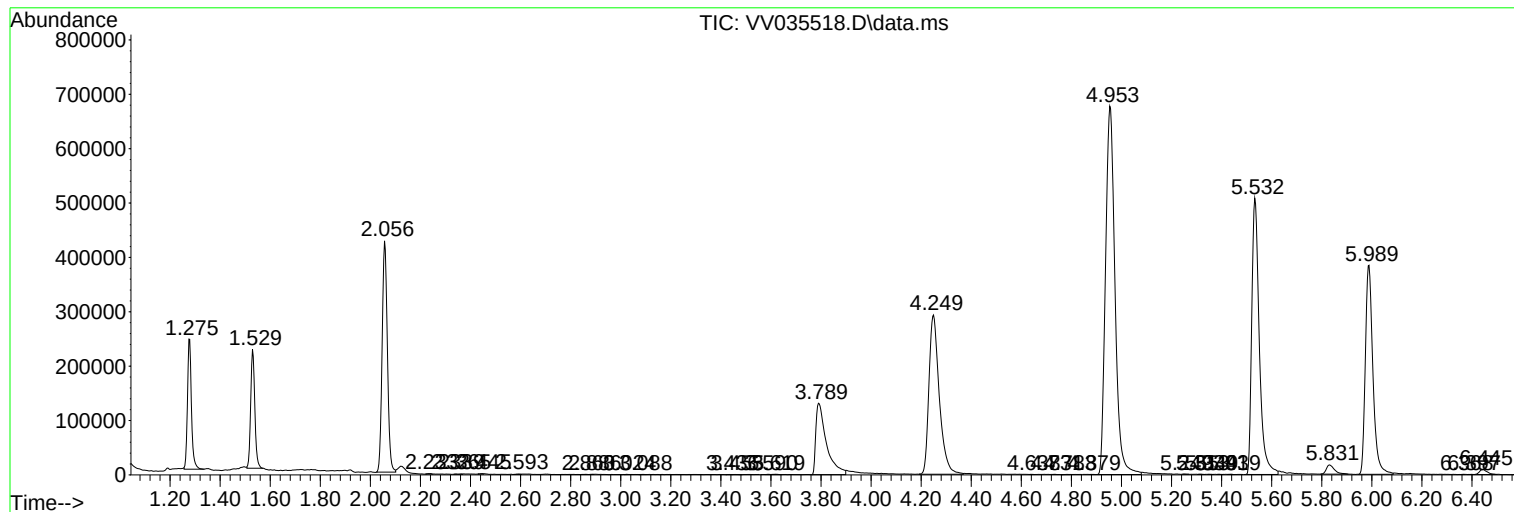

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035518.D
Acq On : 02 May 2024 13:16
Operator : SY/MD
Sample : P2349-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035518.D
Acq On : 02 May 2024 13:16
Operator : SY/MD
Sample : P2349-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------