
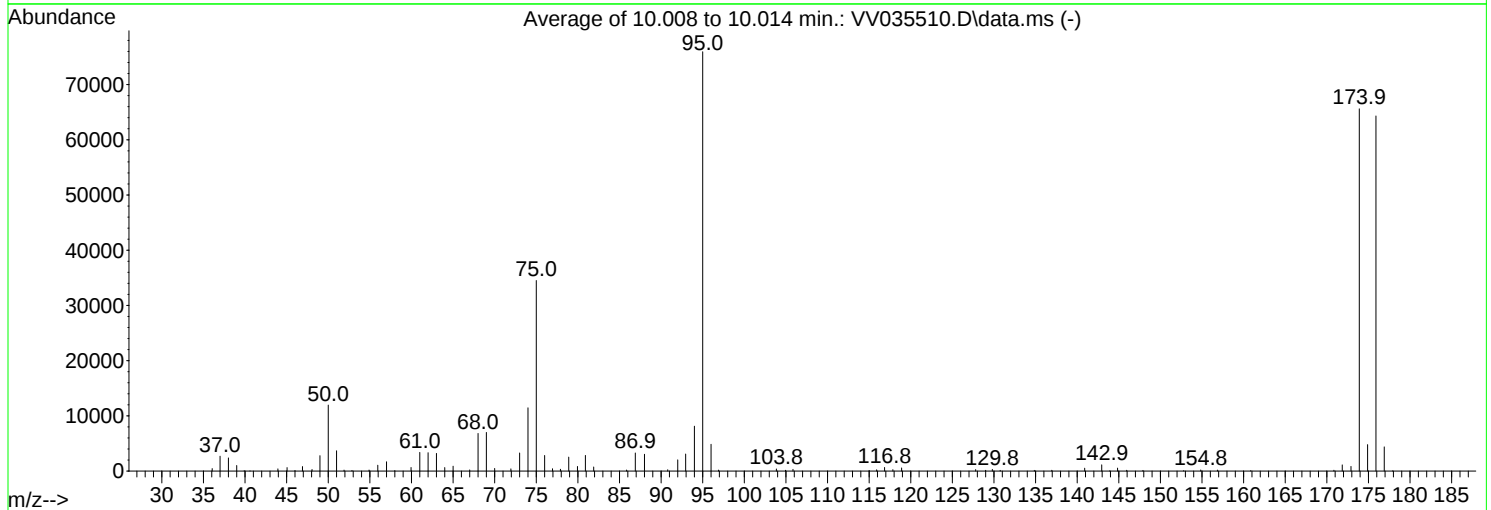


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050224\
Data File : VV035510.D
Acq On : 02 May 2024 09:41
Operator : SY/MD
Sample : BFB295
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB295

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Title : VOC Analysis
Last Update : Fri May 03 05:13:05 2024

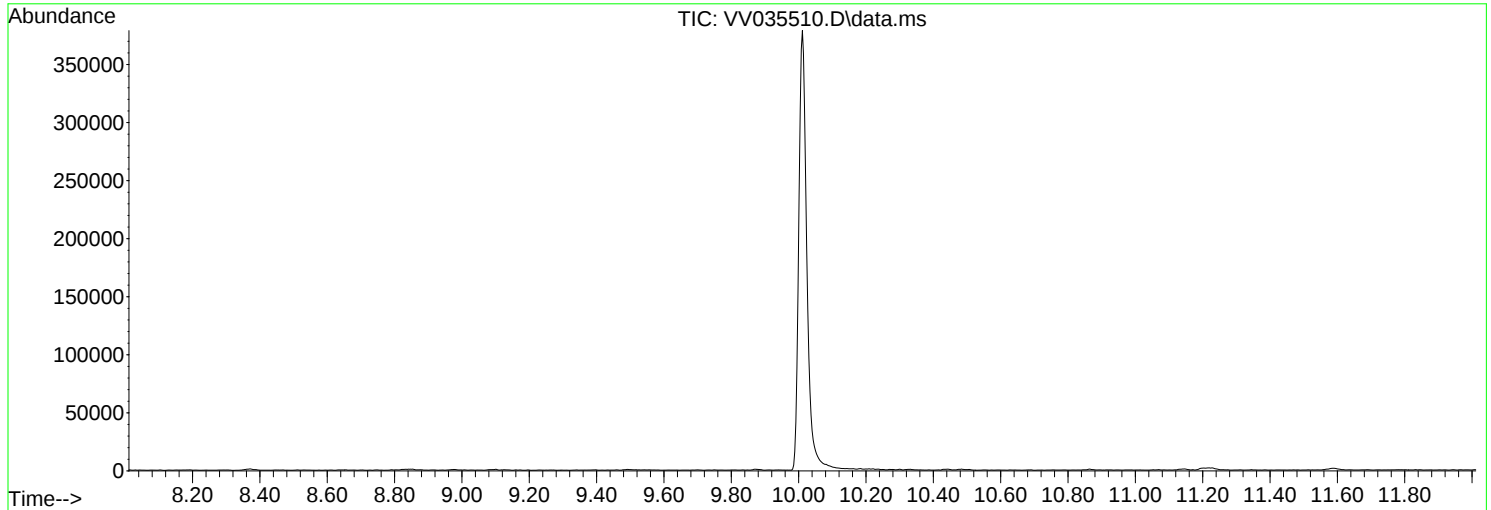

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	11954	PASS
75	95	30	80	45.4	34517	PASS
95	95	100	100	100.0	75952	PASS
96	95	5	9	6.4	4854	PASS
173	174	0.00	2	1.3	842	PASS
174	95	50	120	86.4	65619	PASS
175	174	5	9	7.3	4789	PASS
176	174	95	105	98.0	64317	PASS
177	176	5	10	6.8	4384	PASS

m/z	Abundance
39.80	189.0
43.90	468.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

m/z	Abundance
36.00	413.0
37.00	2624.0
38.00	2526.0
39.00	1015.0
40.00	294.0
44.00	792.0
45.00	713.0
46.00	173.0
46.90	790.0
48.00	292.0
49.00	2909.0
50.00	12111.0
51.00	3775.0
51.90	205.0
52.90	123.0
54.90	218.0
56.00	1120.0
57.00	1592.0
58.00	131.0
59.90	716.0
61.00	3412.0
62.00	3469.0
63.00	3189.0
64.00	604.0
65.00	829.0
67.00	193.0
68.00	6931.0
69.00	6976.0
70.00	491.0
71.90	374.0
73.00	3243.0
74.00	11466.0
75.00	33912.0
76.00	2883.0
76.90	432.0
77.90	288.0
78.90	2404.0
79.90	821.0
80.90	2817.0
81.90	800.0
85.90	182.0
86.90	3309.0
88.00	3076.0
90.70	215.0
92.00	2177.0
93.00	3077.0
94.00	7993.0
95.00	75416.0
96.00	4777.0
96.90	212.0
103.80	396.0
105.00	130.0
105.90	287.0
115.10	106.0
115.80	263.0
116.90	603.0
117.80	300.0
118.90	564.0
127.80	286.0
129.00	120.0
129.80	319.0
130.70	124.0
134.90	107.0
137.00	141.0
140.90	455.0
143.00	1137.0
144.90	521.0
145.90	151.0
147.90	117.0
154.80	205.0
156.80	190.0
160.90	108.0
170.90	163.0
171.90	1049.0
172.90	850.0
173.90	63760.0
174.90	4737.0
175.90	62784.0
176.90	4427.0
177.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

m/z	Abundance
36.10	471.0
37.00	2797.0
38.00	2445.0
39.00	1033.0
40.00	259.0
44.00	892.0
45.00	648.0
46.00	157.0
46.90	838.0
48.10	296.0
49.00	2905.0
50.00	12311.0
51.00	3834.0
51.90	189.0
52.80	120.0
54.90	188.0
56.00	1095.0
57.00	1756.0
58.00	115.0
59.90	679.0
61.00	3518.0
62.00	3402.0
63.00	3349.0
64.00	655.0
65.00	935.0
67.00	211.0
68.00	7014.0
69.00	7223.0
70.00	494.0
71.90	401.0
73.00	3462.0
74.00	11822.0
75.00	35456.0
76.00	2888.0
76.90	417.0
77.90	338.0
78.90	2594.0
80.00	847.0
80.90	2937.0
81.90	749.0
85.80	199.0
86.90	3396.0
88.00	3135.0
90.80	249.0
92.00	2039.0
92.90	3155.0
94.00	8409.0
95.00	78544.0
96.00	4995.0
96.90	180.0
103.80	404.0
105.00	162.0
105.80	337.0
115.00	118.0
115.90	241.0
116.90	684.0
117.80	259.0
118.90	585.0
127.80	275.0
129.00	148.0
129.80	321.0
130.80	134.0
134.80	134.0
136.90	158.0
140.90	546.0
142.90	1141.0
143.90	101.0
144.90	568.0
145.90	159.0
147.90	130.0
152.80	122.0
154.80	200.0
156.80	186.0
160.80	128.0
170.90	140.0
171.90	1143.0
172.90	860.0
173.90	67616.0
174.90	4896.0
175.90	66784.0
176.90	4485.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

m/z	Abundance
36.10	493.0
37.00	2673.0
38.00	2187.0
39.00	979.0
40.00	201.0
40.60	101.0
44.00	912.0
45.10	543.0
46.90	826.0
48.00	280.0
49.00	2571.0
50.00	11439.0
51.00	3438.0
51.90	152.0
52.80	109.0
54.90	179.0
55.90	985.0
57.00	1705.0
60.00	570.0
61.00	3219.0
62.00	3124.0
63.00	3054.0
64.00	655.0
65.00	905.0
67.00	224.0
68.00	6501.0
69.00	6806.0
70.00	443.0
72.00	416.0
73.00	3130.0
74.00	11081.0
75.00	34184.0
76.00	2715.0
77.00	432.0
77.90	378.0
78.90	2601.0
80.00	833.0
80.90	2750.0
81.90	661.0
85.80	188.0
86.90	3140.0
88.00	2917.0
90.90	278.0
92.00	1883.0
93.00	3039.0
94.00	8000.0
95.00	73896.0
96.00	4790.0
96.90	149.0
103.90	344.0
104.90	151.0
105.80	324.0
114.90	101.0
116.00	203.0
116.80	678.0
117.90	223.0
118.90	554.0
127.80	245.0
129.00	151.0
129.80	278.0
130.70	144.0
134.80	149.0
136.90	154.0
140.90	558.0
142.90	1105.0
144.80	537.0
146.00	152.0
147.90	119.0
152.80	127.0
154.90	184.0
156.90	170.0
170.80	166.0
171.80	1182.0
172.90	815.0
173.90	65480.0
174.90	4733.0
175.90	63384.0
176.90	4239.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295