

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035527.D
 Acq On : 03 May 2024 10:54
 Operator : SY/MD
 Sample : P2349-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 03 23:18:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 03 23:16:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	417289	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	426580	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	191899	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	143926	44.732	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	89.460%		
7) Chloroethane-d5	1.529	69	128346	54.130	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	108.260%		
11) 1,1-Dichloroethene-d2	2.056	65	63887	46.256	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.520%		
21) 2-Butanone-d5	3.786	46	220284	101.443	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.440%		
24) Chloroform-d	4.246	84	302546	51.263	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.520%		
26) 1,2-Dichloroethane-d4	4.937	65	187679	53.999	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	108.000%		
32) Benzene-d6	4.957	84	577831	48.124	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.240%		
36) 1,2-Dichloropropane-d6	5.986	67	191721	51.210	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.420%		
41) Toluene-d8	7.243	98	494760	45.269	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.540%		
43) trans-1,3-Dichloroprop...	7.551	79	82713	45.331	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.660%		
47) 2-Hexanone-d5	8.024	63	165810	96.378	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.380%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	284999	49.958	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.920%		
66) 1,2-Dichlorobenzene-d4	11.558	152	197003	51.672	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.340%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.912	75	4364	0.878	ug/L #	61
61) 1,2,3-Trichloropropane	11.181	75	20155	5.235	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035527.D
Acq On : 03 May 2024 10:54
Operator : SY/MD
Sample : P2349-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 03 23:18:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 03 23:16:53 2024
Response via : Initial Calibration




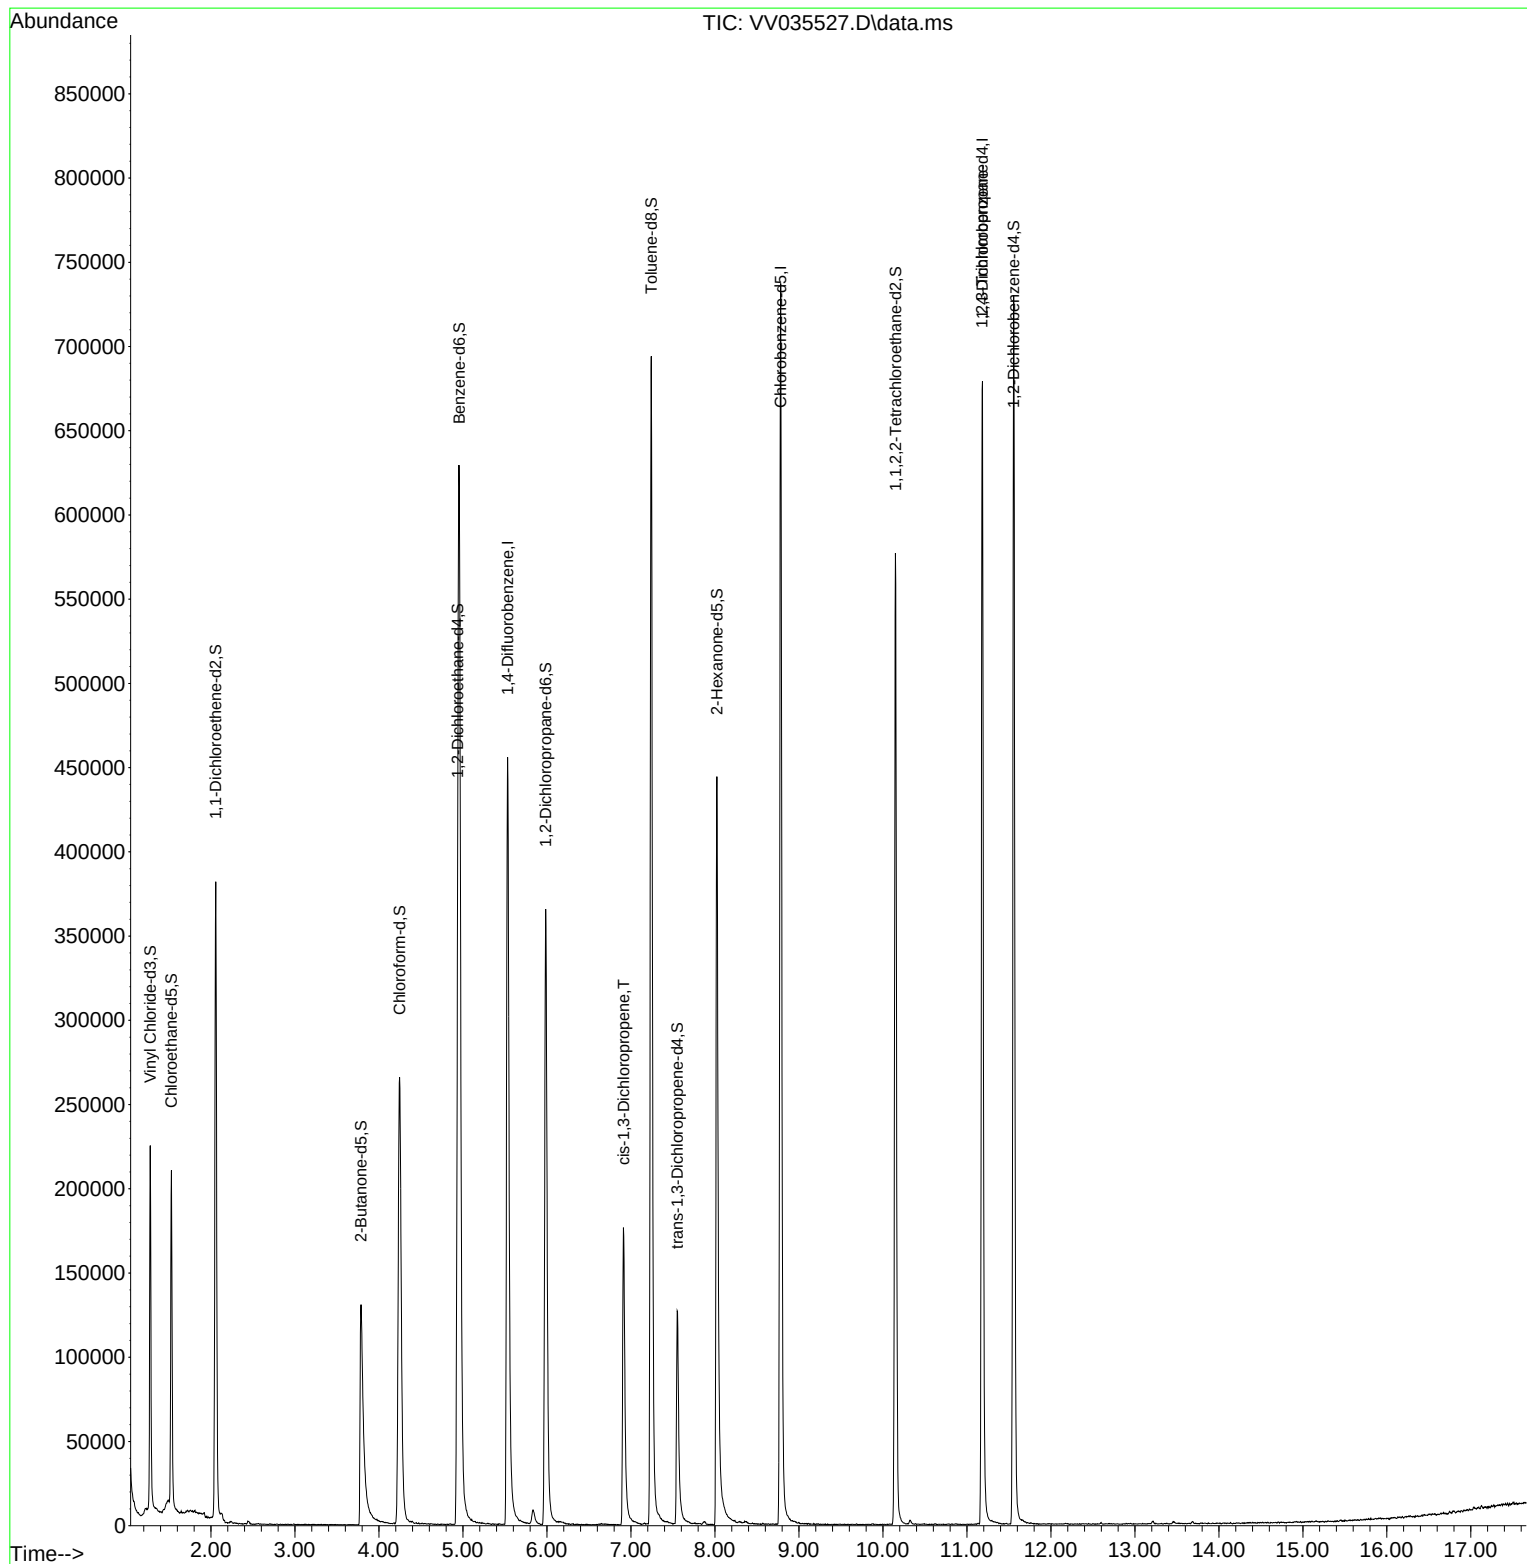


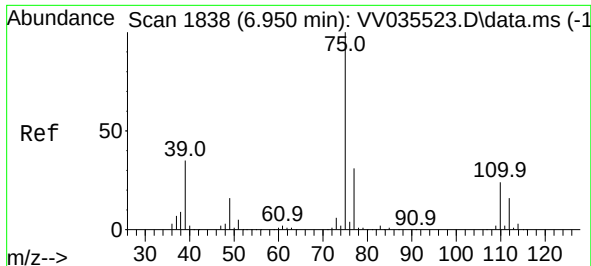

#39
cis-1,3-Dichloropropene
Concen: 0.878 ug/L
RT: 6.912 min Scan# 11
Delta R.T. -0.039 min
Lab File: VV035527.D
Acq: 03 May 2024 10:54

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 4364
Ion Ratio Lower Upper
75 100
77 53.6 22.3 41.3#

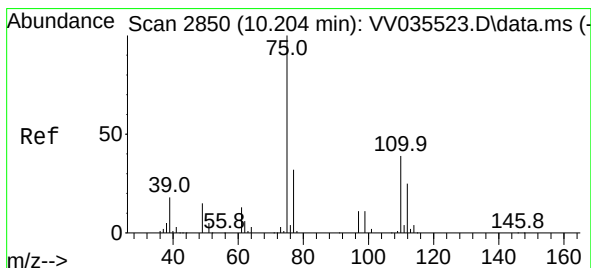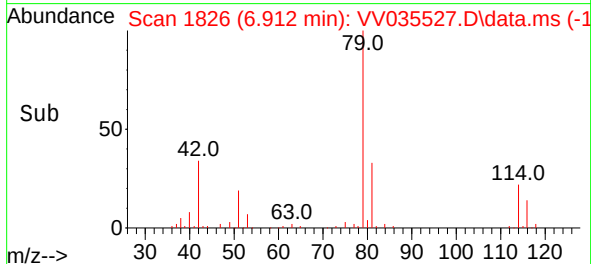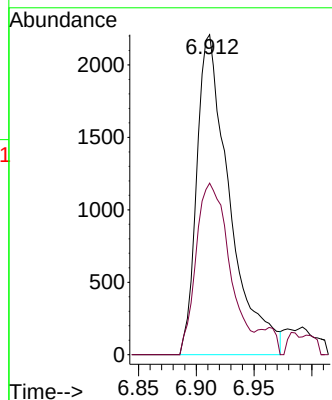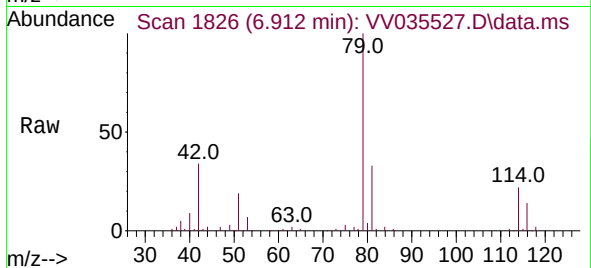

#61
1,2,3-Trichloropropane
Concen: 5.235 ug/L
RT: 11.181 min Scan# 3154
Delta R.T. 0.977 min
Lab File: VV035527.D
Acq: 03 May 2024 10:54

Tgt Ion: 75 Resp: 20155
Ion Ratio Lower Upper
75 100
77 33.9 25.8 38.6
110 2.5 31.6 47.4#

