

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035524.D
 Acq On : 03 May 2024 09:31
 Operator : SY/MD
 Sample : VV0503WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK282

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	242508	259214	14.76%	1.926%
2	1.532	145	153	171	rVB	216977	255445	14.54%	1.898%
3	2.056	306	316	333	rBV	411355	599582	34.14%	4.456%
4	2.233	367	371	373	rBV3	1090	890	0.05%	0.007%
5	2.346	401	406	409	rBV2	531	422	0.02%	0.003%
6	2.417	422	428	430	rBV2	409	435	0.02%	0.003%
7	2.449	430	438	446	rVB6	2194	3522	0.20%	0.026%
8	2.638	494	497	504	rVB2	318	380	0.02%	0.003%
9	2.690	510	513	515	rVV3	459	302	0.02%	0.002%
10	2.706	515	518	524	rVB5	703	788	0.04%	0.006%
11	2.757	525	534	538	rBV2	365	432	0.02%	0.003%
12	3.146	650	655	660	rVB2	324	265	0.02%	0.002%
13	3.175	660	664	666	rBV2	306	215	0.01%	0.002%
14	3.285	692	698	701	rVB2	260	237	0.01%	0.002%
15	3.436	740	745	750	rVB2	277	328	0.02%	0.002%
16	3.471	750	756	758	rBV2	409	305	0.02%	0.002%
17	3.796	848	857	918	rBV	121397	403656	22.98%	3.000%
18	4.246	979	997	1032	rBV	279225	724075	41.22%	5.381%
19	4.667	1126	1128	1132	rVB2	293	214	0.01%	0.002%
20	4.815	1172	1174	1180	rBV2	286	239	0.01%	0.002%
21	4.953	1201	1217	1251	rBV2	666809	1756441	100.00%	13.053%
22	5.195	1288	1292	1296	rVB4	747	716	0.04%	0.005%
23	5.236	1302	1305	1308	rBV3	320	247	0.01%	0.002%
24	5.352	1337	1341	1343	rBV2	466	308	0.02%	0.002%
25	5.387	1348	1352	1356	rBV3	315	264	0.02%	0.002%
26	5.532	1386	1397	1436	rBV	493945	1043798	59.43%	7.757%
27	5.834	1481	1491	1517	rVB2	9787	23974	1.36%	0.178%
28	5.944	1520	1525	1526	rBV3	338	228	0.01%	0.002%
29	5.986	1526	1538	1576	rBV	382358	800473	45.57%	5.949%
30	6.256	1619	1622	1626	rVB3	508	413	0.02%	0.003%
31	6.320	1636	1642	1644	rVV2	357	278	0.02%	0.002%
32	6.336	1644	1647	1653	rVB4	402	310	0.02%	0.002%
33	6.452	1679	1683	1686	rVB3	518	376	0.02%	0.003%
34	6.587	1721	1725	1729	rBV2	340	212	0.01%	0.002%
35	6.638	1737	1741	1745	rVV2	553	424	0.02%	0.003%
36	6.738	1770	1772	1774	rBV	393	228	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035524.D
 Acq On : 03 May 2024 09:31
 Operator : SY/MD
 Sample : VV0503WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK282

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.912	1816	1826	1858	rBV	187852	364230	20.74%	2.707%
38	7.243	1917	1929	1963	rBV	748510	1348383	76.77%	10.020%
39	7.551	2016	2025	2052	rBV	132727	252753	14.39%	1.878%
40	7.770	2091	2093	2096	rBV3	369	217	0.01%	0.002%
41	7.805	2101	2104	2109	rVB3	473	398	0.02%	0.003%
42	7.873	2116	2125	2130	rBV4	1007	1590	0.09%	0.012%
43	7.915	2135	2138	2143	rVB4	770	783	0.04%	0.006%
44	7.976	2155	2157	2162	rVB3	354	295	0.02%	0.002%
45	8.024	2163	2172	2210	rBV	463665	875375	49.84%	6.505%
46	8.317	2261	2263	2268	rVB3	981	740	0.04%	0.005%
47	8.510	2321	2323	2327	rVB2	561	253	0.01%	0.002%
48	8.542	2329	2333	2337	rBV4	377	368	0.02%	0.003%
49	8.696	2379	2381	2385	rVB3	420	272	0.02%	0.002%
50	8.725	2385	2390	2394	rBV2	409	452	0.03%	0.003%
51	8.783	2397	2408	2443	rBV	781267	1315227	74.88%	9.774%
52	9.130	2513	2516	2517	rBV2	451	239	0.01%	0.002%
53	9.172	2526	2529	2534	rBV2	414	331	0.02%	0.002%
54	9.233	2543	2548	2551	rBV3	464	323	0.02%	0.002%
55	9.333	2576	2579	2582	rBV2	305	232	0.01%	0.002%
56	9.493	2623	2629	2631	rBV2	484	400	0.02%	0.003%
57	9.551	2637	2647	2654	rBV5	573	1153	0.07%	0.009%
58	9.657	2676	2680	2685	rVB2	279	285	0.02%	0.002%
59	9.744	2700	2707	2710	rBV2	396	476	0.03%	0.004%
60	9.860	2739	2743	2745	rVV3	484	358	0.02%	0.003%
61	9.879	2747	2749	2754	rVB4	624	400	0.02%	0.003%
62	10.027	2791	2795	2796	rBV	1140	608	0.03%	0.005%
63	10.149	2821	2833	2868	rVV	594867	952805	54.25%	7.081%
64	10.313	2881	2884	2886	rBV2	564	361	0.02%	0.003%
65	10.374	2899	2903	2908	rBV3	386	422	0.02%	0.003%
66	10.471	2928	2933	2934	rBV2	283	221	0.01%	0.002%
67	10.487	2936	2938	2941	rVB3	476	221	0.01%	0.002%
68	10.542	2950	2955	2957	rBV	293	263	0.01%	0.002%
69	10.725	3009	3012	3016	rVB3	331	257	0.01%	0.002%
70	10.796	3025	3034	3039	rBV4	622	722	0.04%	0.005%
71	10.860	3048	3054	3055	rBV	572	506	0.03%	0.004%
72	10.950	3077	3082	3084	rBV3	306	243	0.01%	0.002%
73	11.030	3103	3107	3113	rVB2	277	319	0.02%	0.002%
74	11.130	3131	3138	3144	rBV4	2300	3460	0.20%	0.026%
75	11.185	3144	3155	3181	rVV	734530	1163417	66.24%	8.646%
76	11.558	3258	3271	3297	rBV	794099	1245109	70.89%	9.253%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035524.D
 Acq On : 03 May 2024 09:31
 Operator : SY/MD
 Sample : VV0503WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK282

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.773	3335	3338	3341	rVB4	333	233	0.01%	0.002%
78	12.014	3411	3413	3417	rVB2	341	226	0.01%	0.002%
79	12.040	3417	3421	3425	rBV2	433	469	0.03%	0.003%
80	12.069	3428	3430	3435	rVB2	480	340	0.02%	0.003%
81	12.133	3448	3450	3453	rVB2	396	241	0.01%	0.002%
82	12.239	3481	3483	3487	rVB2	351	232	0.01%	0.002%
83	12.323	3504	3509	3515	rBV2	428	433	0.02%	0.003%
84	12.378	3522	3526	3534	rBV4	696	947	0.05%	0.007%
85	12.500	3562	3564	3567	rBV2	384	220	0.01%	0.002%
86	12.593	3584	3593	3603	rBV5	2800	4636	0.26%	0.034%
87	12.927	3695	3697	3705	rVB2	476	456	0.03%	0.003%
88	12.982	3710	3714	3717	rVV2	375	344	0.02%	0.003%
89	13.001	3717	3720	3724	rVB	417	292	0.02%	0.002%
90	13.056	3731	3737	3740	rBV3	385	350	0.02%	0.003%
91	13.095	3747	3749	3752	rBV3	309	247	0.01%	0.002%
92	13.207	3777	3784	3796	rVB4	4410	6993	0.40%	0.052%
93	13.448	3851	3859	3871	rBV2	9008	15355	0.87%	0.114%
94	13.522	3880	3882	3887	rVB4	561	262	0.01%	0.002%
95	13.686	3925	3933	3944	rBV3	4877	8115	0.46%	0.060%
96	13.763	3955	3957	3961	rBV3	364	231	0.01%	0.002%
97	14.033	4039	4041	4047	rVB3	469	379	0.02%	0.003%
98	14.410	4156	4158	4161	rBV3	471	279	0.02%	0.002%
99	14.689	4243	4245	4249	rBV3	528	264	0.02%	0.002%
100	15.577	4518	4521	4523	rBV3	1143	841	0.05%	0.006%

Sum of corrected areas: 13456488




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035524.D
Acq On : 03 May 2024 09:31
Operator : SY/MD
Sample : VV0503WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK282

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

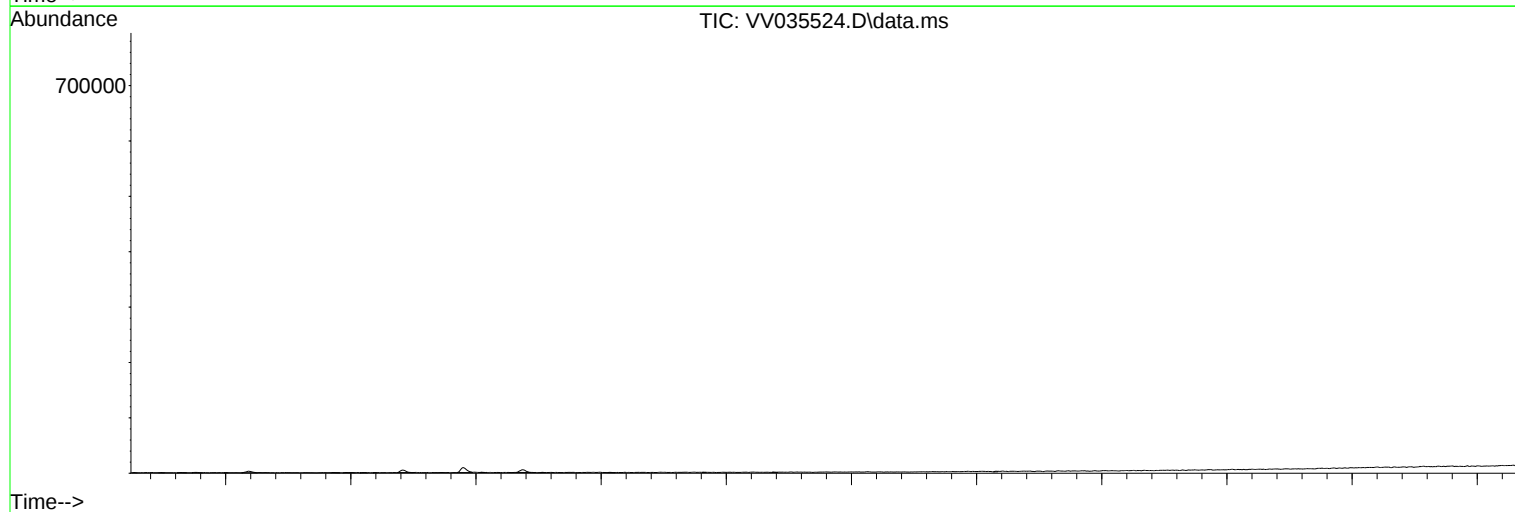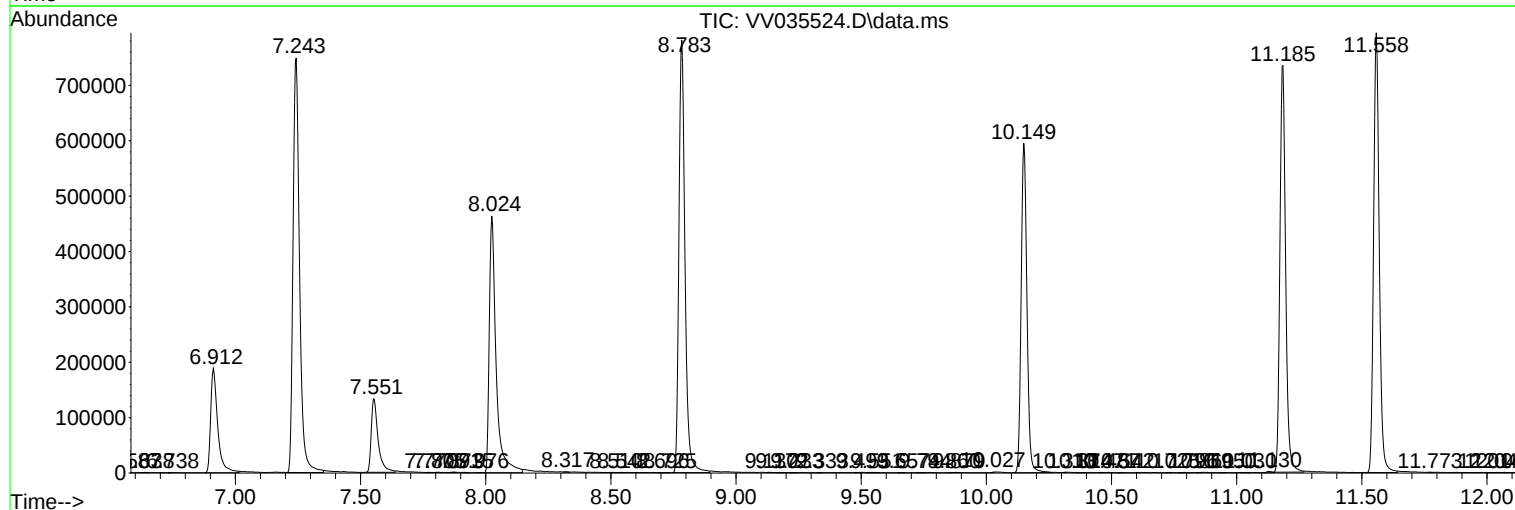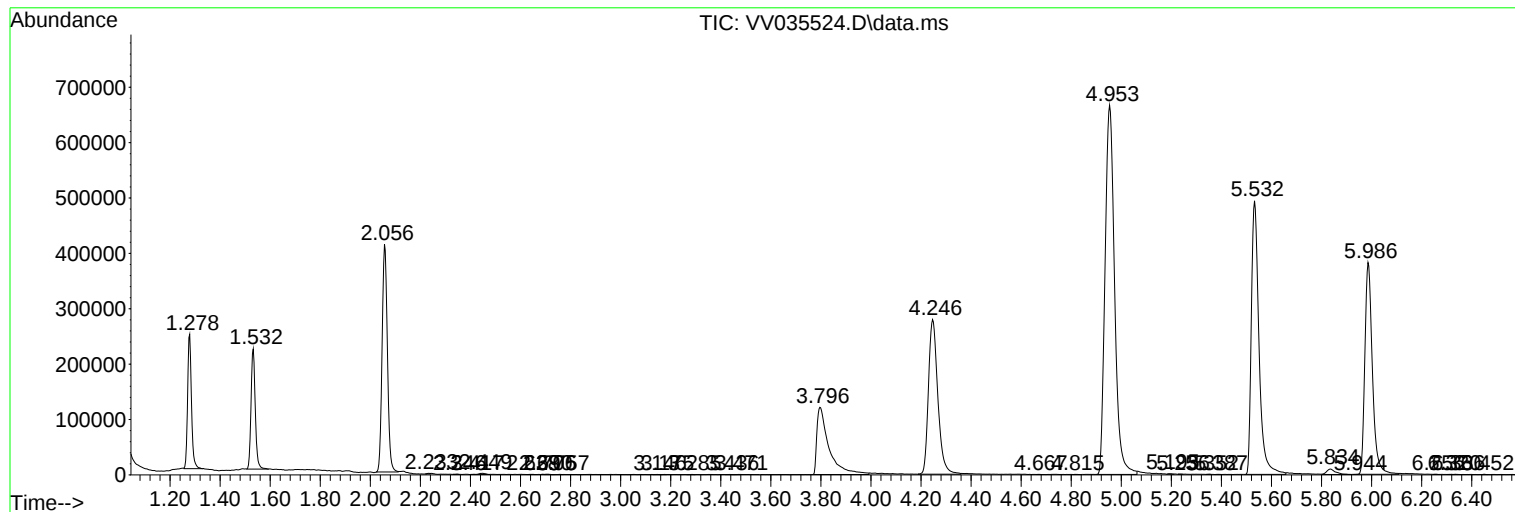

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035524.D
Acq On : 03 May 2024 09:31
Operator : SY/MD
Sample : VV0503WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK282

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035524.D
Acq On : 03 May 2024 09:31
Operator : SY/MD
Sample : VV0503WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK282

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------