

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035526.D
 Acq On : 03 May 2024 10:30
 Operator : SY/MD
 Sample : P2349-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08R6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	43	46	50	rBV2	4884	4460	0.26%	0.033%
2	1.278	67	74	92	rVB	235856	250301	14.38%	1.833%
3	1.532	145	153	166	rVB	212334	244520	14.05%	1.791%
4	2.056	306	316	331	rBV	404379	584889	33.61%	4.283%
5	2.445	432	437	447	rVB7	1262	2373	0.14%	0.017%
6	2.567	472	475	478	rVB	553	283	0.02%	0.002%
7	2.590	478	482	483	rBV3	529	341	0.02%	0.002%
8	2.699	511	516	517	rBV2	659	609	0.03%	0.004%
9	2.809	546	550	551	rBV	368	218	0.01%	0.002%
10	2.879	568	572	574	rBV3	512	435	0.02%	0.003%
11	2.966	593	599	600	rVV2	247	238	0.01%	0.002%
12	3.330	706	712	715	rBV2	226	217	0.01%	0.002%
13	3.384	726	729	733	rVB2	305	222	0.01%	0.002%
14	3.510	765	768	774	rVB2	290	244	0.01%	0.002%
15	3.632	803	806	809	rBV	390	282	0.02%	0.002%
16	3.696	822	826	833	rVB2	272	280	0.02%	0.002%
17	3.738	833	839	843	rBV2	299	308	0.02%	0.002%
18	3.793	847	856	886	rBV	126472	374448	21.52%	2.742%
19	4.246	981	997	1037	rBV2	292796	840015	48.27%	6.152%
20	4.587	1101	1103	1107	rVB2	369	228	0.01%	0.002%
21	4.648	1119	1122	1129	rVB2	555	580	0.03%	0.004%
22	4.783	1162	1164	1171	rVB2	404	416	0.02%	0.003%
23	4.818	1171	1175	1180	rBV2	233	250	0.01%	0.002%
24	4.953	1199	1217	1245	rBV2	663800	1740115	100.00%	12.744%
25	5.201	1291	1294	1297	rBV3	643	504	0.03%	0.004%
26	5.532	1386	1397	1436	rBV	517373	1084515	62.32%	7.943%
27	5.828	1478	1489	1518	rVB2	22007	52111	2.99%	0.382%
28	5.931	1518	1521	1524	rVB2	594	323	0.02%	0.002%
29	5.985	1525	1538	1578	rBV	382816	802930	46.14%	5.880%
30	6.207	1604	1607	1611	rBV3	498	309	0.02%	0.002%
31	6.265	1621	1625	1631	rBV3	543	524	0.03%	0.004%
32	6.317	1637	1641	1643	rVB2	421	267	0.02%	0.002%
33	6.333	1643	1646	1648	rBV2	373	263	0.02%	0.002%
34	6.442	1669	1680	1695	rBV2	10842	22215	1.28%	0.163%
35	6.612	1730	1733	1737	rVV2	329	308	0.02%	0.002%
36	6.683	1751	1755	1757	rBV2	380	271	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035526.D
 Acq On : 03 May 2024 10:30
 Operator : SY/MD
 Sample : P2349-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08R6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.837	1797	1803	1805	rBV2	262	238	0.01%	0.002%
38	6.911	1816	1826	1856	rBV	187439	366184	21.04%	2.682%
39	7.146	1894	1899	1900	rBV2	587	473	0.03%	0.003%
40	7.185	1909	1911	1915	rVB4	564	253	0.01%	0.002%
41	7.243	1917	1929	1951	rBV	755559	1338280	76.91%	9.801%
42	7.551	2016	2025	2053	rBV	131989	254697	14.64%	1.865%
43	7.799	2100	2102	2106	rVB2	488	286	0.02%	0.002%
44	7.818	2106	2108	2110	rBV	469	234	0.01%	0.002%
45	7.831	2110	2112	2114	rVV2	474	306	0.02%	0.002%
46	7.844	2114	2116	2117	rVV	614	278	0.02%	0.002%
47	7.873	2117	2125	2135	rVV4	4154	7964	0.46%	0.058%
48	7.918	2135	2139	2142	rVB3	857	694	0.04%	0.005%
49	7.956	2148	2151	2153	rBV2	312	208	0.01%	0.002%
50	8.024	2163	2172	2214	rBV	456208	874598	50.26%	6.405%
51	8.461	2306	2308	2311	rBV2	473	255	0.01%	0.002%
52	8.500	2318	2320	2325	rVB4	561	469	0.03%	0.003%
53	8.783	2394	2408	2439	rBV	827567	1364100	78.39%	9.990%
54	9.066	2494	2496	2501	rVB3	347	225	0.01%	0.002%
55	9.095	2502	2505	2510	rBV3	679	737	0.04%	0.005%
56	9.152	2520	2523	2527	rVB4	359	274	0.02%	0.002%
57	9.168	2527	2528	2533	rVB2	331	211	0.01%	0.002%
58	9.268	2557	2559	2563	rVB3	377	237	0.01%	0.002%
59	9.355	2583	2586	2590	rBV2	378	265	0.02%	0.002%
60	9.490	2626	2628	2636	rVB4	420	509	0.03%	0.004%
61	9.696	2688	2692	2694	rBV2	321	242	0.01%	0.002%
62	9.812	2722	2728	2732	rBV3	285	323	0.02%	0.002%
63	9.841	2732	2737	2740	rVB2	346	247	0.01%	0.002%
64	9.988	2779	2783	2787	rVB2	330	227	0.01%	0.002%
65	10.030	2794	2796	2804	rVB2	337	326	0.02%	0.002%
66	10.149	2821	2833	2861	rBV	577615	906872	52.12%	6.642%
67	10.326	2879	2888	2901	rVB2	8315	14256	0.82%	0.104%
68	10.445	2920	2925	2928	rBV2	227	243	0.01%	0.002%
69	10.484	2933	2937	2944	rBV3	792	840	0.05%	0.006%
70	10.593	2966	2971	2973	rBV	266	237	0.01%	0.002%
71	10.625	2977	2981	2986	rBV2	337	323	0.02%	0.002%
72	10.818	3037	3041	3042	rBV2	301	202	0.01%	0.001%
73	11.030	3104	3107	3109	rBV2	407	229	0.01%	0.002%
74	11.069	3115	3119	3120	rBV2	317	202	0.01%	0.001%
75	11.104	3127	3130	3133	rBV	381	250	0.01%	0.002%
76	11.123	3133	3136	3143	rBV6	1011	1464	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035526.D
 Acq On : 03 May 2024 10:30
 Operator : SY/MD
 Sample : P2349-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08R6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.181	3143	3154	3183	rBV	772822	1223111	70.29%	8.958%
78	11.429	3229	3231	3236	rVB4	651	429	0.02%	0.003%
79	11.509	3254	3256	3259	rBV3	505	370	0.02%	0.003%
80	11.557	3259	3271	3296	rBV	799293	1263249	72.60%	9.252%
81	11.889	3372	3374	3379	rVB3	408	343	0.02%	0.003%
82	12.197	3463	3470	3477	rVB5	1708	2260	0.13%	0.017%
83	12.233	3477	3481	3482	rBV	326	225	0.01%	0.002%
84	12.320	3505	3508	3511	rBV2	422	375	0.02%	0.003%
85	12.419	3536	3539	3543	rVB3	510	347	0.02%	0.003%
86	12.490	3557	3561	3564	rBV	384	315	0.02%	0.002%
87	12.535	3573	3575	3578	rBV2	259	205	0.01%	0.002%
88	12.593	3587	3593	3603	rVV7	1330	1747	0.10%	0.013%
89	12.631	3603	3605	3610	rVB2	405	294	0.02%	0.002%
90	12.731	3633	3636	3640	rBV3	340	263	0.02%	0.002%
91	12.795	3651	3656	3658	rBV3	449	394	0.02%	0.003%
92	13.207	3777	3784	3795	rBV6	1831	3020	0.17%	0.022%
93	13.294	3805	3811	3815	rBV2	559	734	0.04%	0.005%
94	13.403	3842	3845	3846	rBV	451	247	0.01%	0.002%
95	13.451	3852	3860	3873	rBV2	2658	4266	0.25%	0.031%
96	13.541	3885	3888	3891	rBV2	478	353	0.02%	0.003%
97	13.580	3897	3900	3904	rBV2	322	325	0.02%	0.002%
98	13.692	3929	3935	3940	rVV4	1570	1618	0.09%	0.012%
99	13.799	3966	3968	3973	rBV	370	304	0.02%	0.002%
100	14.499	4183	4186	4189	rBV2	554	428	0.02%	0.003%

Sum of corrected areas: 13654492




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035526.D
Acq On : 03 May 2024 10:30
Operator : SY/MD
Sample : P2349-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08R6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

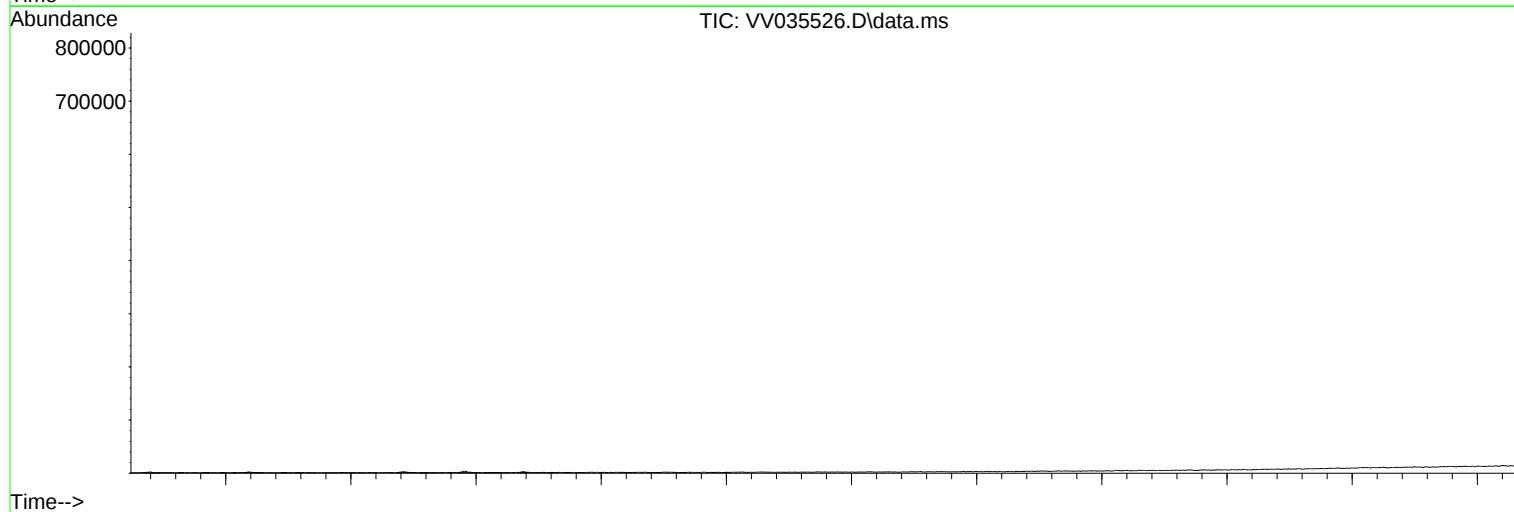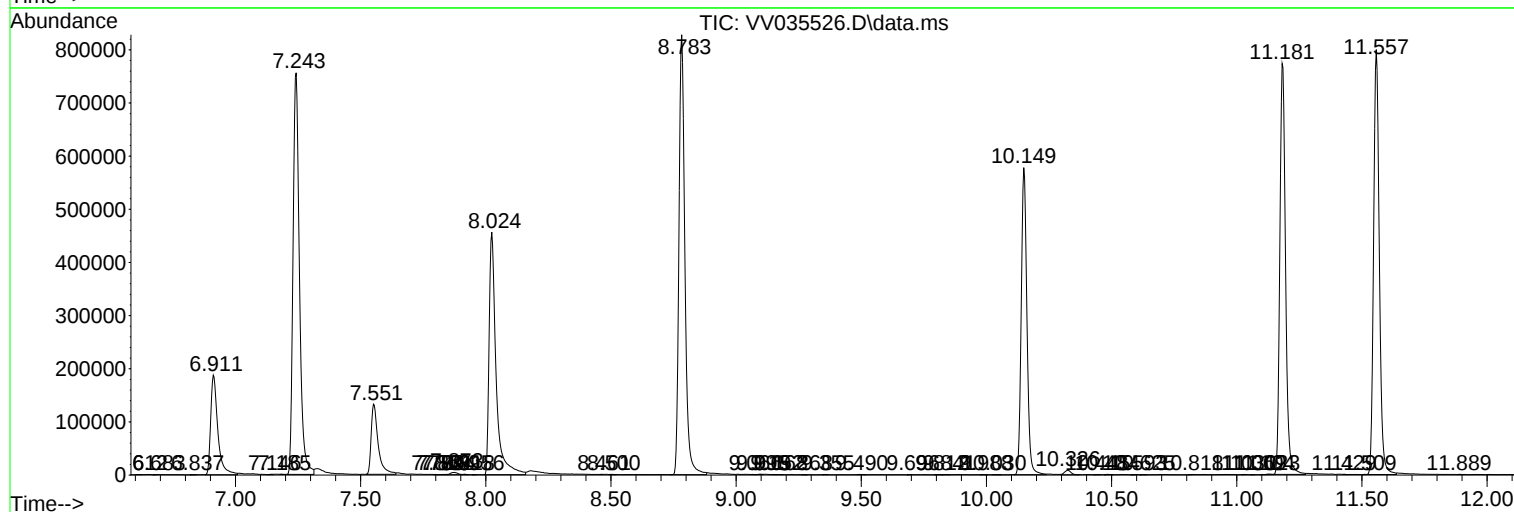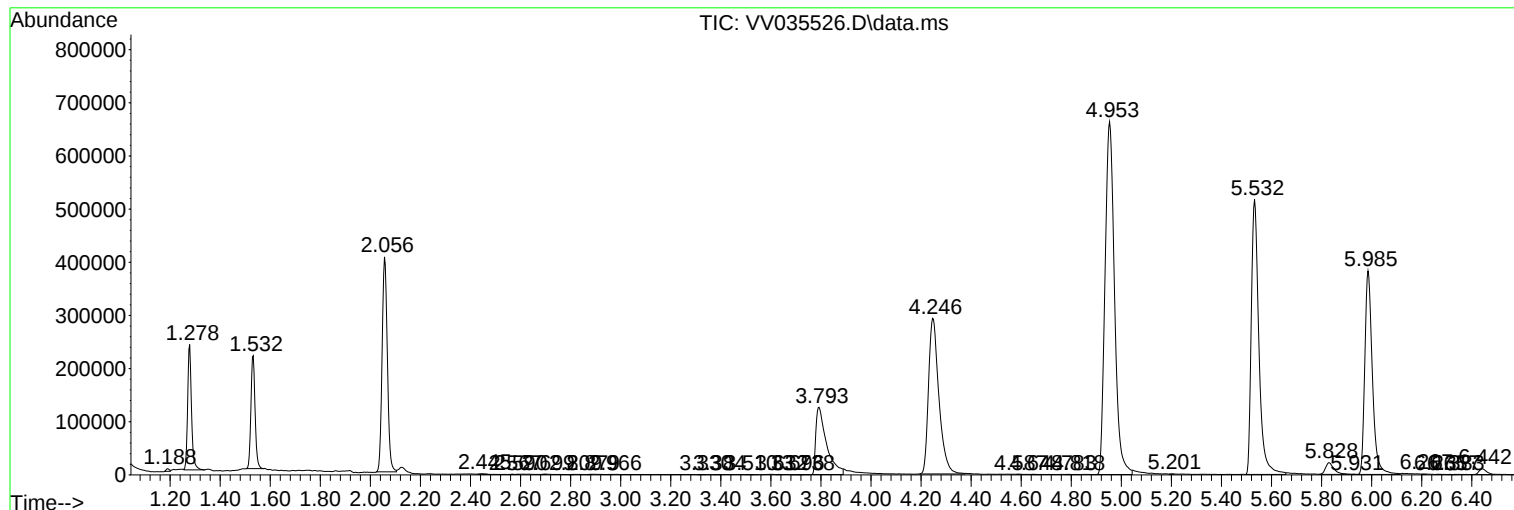

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035526.D
Acq On : 03 May 2024 10:30
Operator : SY/MD
Sample : P2349-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08R6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035526.D
Acq On : 03 May 2024 10:30
Operator : SY/MD
Sample : P2349-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08R6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------